


Data Path : Z:\HPCHEM1\BNA E\Data\BE072117\
 Data File : BE093504.D
 Acq On : 21 Jul 2017 11:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 21 16:13:20 2017

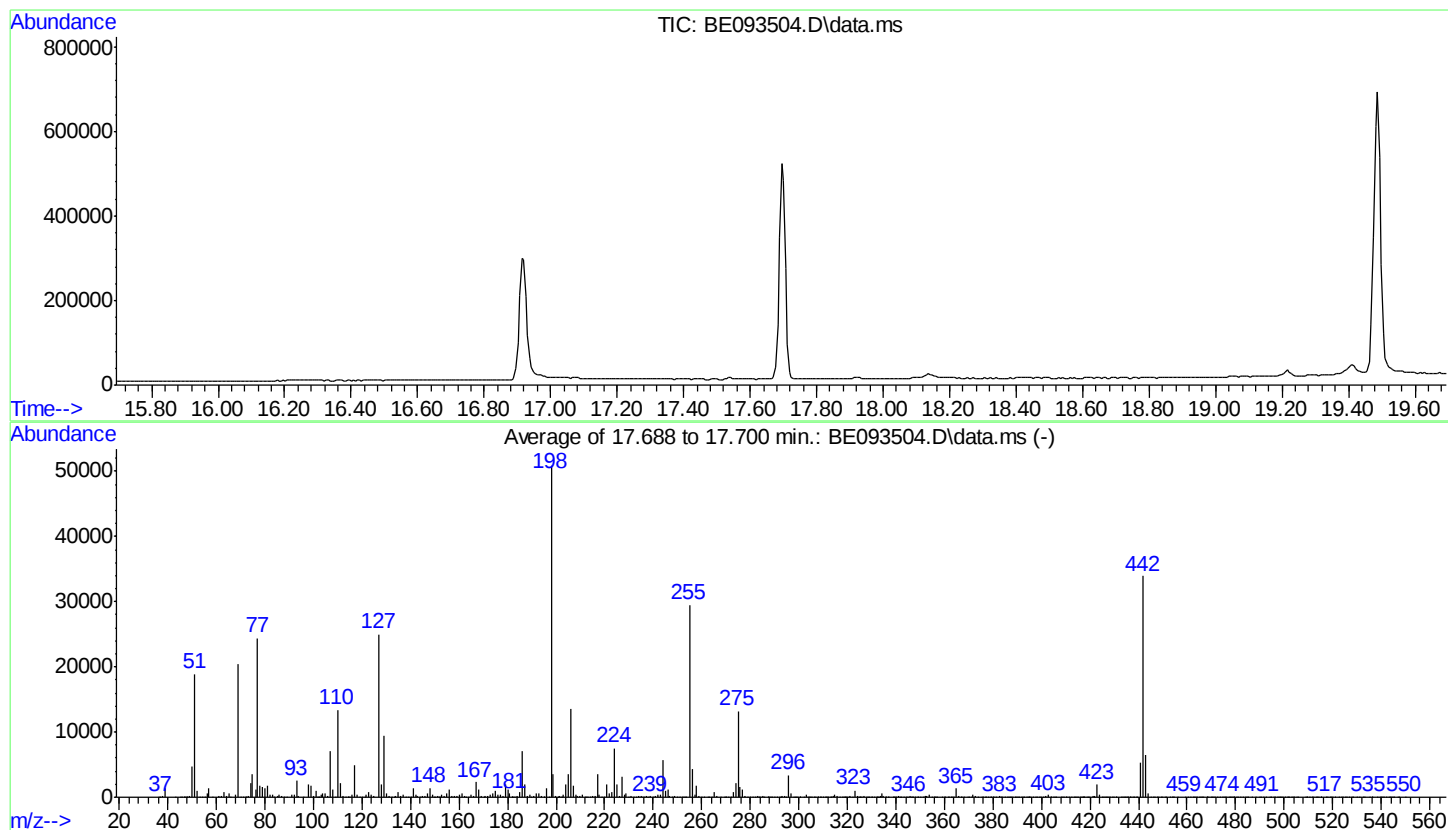

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	18923	PASS
68	69	0.00	2	1.6	327	PASS
69	198	0.00	100	40.2	20476	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	49.1	24976	PASS
197	198	0.00	2	0.1	75	PASS
198	198	100	100	100.0	50885	PASS
199	198	5	9	7.1	3615	PASS
275	198	10	60	26.0	13208	PASS
365	198	1	100	2.6	1312	PASS
441	442	0.01	24	15.7	5323	PASS
442	198	50	100	66.6	33898	PASS
443	442	15	24	18.9	6412	PASS