
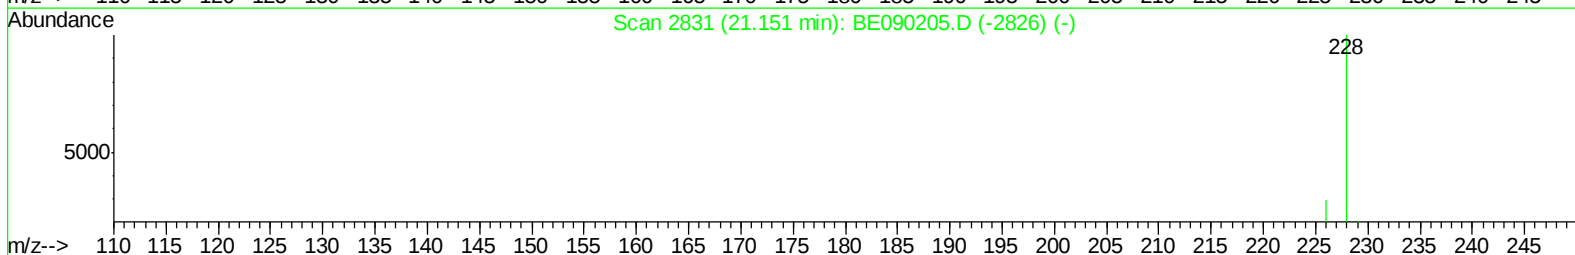
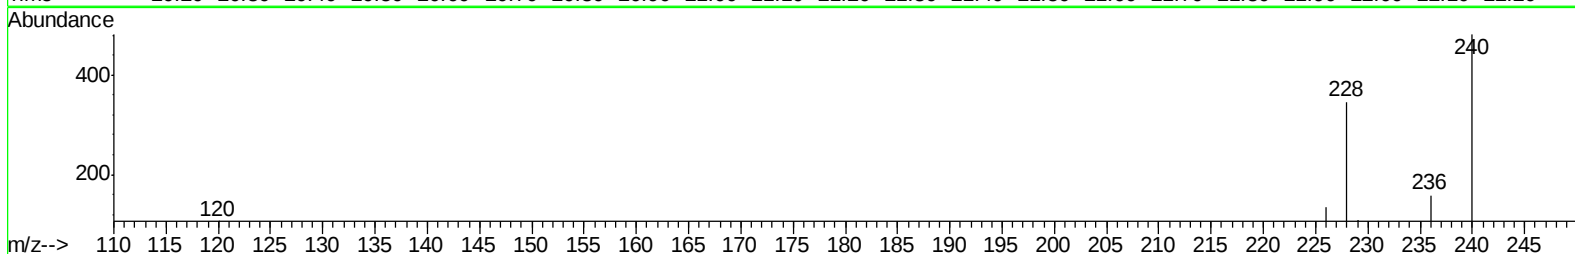


Data Path : Z:\HPCHEM1\BNA E\DATA\BE072215\
Data File : BE090210.D
Acq On : 21 Jul 2015 21:39
Operator : TP/IZ
Sample : MDL-01-S
Misc : MDL-SIM-SOIL-0.07PPM
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Jul 22 04:57:39 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE072215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 22 04:13:39 2015
Response via : Initial Calibration

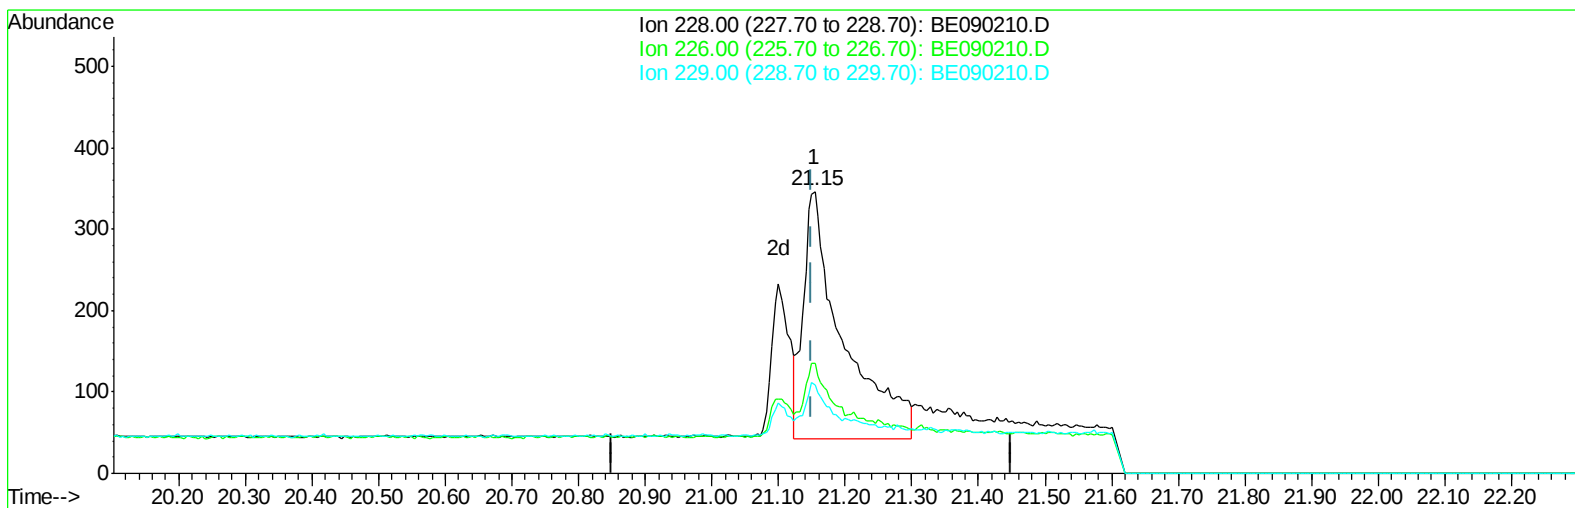

TIC: BE090210.D

(19) Chrysene

21.155min (+0.004) 0.07ng/ul m

response 1268

Ion	Exp%	Act%
228.00	100	100
226.00	30.70	39.02#
229.00	21.80	31.21#
0.00	0.00	0.00