
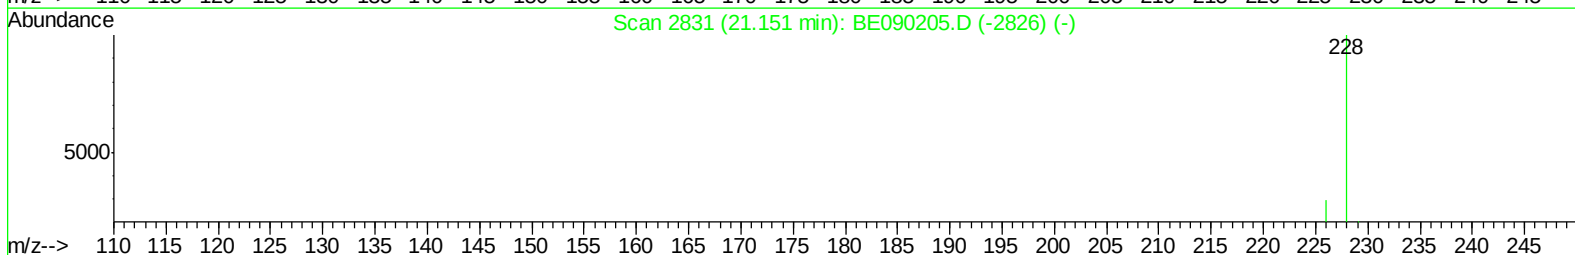
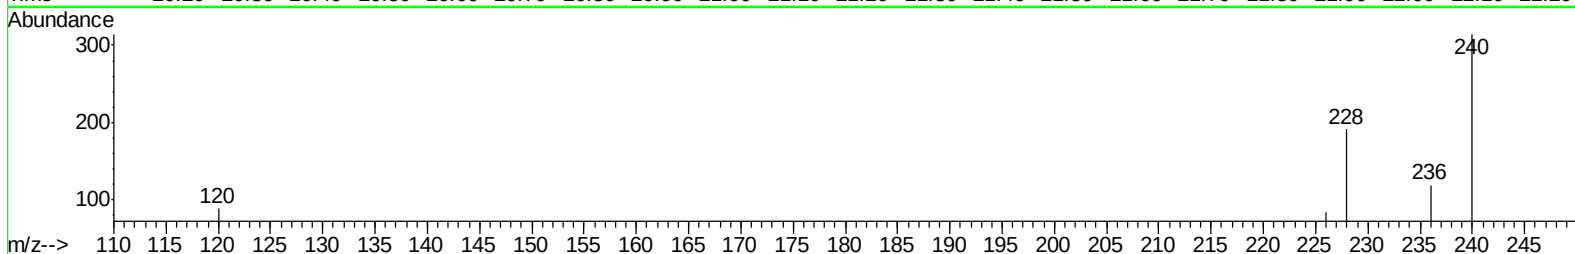


Data Path : Z:\HPCHEM1\BNA E\DATA\BE072215\  
Data File : BE090215.D  
Acq On : 22 Jul 2015 00:44  
Operator : TP/IZ  
Sample : MDL-06-S  
Misc : MDL-SIM-SOIL-0.07PPM  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jul 22 04:58:24 2015  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE072215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 22 04:13:39 2015  
Response via : Initial Calibration

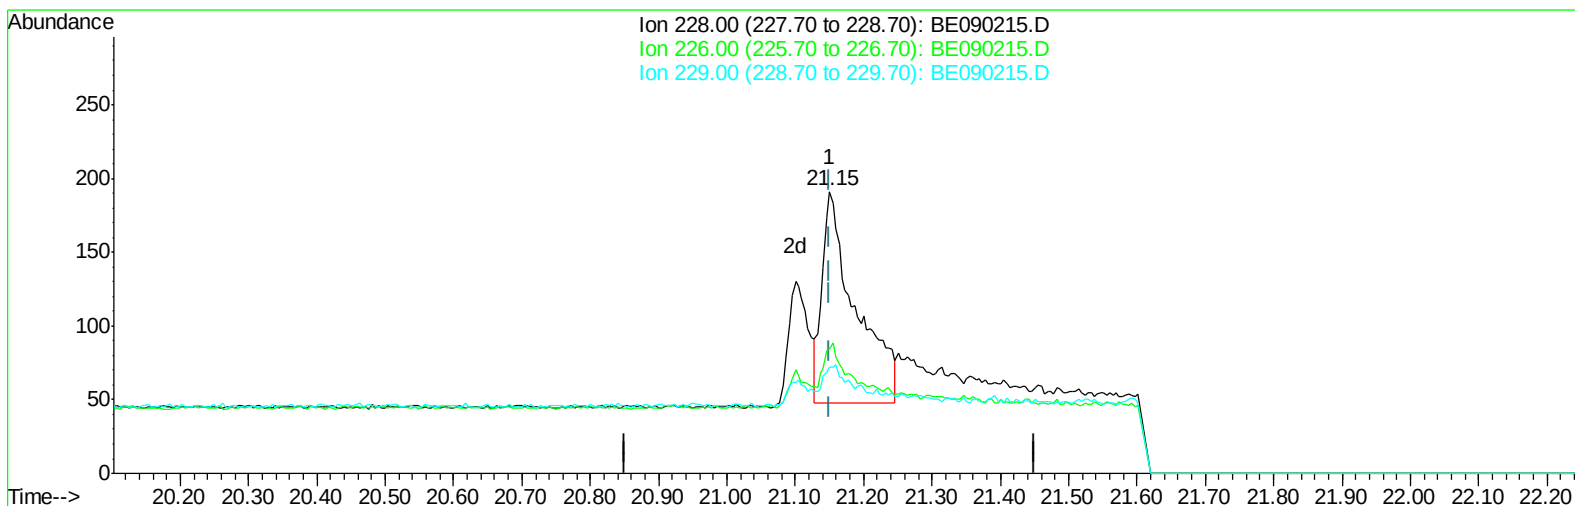

TIC: BE090215.D

(19) Chrysene

21.150min (-0.000) 0.05ng/ul m

response 487

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 226.00 | 30.70 | 43.98# |
| 229.00 | 21.80 | 37.70# |
| 0.00   | 0.00  | 0.00   |