
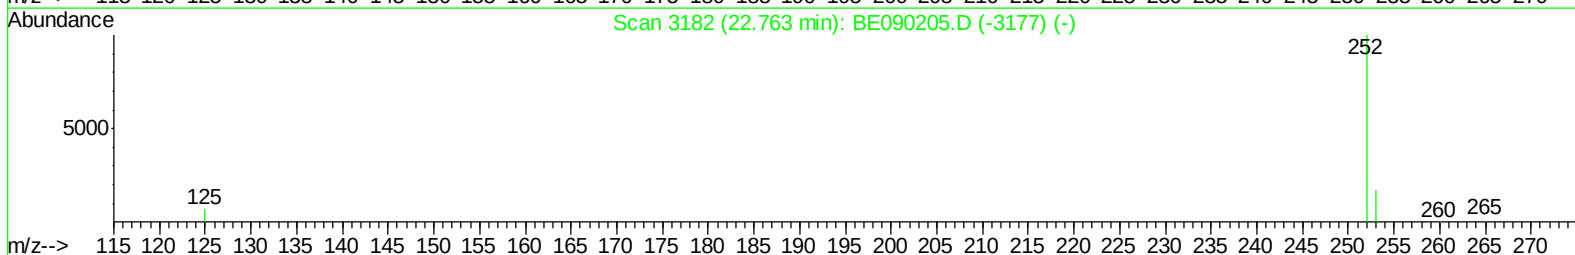
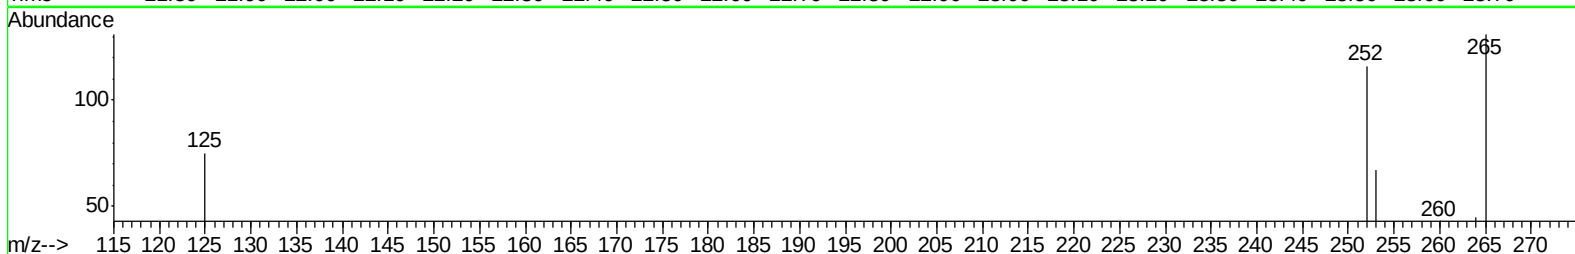


Data Path : Z:\HPCHEM1\BNA E\DATA\BE072215\  
Data File : BE090215.D  
Acq On : 22 Jul 2015 00:44  
Operator : TP/IZ  
Sample : MDL-06-S  
Misc : MDL-SIM-SOIL-0.07PPM  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jul 22 04:58:24 2015  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE072215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 22 04:13:39 2015  
Response via : Initial Calibration

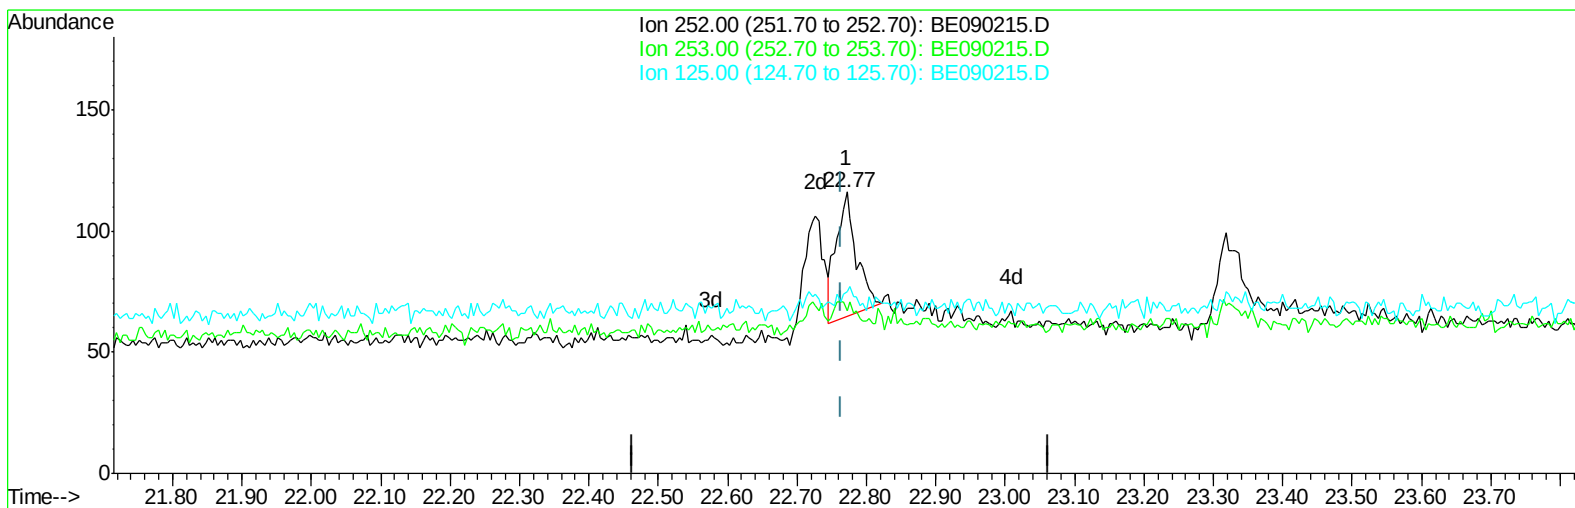

TIC: BE090215.D

(22) Benzo(k)fluoranthene

22.772min (+0.009) 0.02ng/ul

response 104

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 24.40 | 57.76# |
| 125.00 | 14.90 | 64.66# |
| 0.00   | 0.00  | 0.00   |