
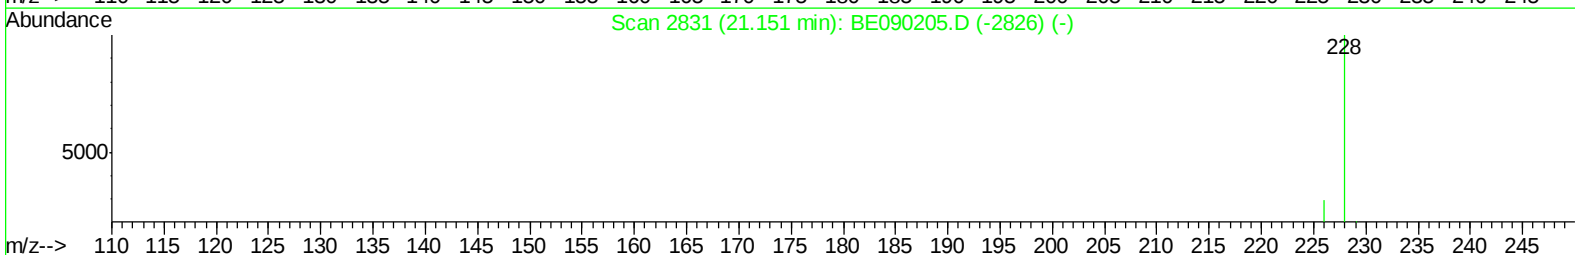
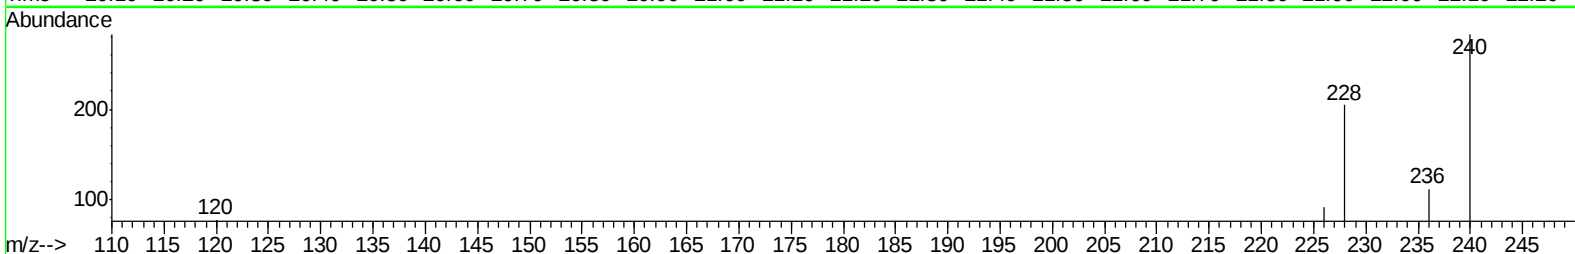


Data Path : Z:\HPCHEM1\BNA E\DATA\BE072215\
 Data File : BE090216.D
 Acq On : 22 Jul 2015 1:23
 Operator : TP/IZ
 Sample : MDL-07-S
 Misc : MDL-SIM-SOIL-0.07PPM
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jul 22 04:58:33 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE072215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 22 04:13:39 2015
 Response via : Initial Calibration

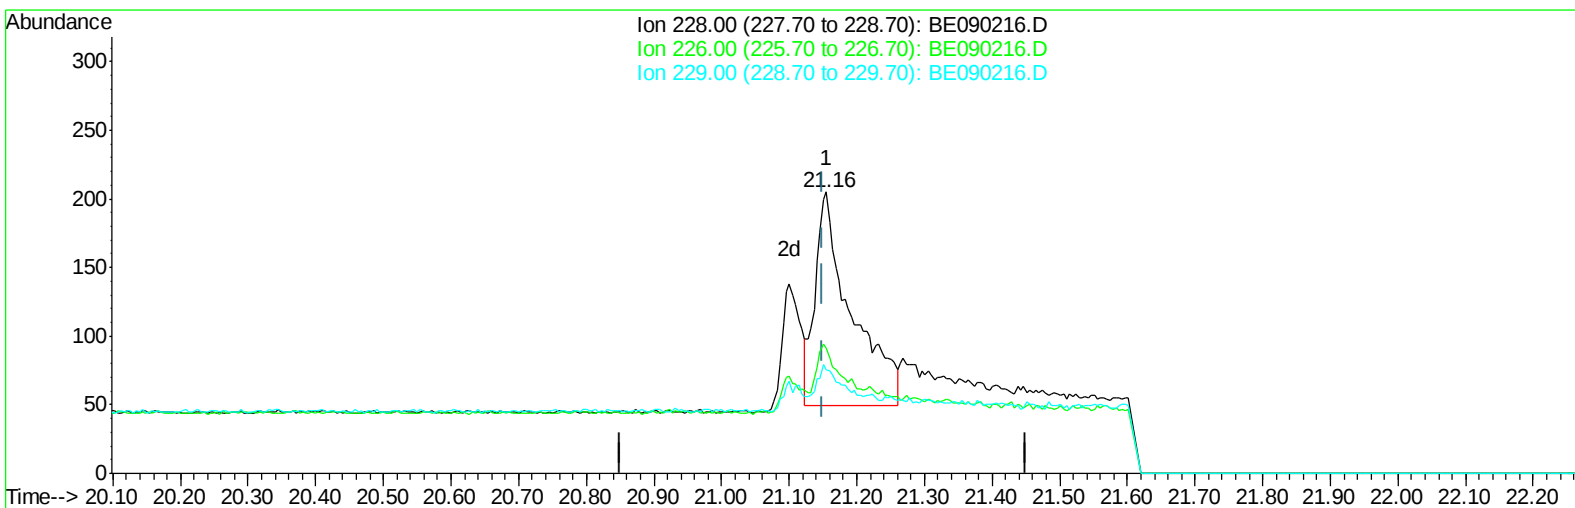

TIC: BE090216.D

(19) Chrysene

21.155min (+0.004) 0.06ng/ul m

response 577

Ion	Exp%	Act%
228.00	100	100
226.00	30.70	44.39#
229.00	21.80	37.07#
0.00	0.00	0.00