


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072215\
Data File : BE090202.D
Acq On : 21 Jul 2015 16:20
Operator : TP/IZ
Sample : DFTPP04
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP04

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 22 05:40:44 2015

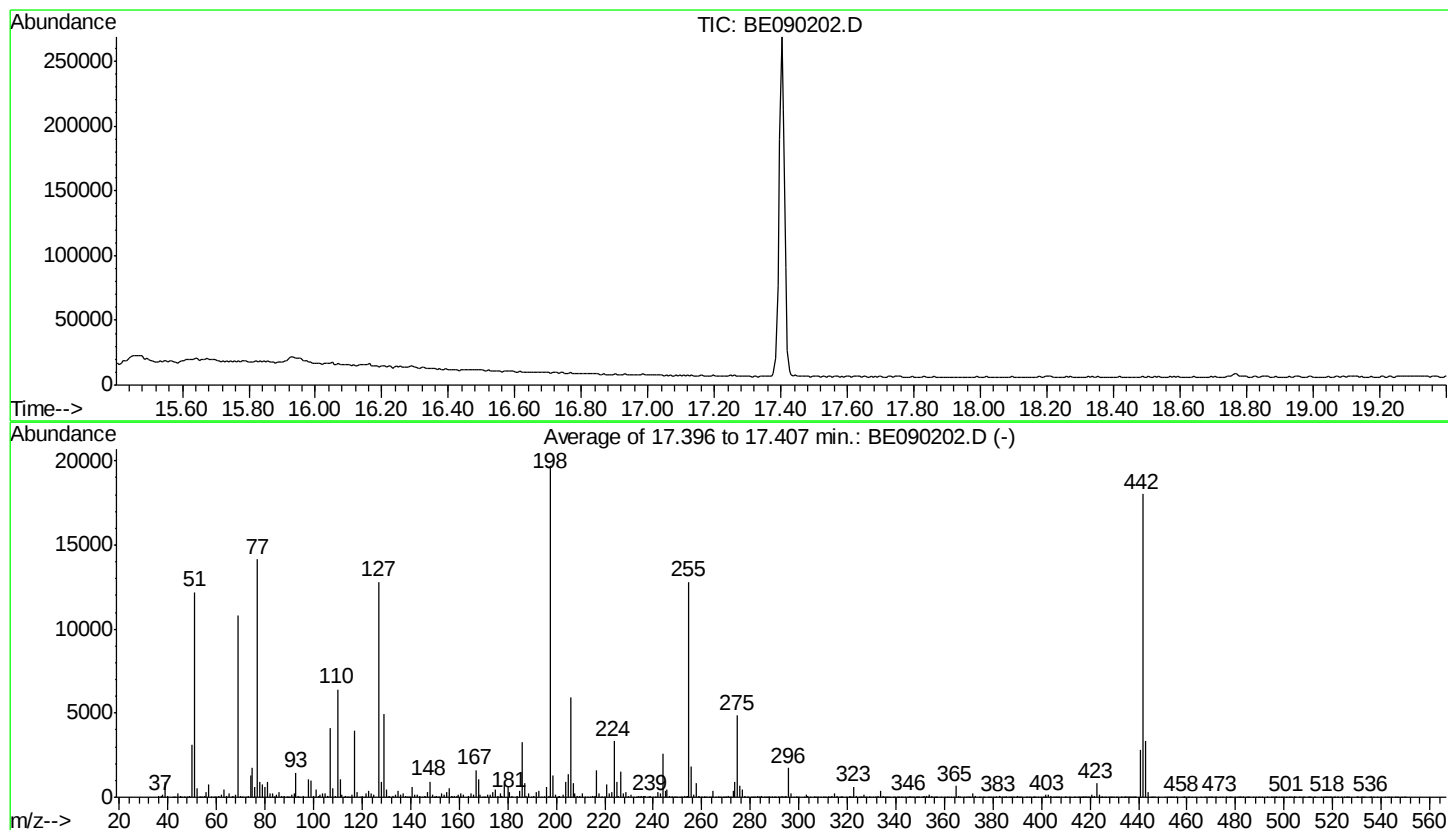

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.9	12210	PASS
68	69	0.00	2	1.7	181	PASS
69	198	0.00	100	54.8	10814	PASS
70	69	0.00	2	1.0	111	PASS
127	198	10	80	65.0	12821	PASS
197	198	0.00	2	0.3	65	PASS
198	198	100	100	100.0	19722	PASS
199	198	5	9	6.6	1295	PASS
275	198	10	60	24.6	4859	PASS
365	198	1	100	3.4	680	PASS
441	443	0.01	100	83.9	2809	PASS
442	198	50	100	91.4	18030	PASS
443	442	15	24	18.6	3347	PASS