
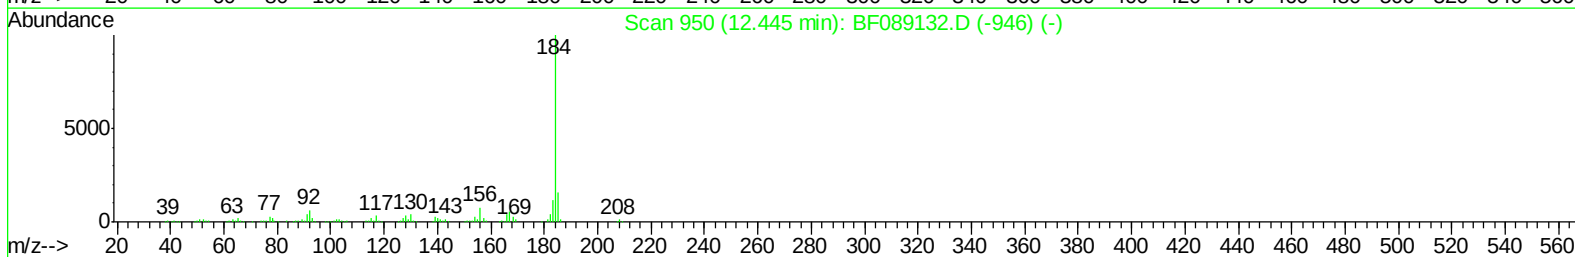
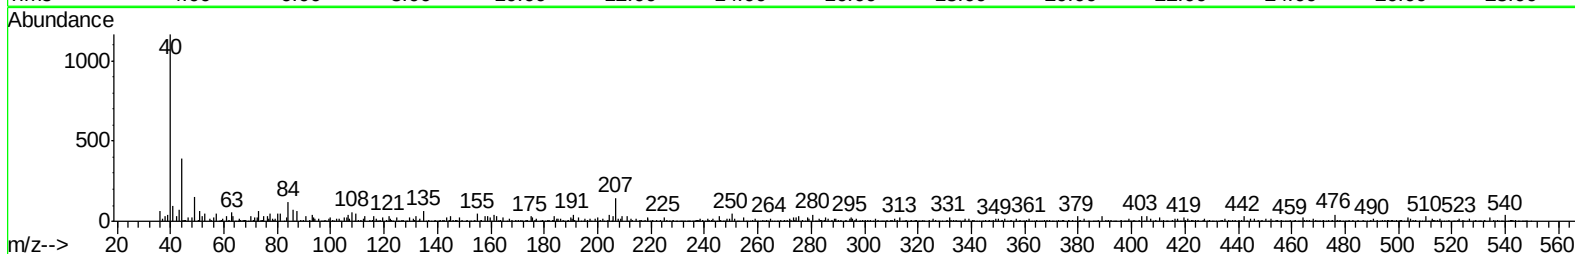


Data Path : Z:\HPCHEM1\BNA_E\Data\Be072216\
Data File : BE092008.D
Acq On : 22 Jul 2016 16:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 07:14:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

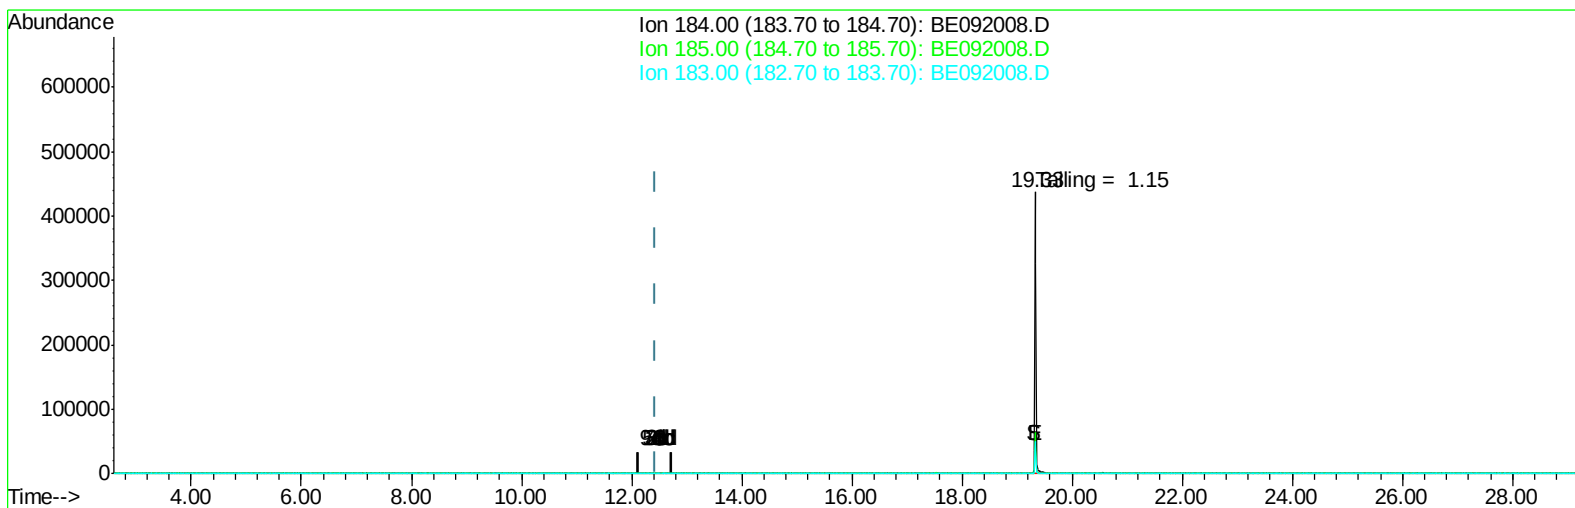

TIC: BE092008.D

(76) Benzidine




12.518min (+0.073) 78.31ng

response 35

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	27.45#
183.00	12.00	29.41#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\Be072216\
Data File : BE092008.D
Acq On : 22 Jul 2016 16:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 07:14:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

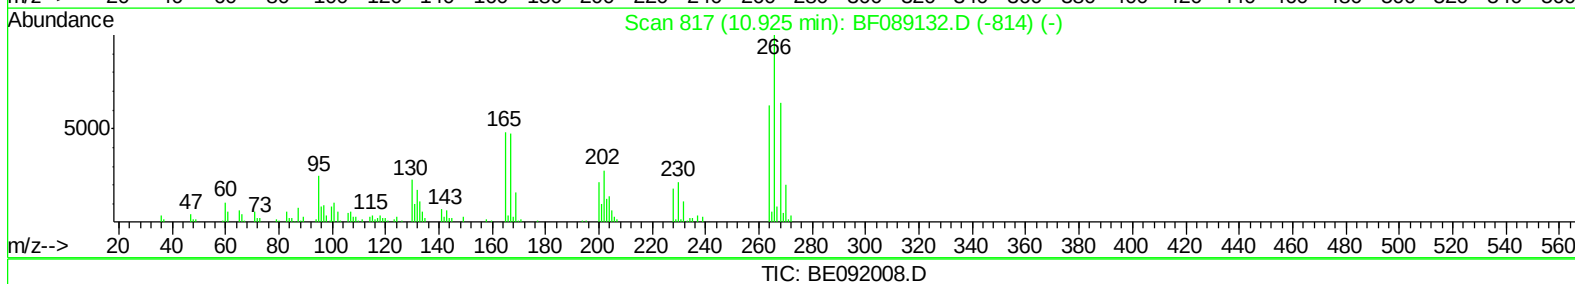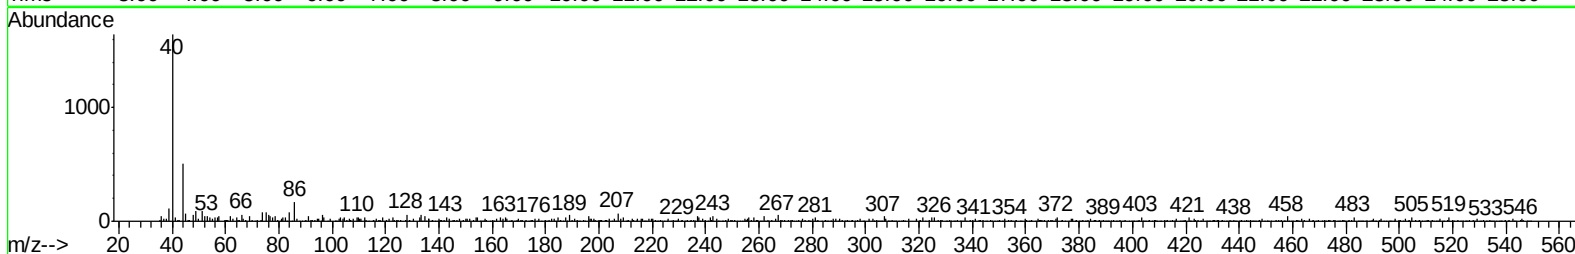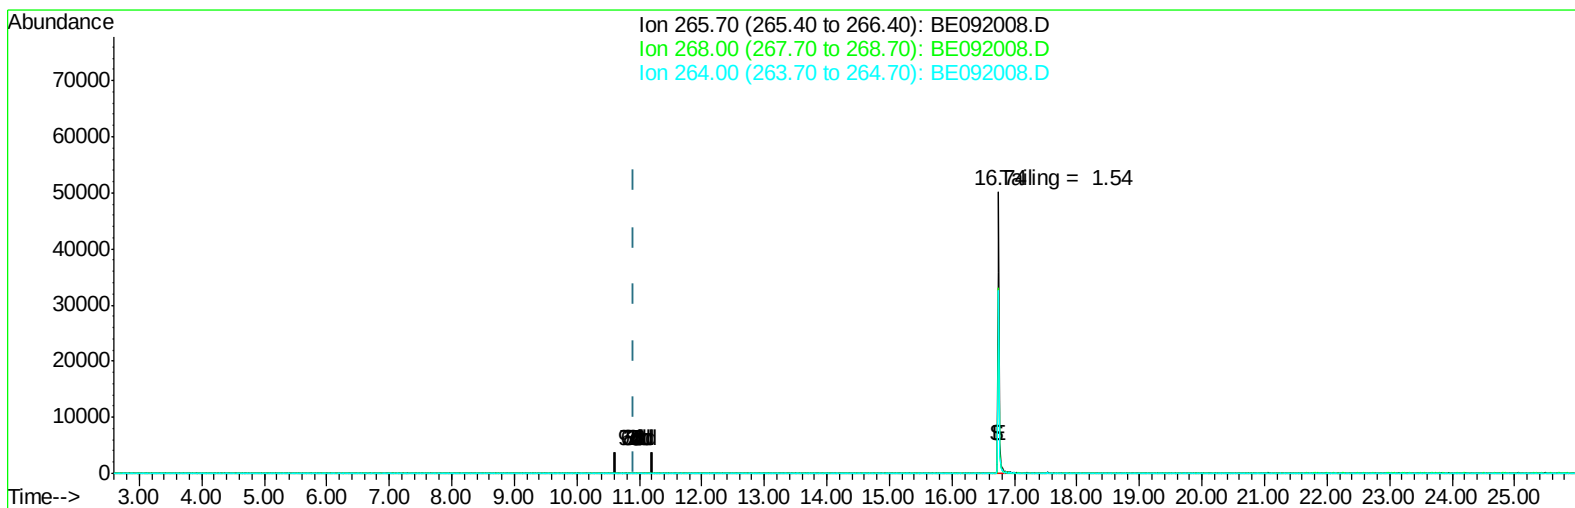

TIC: BE092008.D

(69) Pentachlorophenol (C)

10.984min (+0.060) 49.37ng

response 8

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	70.00
264.00	62.10	15.00#
0.00	0.00	0.00