
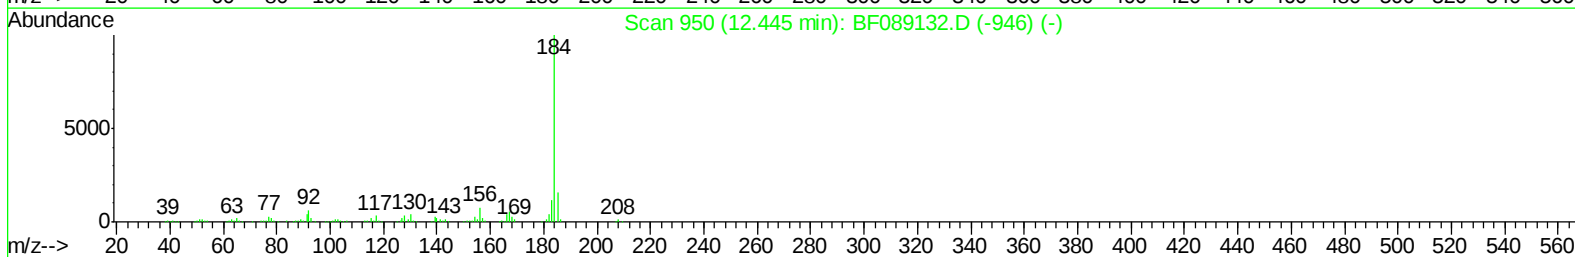
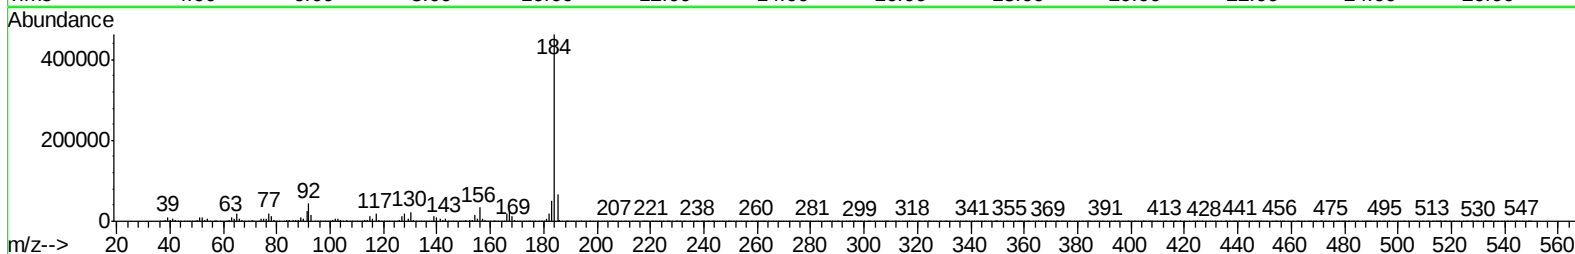


Data Path : Z:\HPCHEM1\BNA_E\Data\Be072216\
Data File : BE092024.D
Acq On : 23 Jul 2016 2:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 07:15:48 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

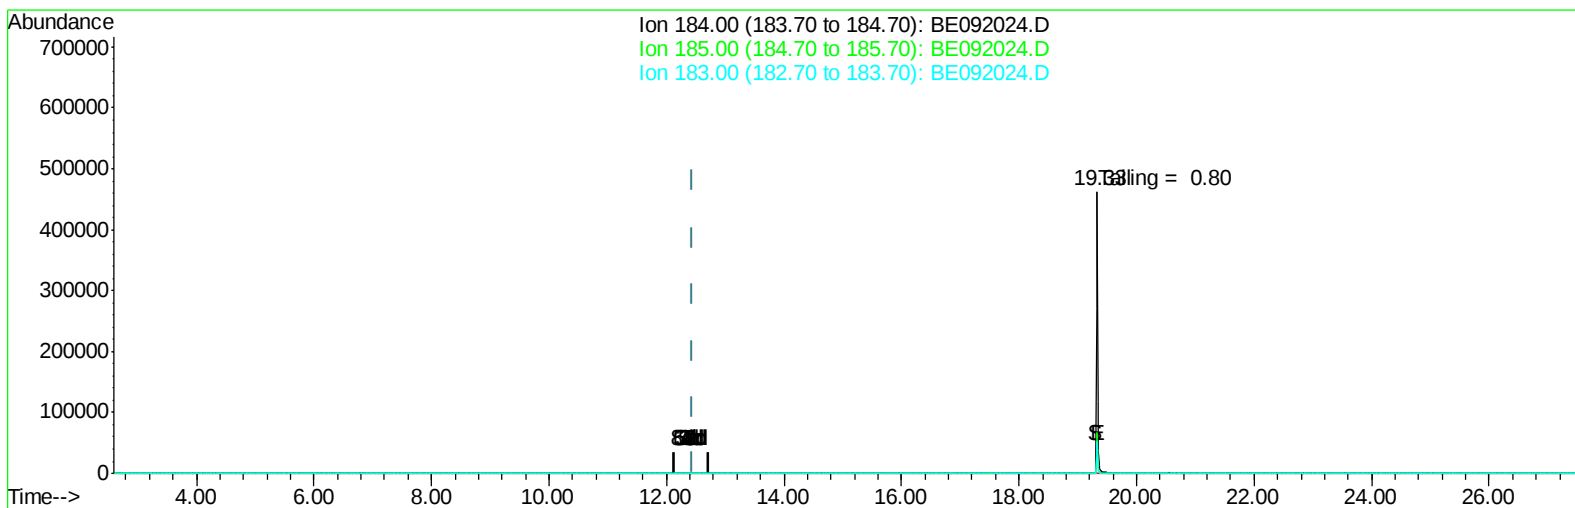

TIC: BE092024.D

(76) Benzidine




19.333min (+6.889) 1103445.29ng m

response 644912

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.63
183.00	12.00	11.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\Be072216\
Data File : BE092024.D
Acq On : 23 Jul 2016 2:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 07:15:48 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

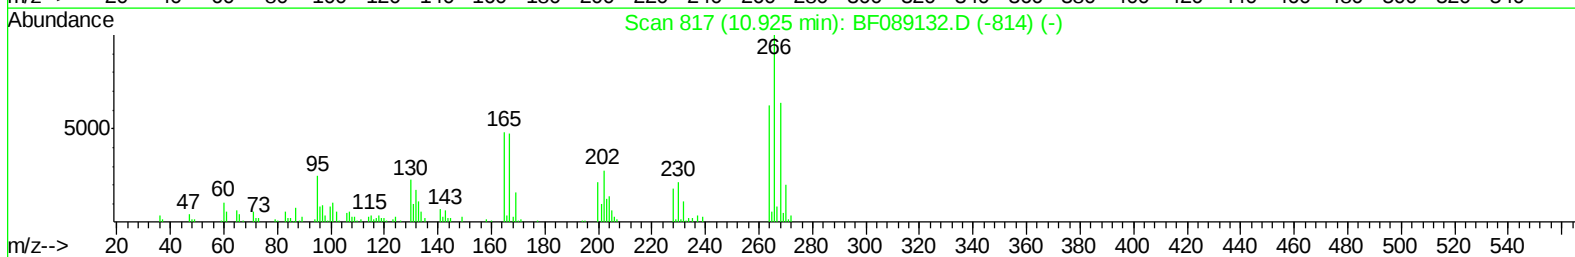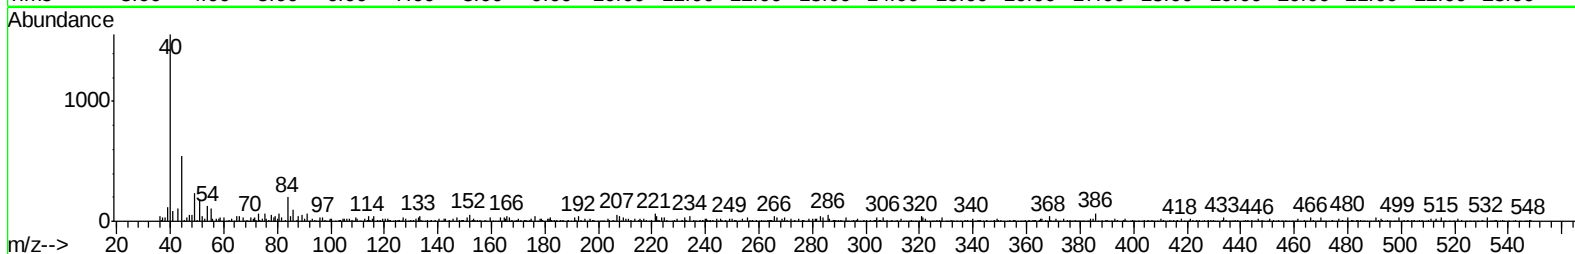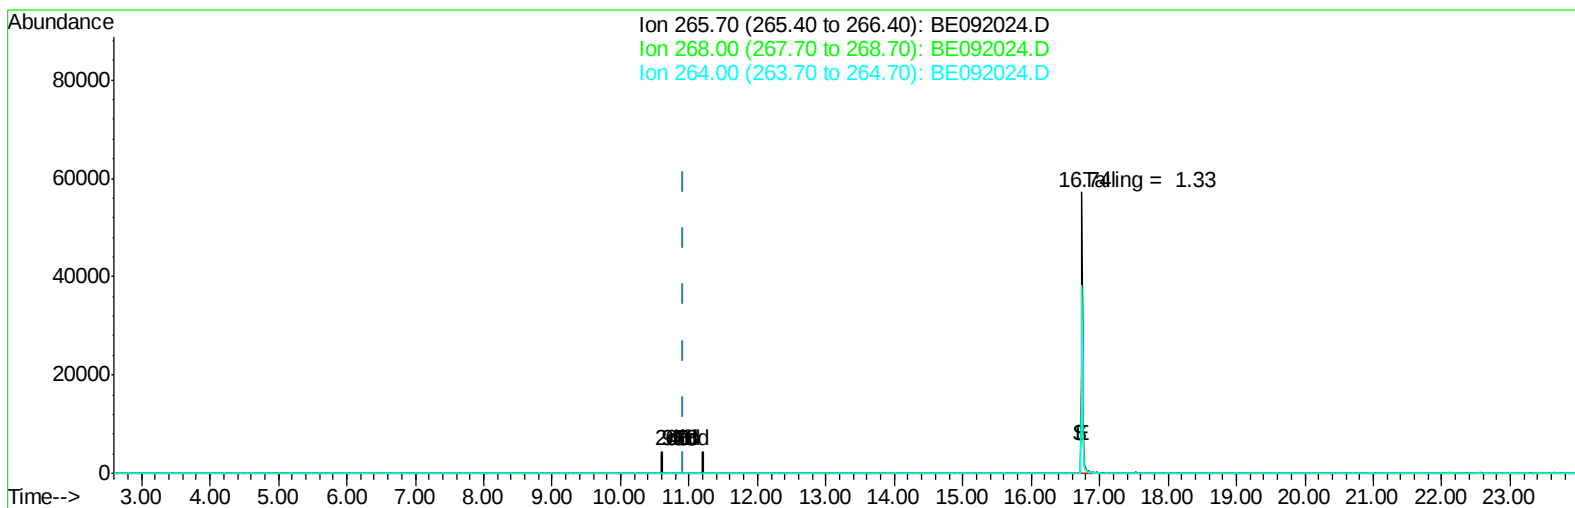

TIC: BE092024.D

(69) Pentachlorophenol (C)
10.884min (-0.040) 208.39ng
response 44

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	56.41
264.00	62.10	53.85
0.00	0.00	0.00