

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072216\
 Data File : BE092030.D
 Acq On : 23 Jul 2016 6:22
 Operator : UM/SJ
 Sample : H4107-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 TILCON-MH-3-4-STONE-002

Quant Time: Jul 25 02:07:34 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 22 15:39:27 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	24738	5.00	ng	0.00
8) Naphthalene-d8	10.99	136	118935	5.00	ng	0.00
15) Acenaphthene-d10	14.86	164	71962	5.00	ng	0.00
24) Phenanthrene-d10	17.59	188	186370	5.00	ng	0.00
31) Chrysene-d12	21.76	240	220806	5.00	ng	0.00
40) Perylene-d12	24.15	264	192985	5.00	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.72	112	35367	7.37	ng	0.00
5) Phenol-d6	7.35	99	52737	6.21	ng	-0.02
9) Nitrobenzene-d5	9.37	82	28012	3.91	ng	-0.02
16) 2,4,6-Tribromophenol	16.35	330	14273	5.77	ng	0.00
17) 2-Fluorobiphenyl	13.47	172	72320	3.82	ng	-0.01
34) Terphenyl-d14	20.20	244	109117	4.92	ng	-0.02
Target Compounds						
38) Bis(2-ethylhexyl)phthalate	21.64	149	66159	1.58	ng	Qvalue # 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072216\
Data File : BE092030.D
Acq On : 23 Jul 2016 6:22
Operator : UM/SJ
Sample : H4107-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TILCON-MH-3-4-STONE-002

Quant Time: Jul 25 02:07:34 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 22 15:39:27 2016
Response via : Initial Calibration

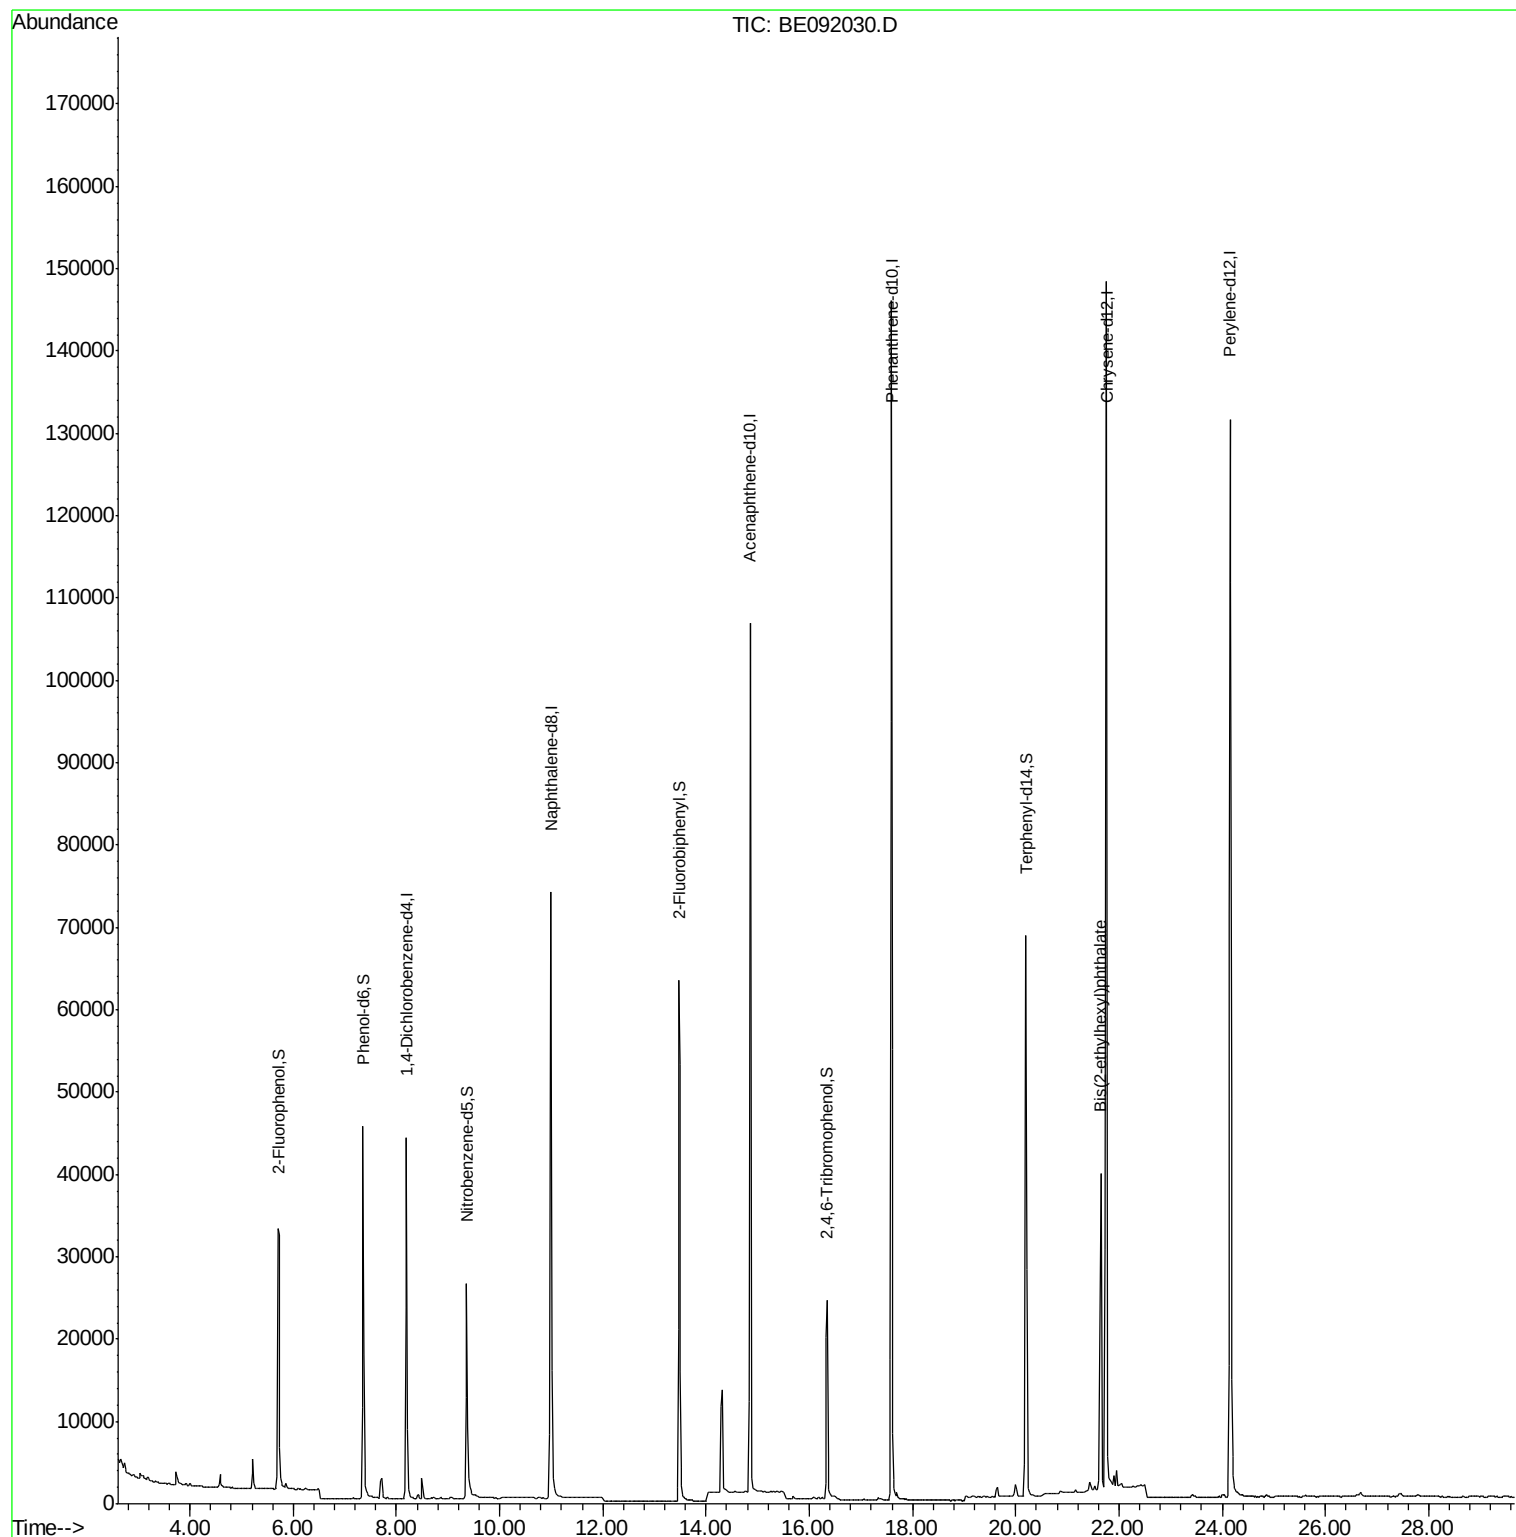



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.20 min Scan# 323

Delta R.T. -0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Instrument :

BNA_E

ClientSampleId :

TILCON-MH-3-4-STONE-002


Tgt Ion:152 Resp: 24738

Ion Ratio Lower Upper

152 100

150 147.8 123.9 185.9




115 54.9 48.3 72.5

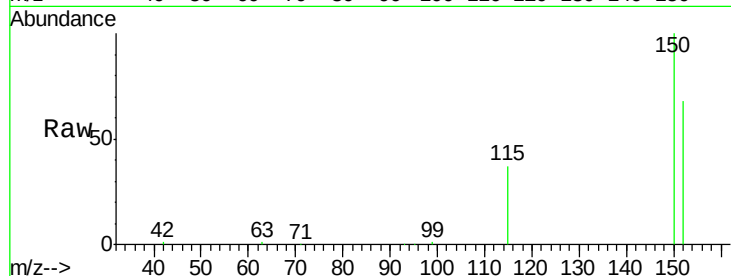

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

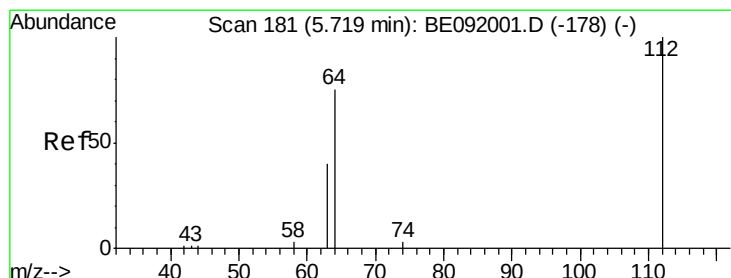

#4

2-Fluorophenol

Concen: 7.37 ng

RT: 5.72 min Scan# 181

Delta R.T. 0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22


Tgt Ion:112 Resp: 35367

Ion Ratio Lower Upper

112 100

64 68.1 53.7 80.5


63 37.3 29.5 44.3

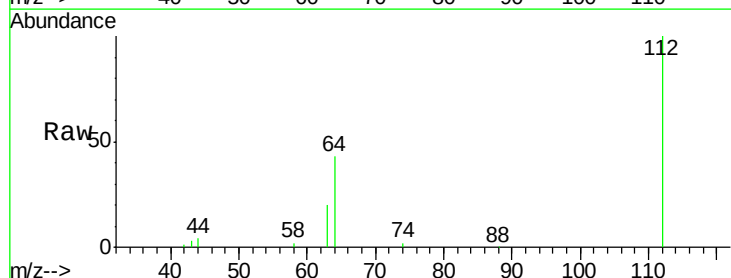


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0



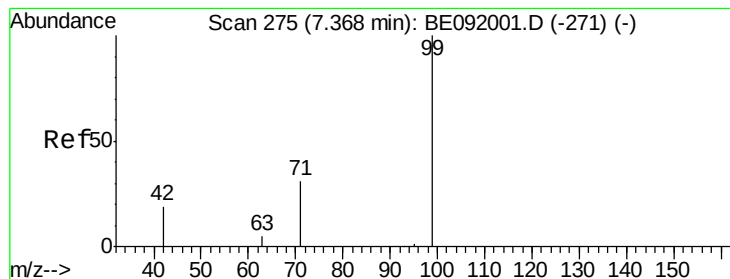

#5

Phenol-d6

Concen: 6.21 ng

RT: 7.35 min Scan# 274

Delta R.T. -0.02 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Instrument :

BNA_E

ClientSampleId :

TILCON-MH-3-4-STONE-002


Tgt Ion: 99 Resp: 52737

Ion Ratio Lower Upper

99 100

42 25.2 19.6 29.4




71 34.8 28.1 42.1

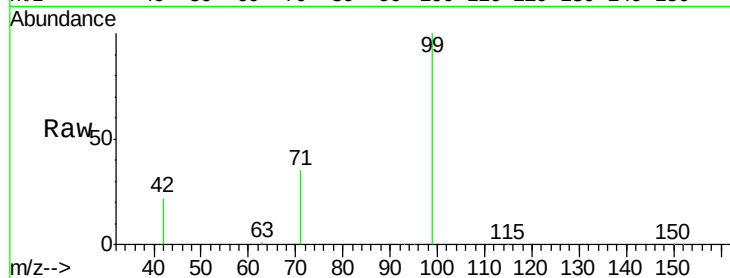

Abundance Ion 99.00 (98.70 to 99.70): BE092001.D (-271) (-)

Ion 42.00 (41.70 to 42.70): BE092001.D (-271) (-)

Ion 71.00 (70.70 to 71.70): BE092001.D (-271) (-)

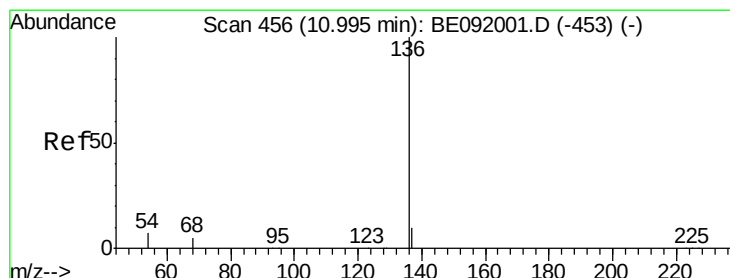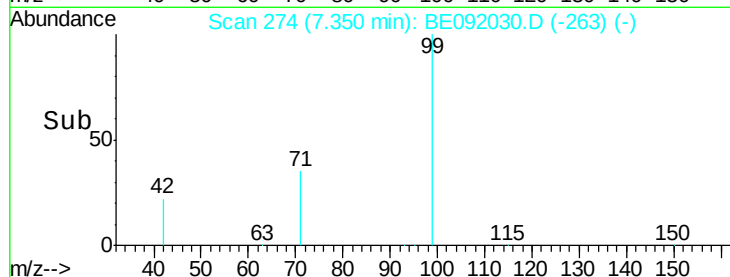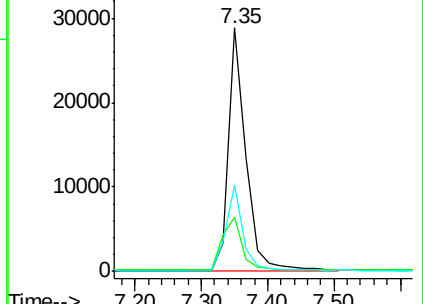

#8

Naphthalene-d8

Concen: 5.00 ng

RT: 10.99 min Scan# 456

Delta R.T. -0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Tgt Ion: 136 Resp: 118935


Ion Ratio Lower Upper

136 100

137 10.5 8.3 12.5

54 6.4 8.2 12.4#

68 4.8 5.9 8.9#


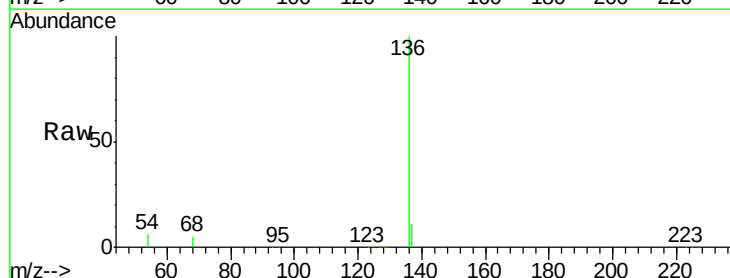



Abundance Ion 136.00 (135.70 to 136.70): BE092001.D (-453) (-)

Ion 137.00 (136.70 to 137.70): BE092001.D (-453) (-)

Ion 54.00 (53.70 to 54.70): BE092001.D (-453) (-)

Ion 68.00 (67.70 to 68.70): BE092001.D (-453) (-)

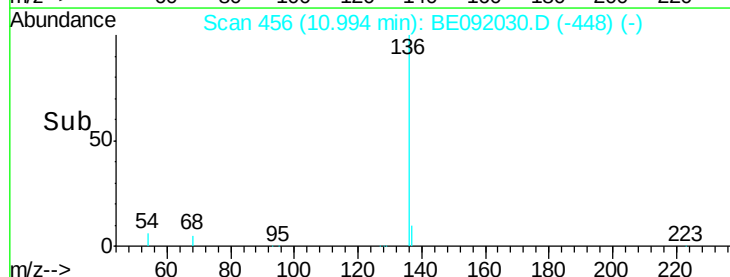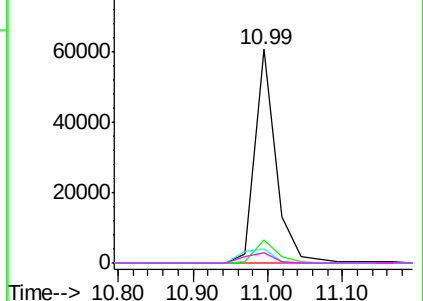

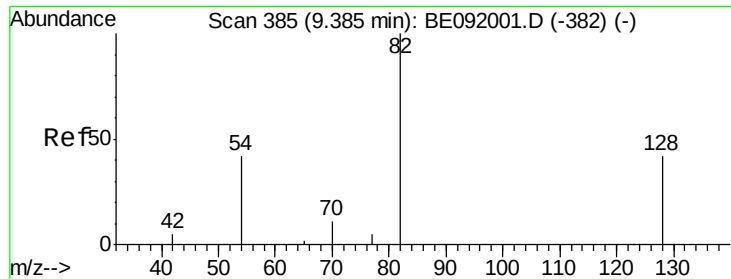

#9

Nitrobenzene-d5

Concen: 3.91 ng

RT: 9.37 min Scan# 384

Delta R.T. -0.02 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Instrument :

BNA_E

ClientSampleId :

TILCON-MH-3-4-STONE-002


Tgt Ion: 82 Resp: 28012

Ion Ratio Lower Upper

82 100

128 35.7 39.5 59.3#




54 45.6 30.3 45.5#

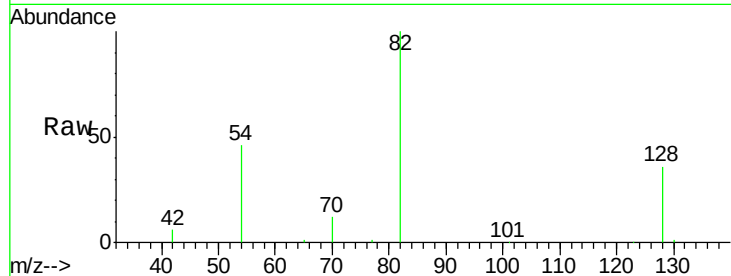

Abundance Ion 82.00 (81.70 to 82.70): BE092001.D (-382) (-)

Ion 128.00 (127.70 to 128.70): BE092001.D (-382) (-)

Ion 54.00 (53.70 to 54.70): BE092001.D (-382) (-)

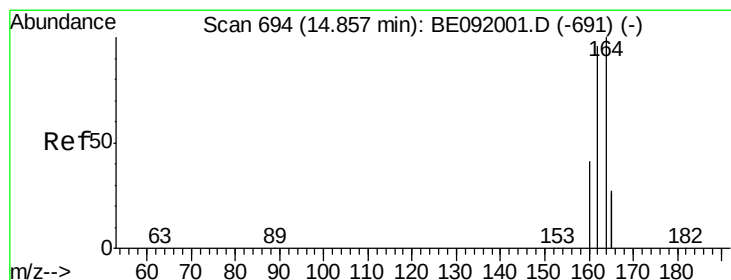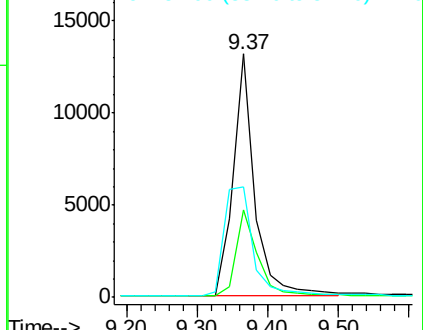

#15

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.86 min Scan# 694

Delta R.T. 0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22


Tgt Ion: 164 Resp: 71962

Ion Ratio Lower Upper

164 100

162 91.3 71.8 107.8



160 36.7 28.0 42.0

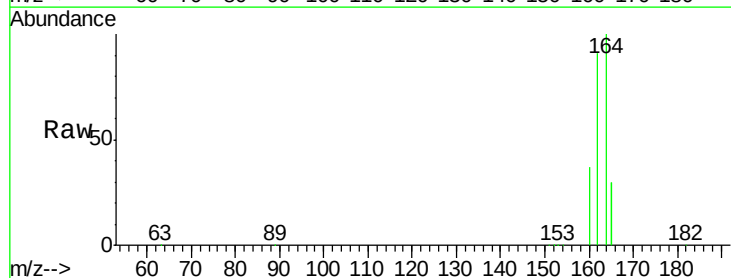


Abundance Ion 164.00 (163.70 to 164.70): BE092001.D (-691) (-)

Ion 162.00 (161.70 to 162.70): BE092001.D (-691) (-)

Ion 160.00 (159.70 to 160.70): BE092001.D (-691) (-)

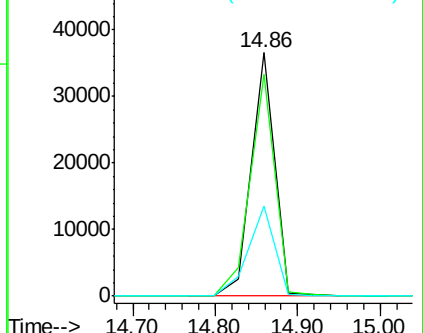


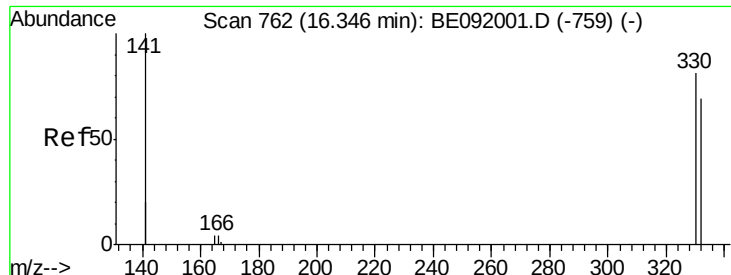




#16
 2,4,6-Tribromophenol
 Concen: 5.77 ng
 RT: 16.35 min Scan# 762
 Delta R.T. -0.00 min
 Lab File: BE092030.D
 Acq: 23 Jul 2016 6:22

Instrument :
 BNA_E
 ClientSampleId :
 TILCON-MH-3-4-STONE-002

Tgt Ion:330 Resp: 14273
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.0 115.6
 141 175.2 138.4 207.6

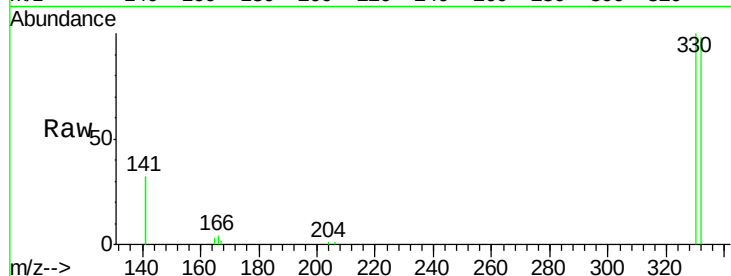


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

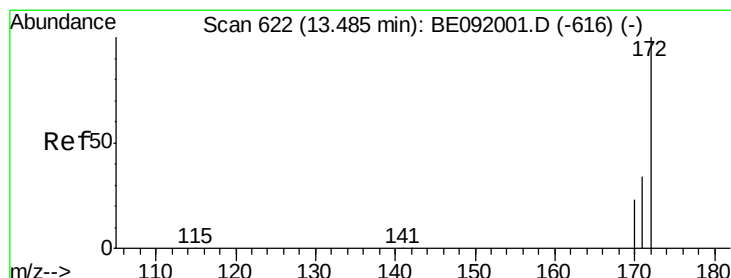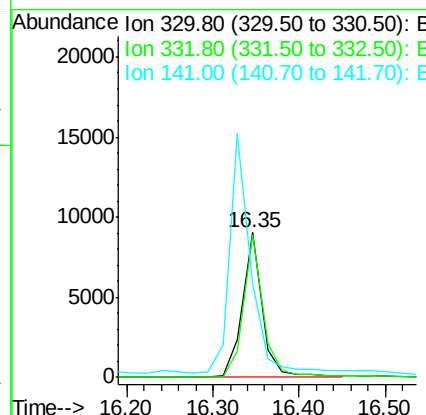




#17
 2-Fluorobiphenyl
 Concen: 3.82 ng
 RT: 13.47 min Scan# 621
 Delta R.T. -0.01 min
 Lab File: BE092030.D
 Acq: 23 Jul 2016 6:22

Tgt Ion:172 Resp: 72320
 Ion Ratio Lower Upper
 172 100
 171 36.9 24.3 36.5#
 170 26.6 14.9 22.3#

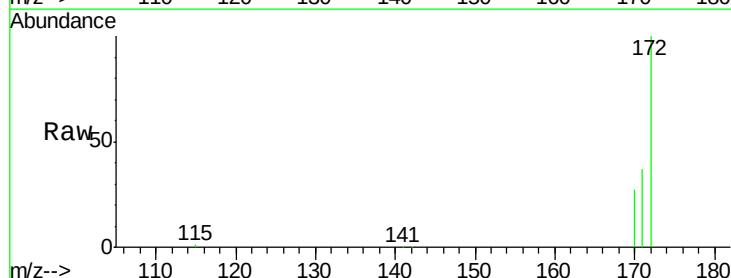

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

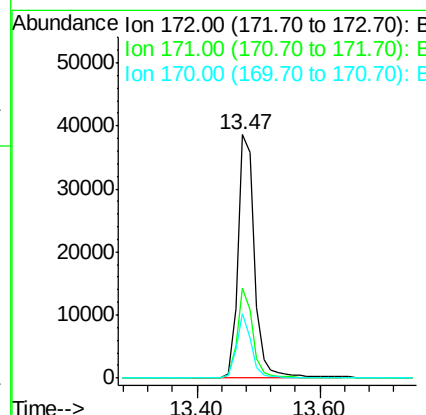



#24

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.59 min Scan# 835

Delta R.T. -0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Instrument :

BNA_E

ClientSampleId :

TILCON-MH-3-4-STONE-002


Tgt Ion:188 Resp: 186370

Ion Ratio Lower Upper

188 100

94 6.6 4.1 6.1#




80 5.8 3.4 5.2#

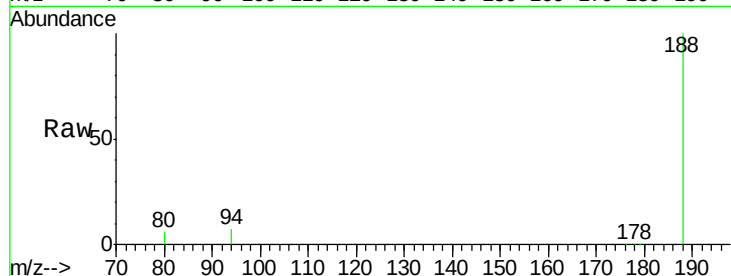

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

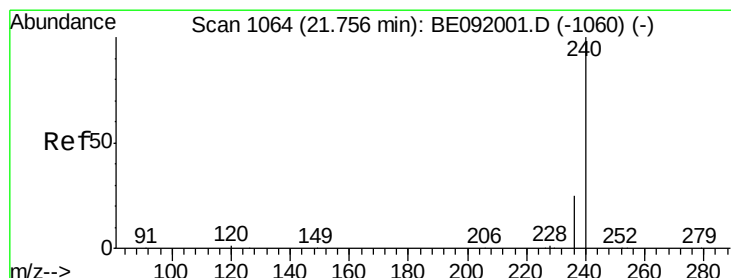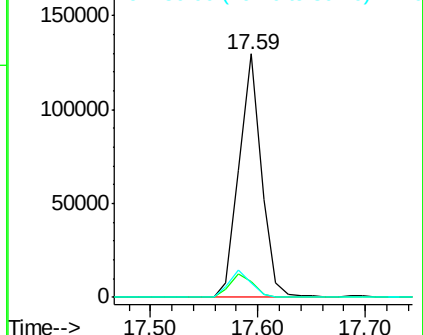

#31

Chrysene-d12

Concen: 5.00 ng

RT: 21.76 min Scan# 1064

Delta R.T. 0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22


Tgt Ion:240 Resp: 220806

Ion Ratio Lower Upper

240 100

120 0.7 1.2 1.8#



236 22.5 19.8 29.8

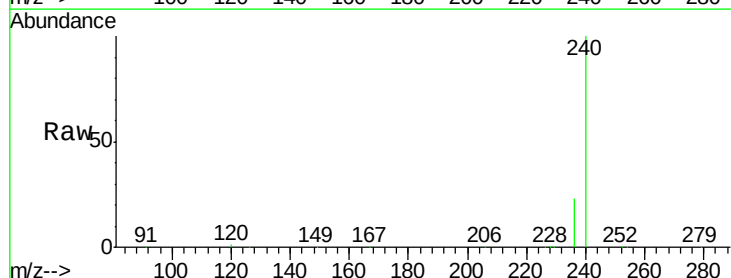


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

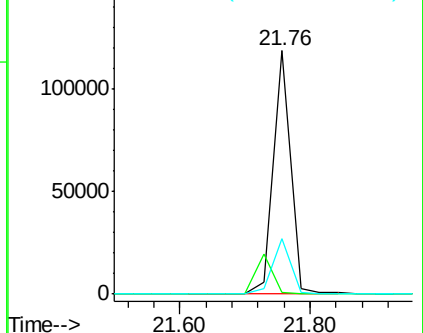

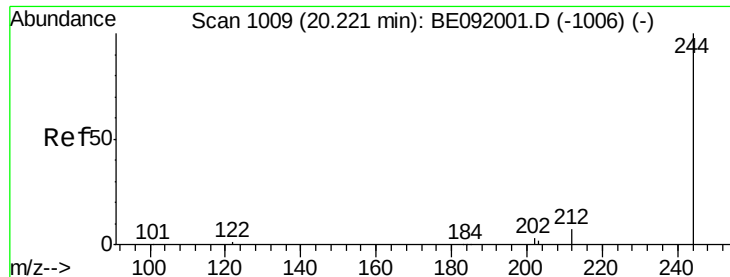

#34

Terphenyl-d14

Concen: 4.92 ng

RT: 20.20 min Scan# 1008

Delta R.T. -0.02 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Instrument :

BNA_E

ClientSampleId :

TILCON-MH-3-4-STONE-002


Tgt Ion: 244 Resp: 109117

Ion Ratio Lower Upper

244 100

212 10.3 6.5 9.7#




122 12.7 2.9 4.3#

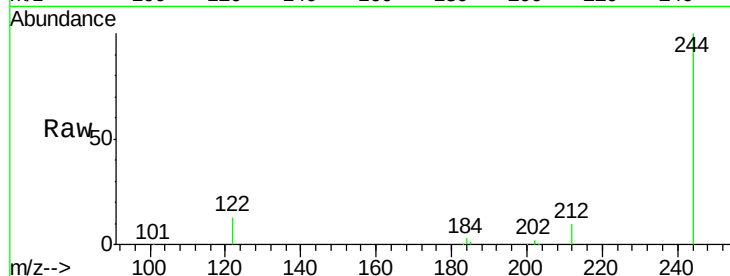

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

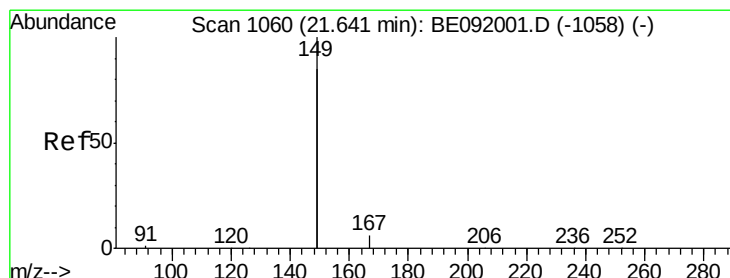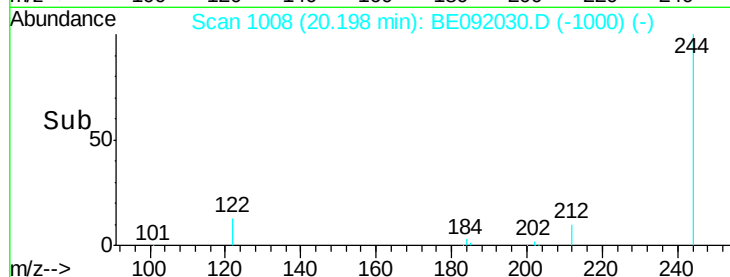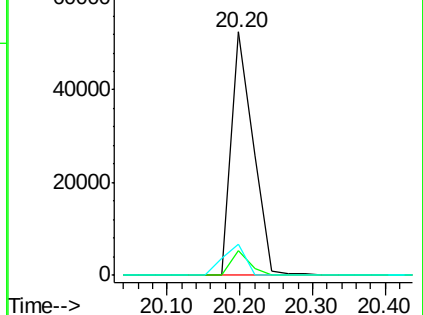

#38

Bis(2-ethylhexyl)phthalate

Concen: 1.58 ng

RT: 21.64 min Scan# 1060

Delta R.T. 0.00 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22


Tgt Ion: 149 Resp: 66159

Ion Ratio Lower Upper

149 100

167 4.8 0.0 0.0#



279 0.0 0.0 0.0



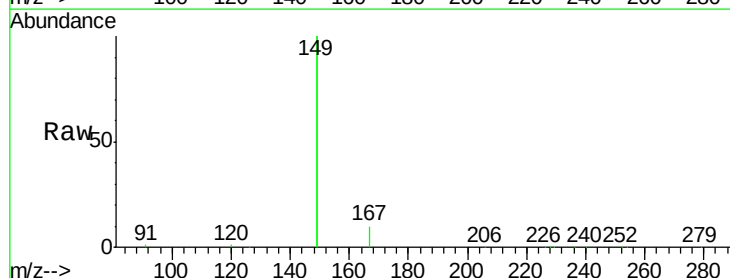


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

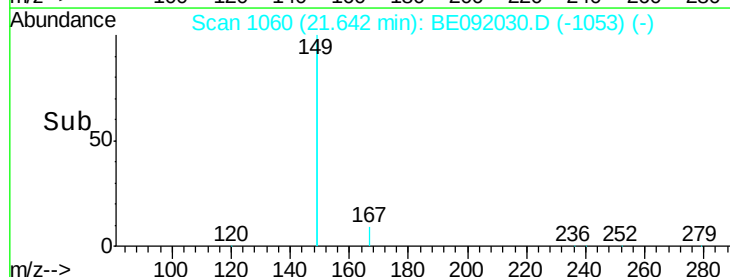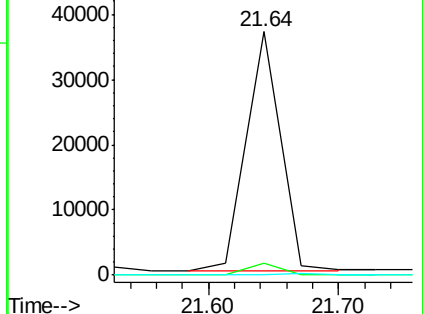

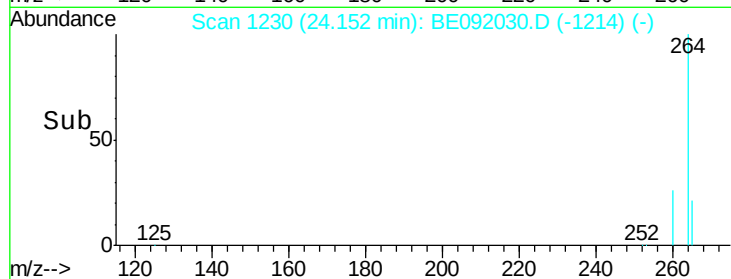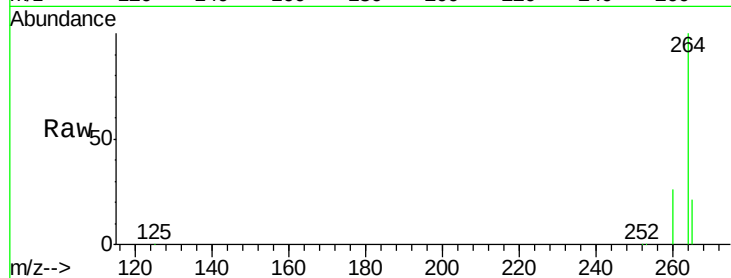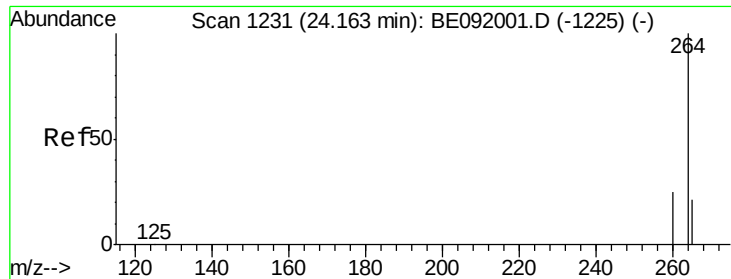

#40

Perylene-d12

Concen: 5.00 ng

RT: 24.15 min Scan# 1230

Delta R.T. -0.01 min

Lab File: BE092030.D

Acq: 23 Jul 2016 6:22

Instrument :

BNA_E

ClientSampleId :

TILCON-MH-3-4-STONE-002

Tgt Ion: 264 Resp: 192985

Ion Ratio Lower Upper

264 100

260 26.1 20.3 30.5

265 21.3 17.6 26.4

