


Data Path : Z:\HPCHEM1\BNA_E\Data\Be072216\
Data File : BE091997.D
Acq On : 22 Jul 2016 8:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 22 15:39:27 2016

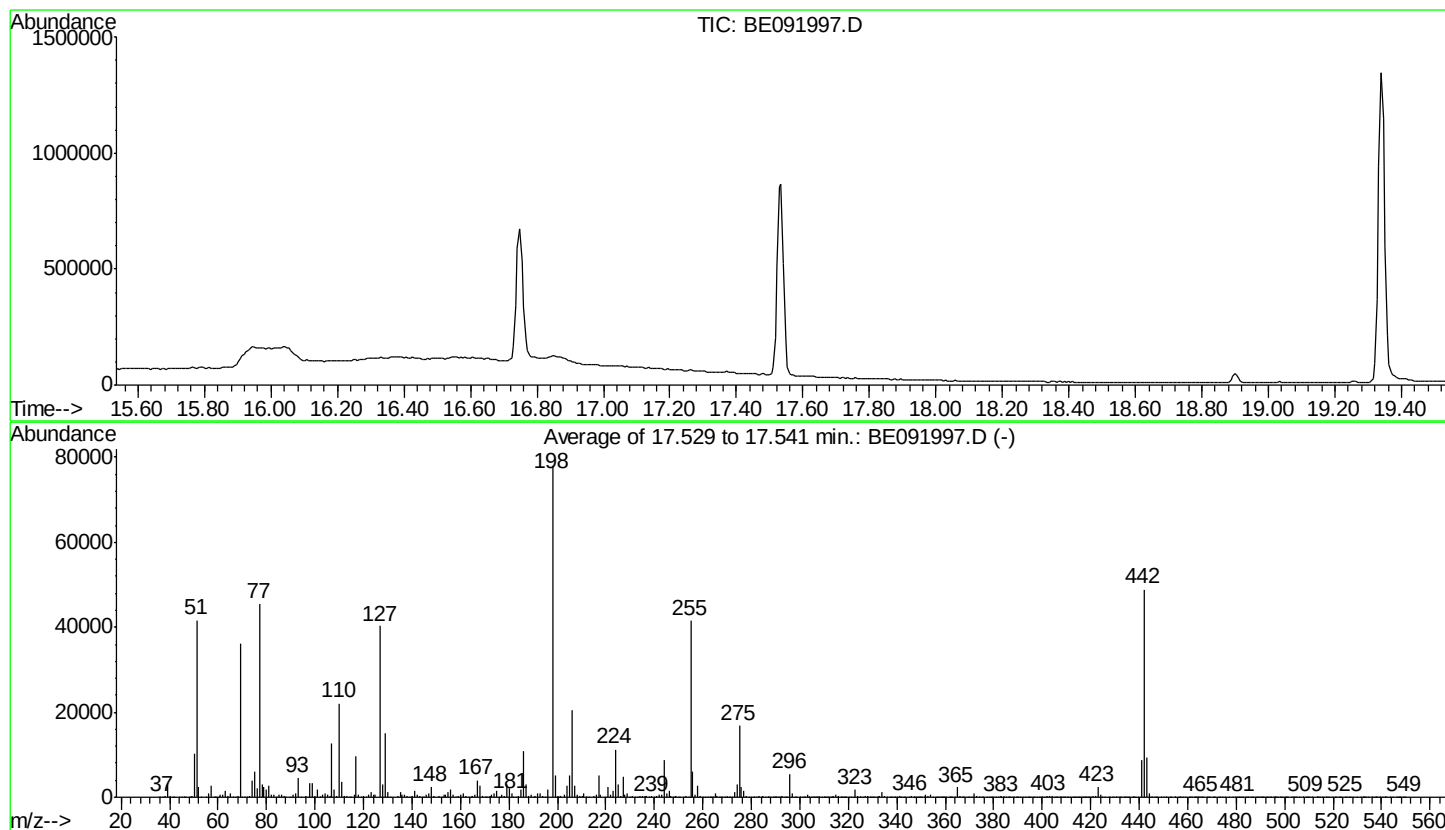

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2534

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	41721	PASS
68	69	0.00	2	1.2	433	PASS
69	198	0.00	100	46.2	36089	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	51.7	40311	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78046	PASS
199	198	5	9	6.7	5192	PASS
275	198	10	60	21.6	16826	PASS
365	198	1	100	3.0	2367	PASS
441	442	0.01	24	17.8	8695	PASS
442	198	50	100	62.7	48933	PASS
443	442	15	24	19.4	9484	PASS