


Data Path : Z:\HPCHEM1\BNA_E\Data\Be072216\
Data File : BE092024.D
Acq On : 23 Jul 2016 2:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 22 15:39:27 2016

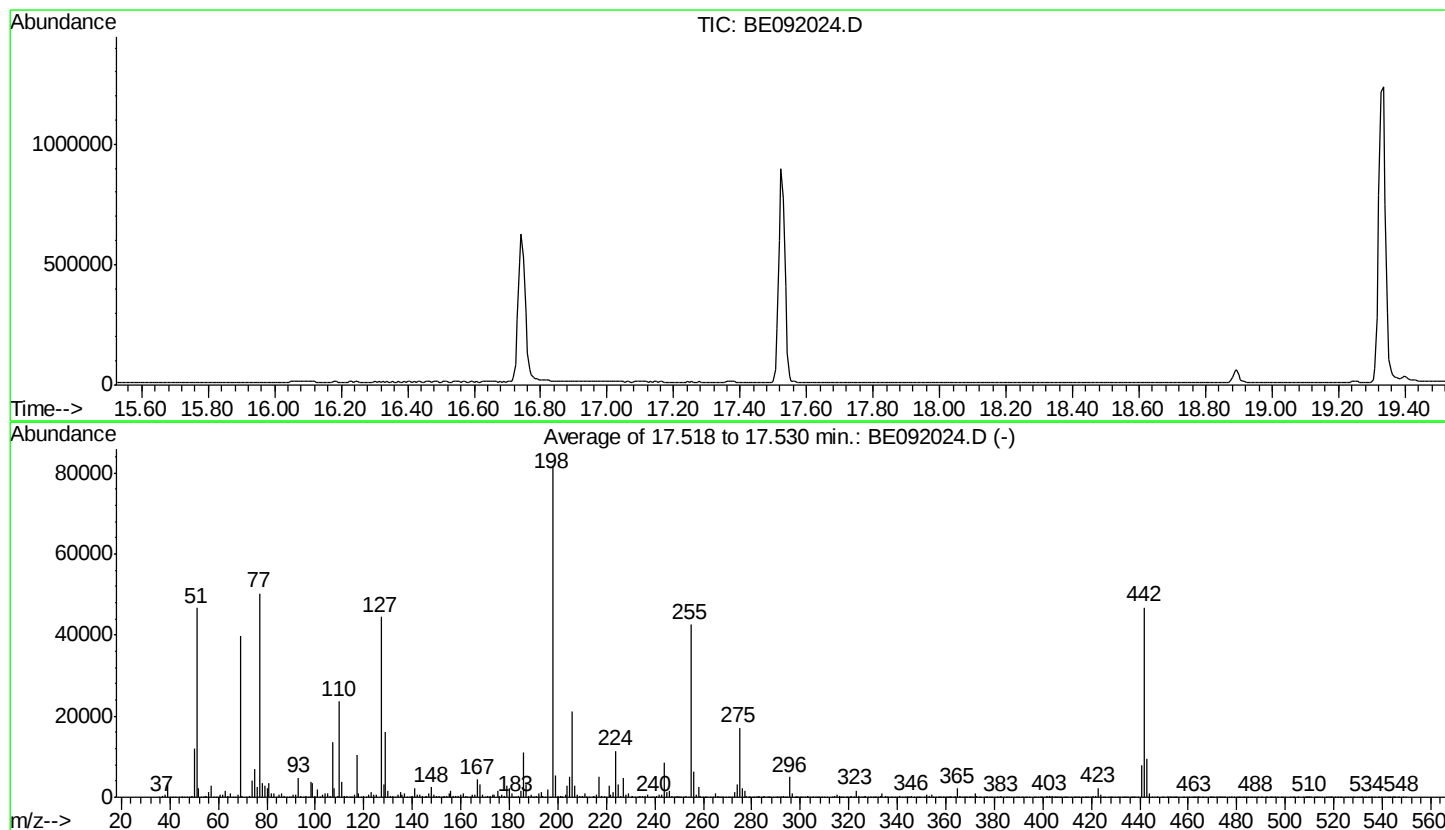

AutoFind: Scans 2541, 2542, 2543; Background Corrected with Scan 2533

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	46660	PASS
68	69	0.00	2	1.8	727	PASS
69	198	0.00	100	48.6	39733	PASS
70	69	0.00	2	0.6	246	PASS
127	198	10	80	54.4	44503	PASS
197	198	0.00	2	0.2	136	PASS
198	198	100	100	100.0	81784	PASS
199	198	5	9	6.6	5437	PASS
275	198	10	60	21.0	17140	PASS
365	198	1	100	2.6	2150	PASS
441	442	0.01	24	17.1	8002	PASS
442	198	50	100	57.2	46769	PASS
443	442	15	24	20.3	9485	PASS