

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
 Data File : BE093538.D
 Acq On : 24 Jul 2017 15:01
 Operator : SJ/JU
 Sample : PB100726BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK26

Quant Time: Jul 24 17:25:58 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 13:14:05 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3131	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16835	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	11599	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	30770	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	2200816	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	8690	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	28493	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.52	166	2977	0.062	ng/ul#	19
17) Pyrene	19.65	202	3919	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
Data File : BE093538.D
Acq On : 24 Jul 2017 15:01
Operator : SJ/JU
Sample : PB100726BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK26

Quant Time: Jul 24 17:25:58 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 13:14:05 2017
Response via : Initial Calibration




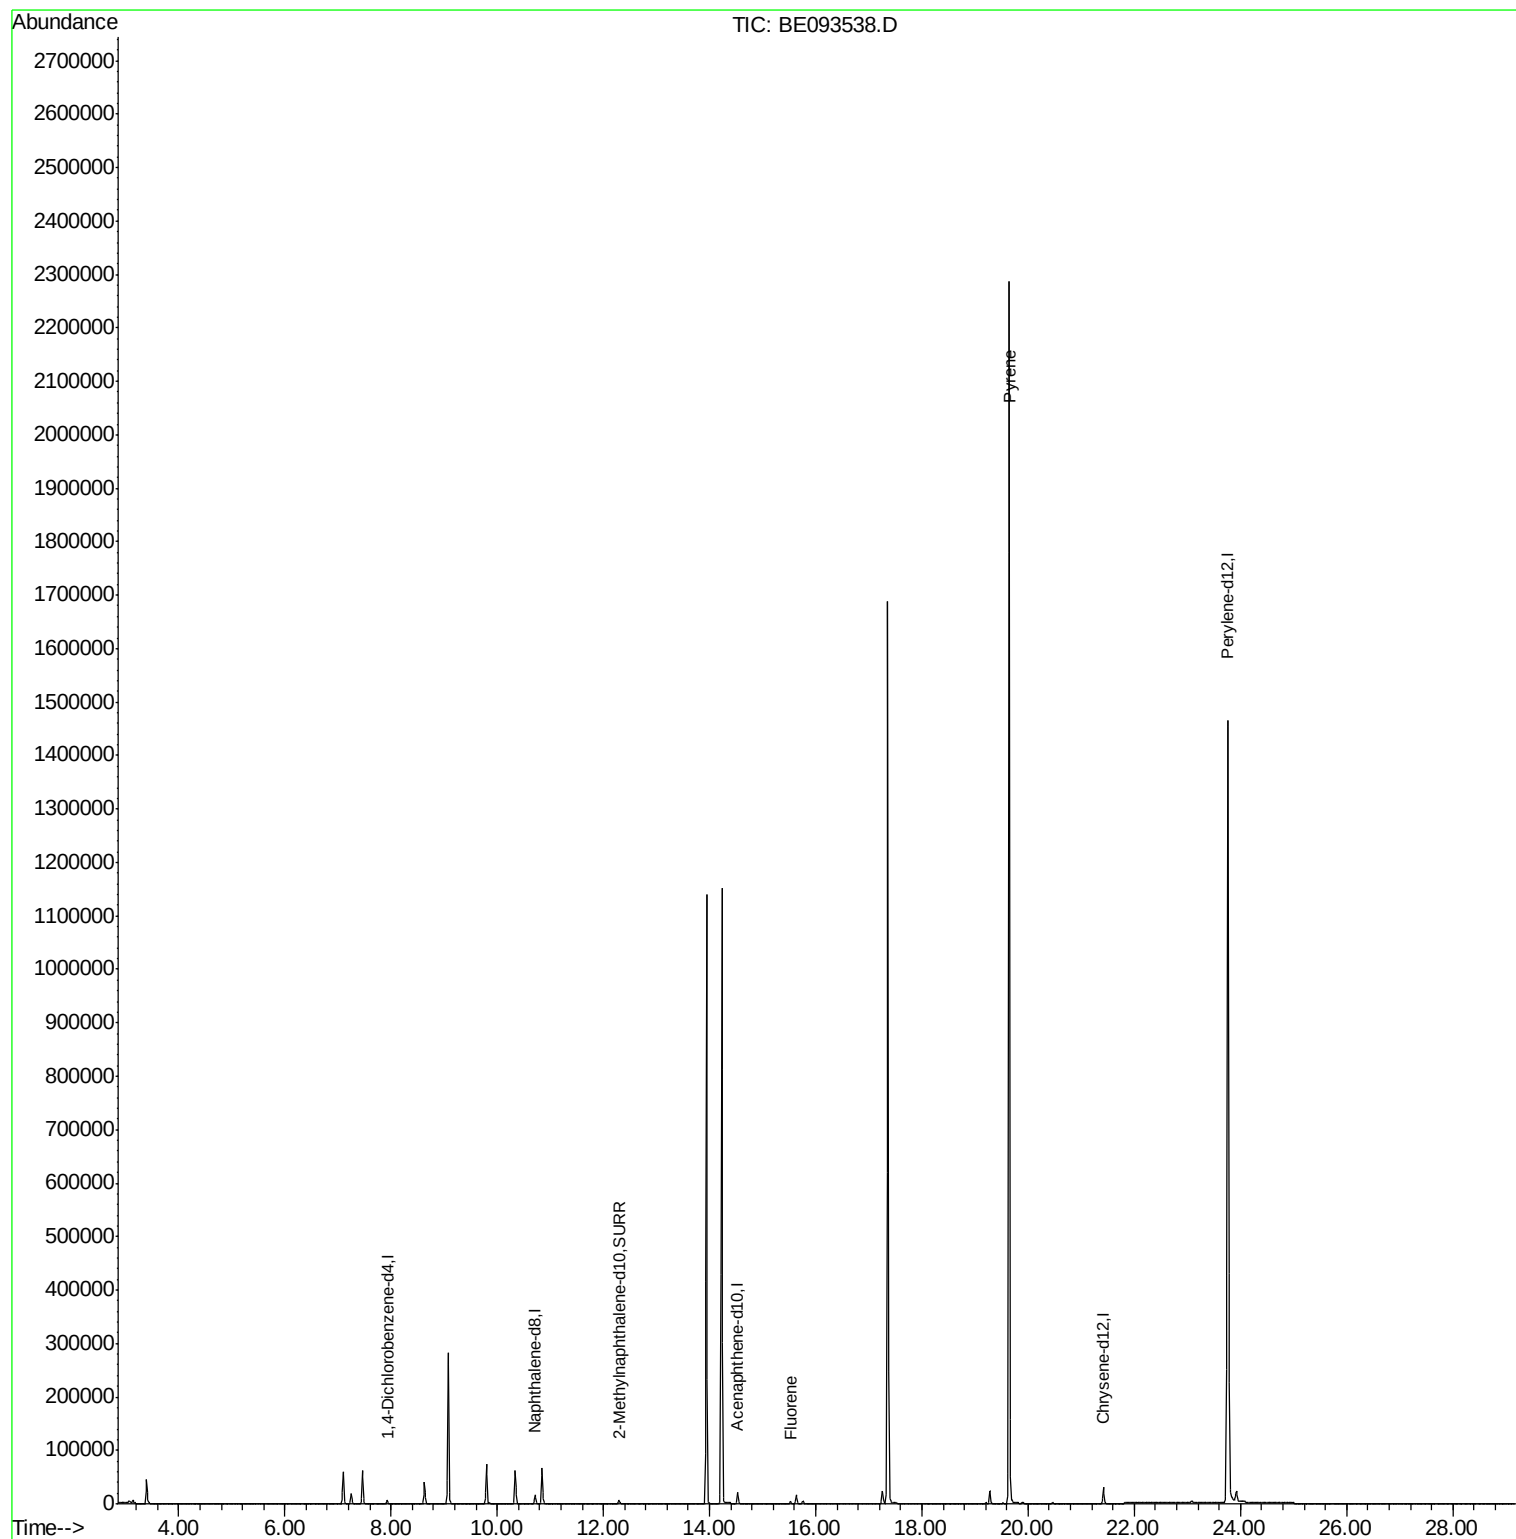


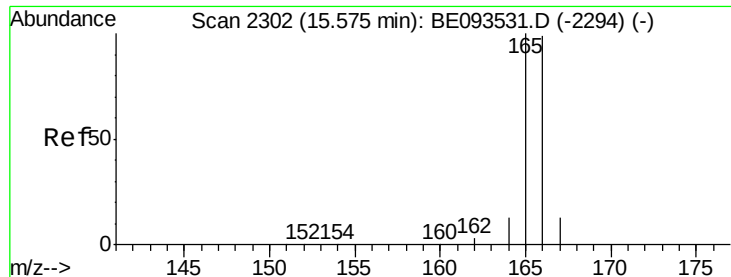

#9
Fluorene
 Concen: 0.062 ng/ul
 RT: 15.52 min Scan# 2294
 Delta R.T. -0.05 min
 Lab File: BE093538.D
 Acq: 24 Jul 2017 15:01

Instrument :
 BNA_E
 ClientSampleId :
 SBLK26

Tgt Ion:166 Resp: 2977
 Ion Ratio Lower Upper
 166 100
 165 6.1 73.4 110.2#
 167 33.8 14.6 22.0#

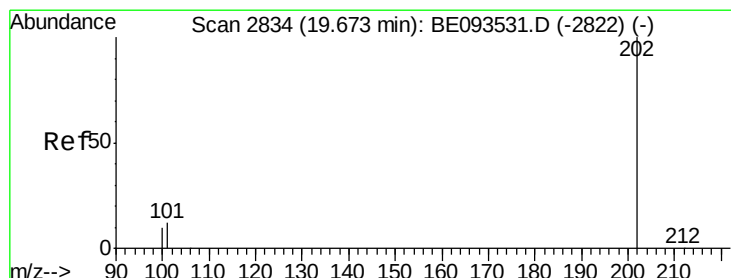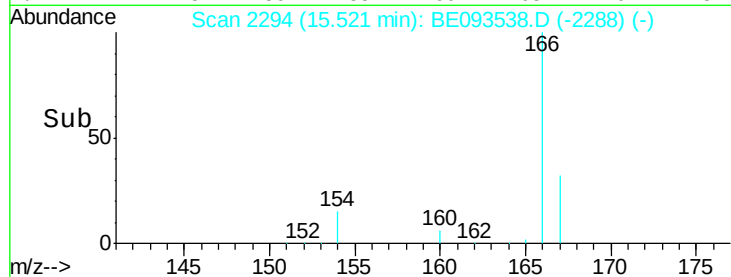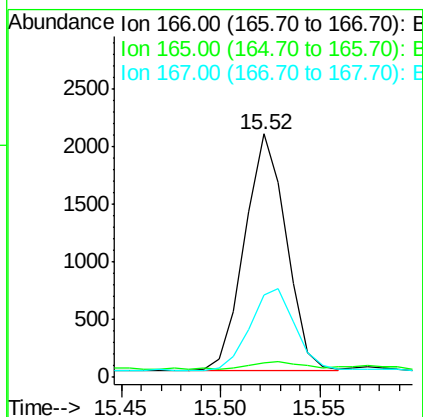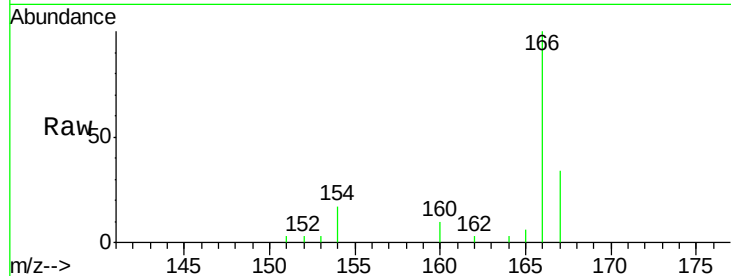

#17
Pyrene
 Concen: 0.044 ng/ul
 RT: 19.65 min Scan# 2827
 Delta R.T. -0.03 min
 Lab File: BE093538.D
 Acq: 24 Jul 2017 15:01

Tgt Ion:202 Resp: 3919
 Ion Ratio Lower Upper
 202 100
 101 161.2 18.2 27.4#
 100 848.2 15.6 23.4#

