

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072417\
 Data File : BE093545.D
 Acq On : 24 Jul 2017 19:18
 Operator : SJ/JU
 Sample : I4214-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B76

Quant Time: Jul 25 01:24:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 18:07:15 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	3012	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16246	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	11234	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	30232	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	2146429	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	8343	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	29079	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.77	128	1791	0.045	ng/ul#	93
17) Pyrene	19.67	202	2218	0.025	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072417\
Data File : BE093545.D
Acq On : 24 Jul 2017 19:18
Operator : SJ/JU
Sample : I4214-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0B76

Quant Time: Jul 25 01:24:03 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 18:07:15 2017
Response via : Initial Calibration

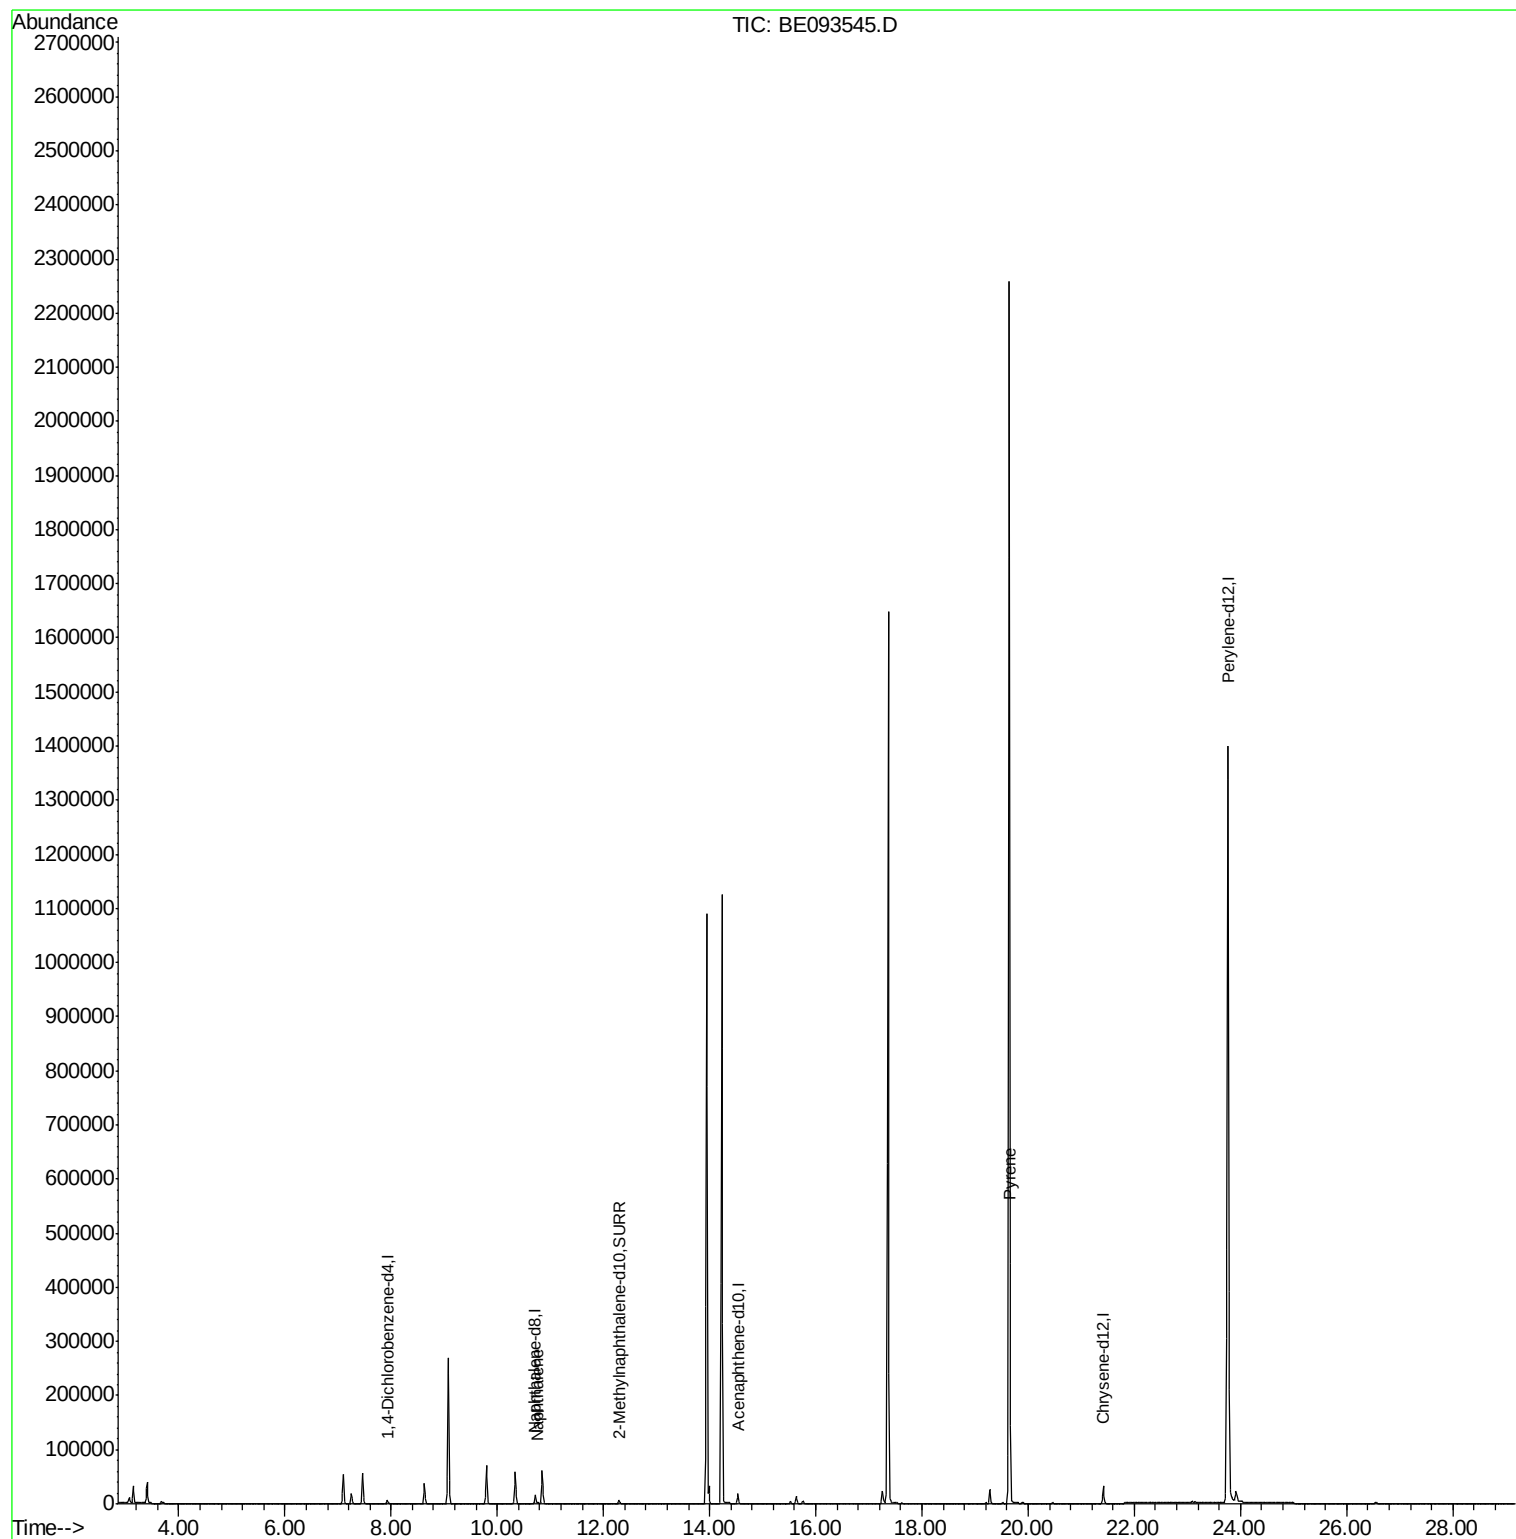

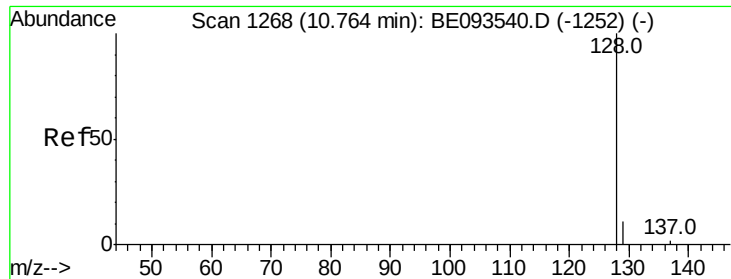

#3

Naphthalene

Concen: 0.045 ng/ul

RT: 10.77 min Scan# 1268

Delta R.T. 0.00 min

Lab File: BE093545.D

Acq: 24 Jul 2017 19:18

Instrument :

BNA_E

ClientSampled :

C0B76


Tot Ion:128 Resp: 1791

Ion Ratio Lower Upper

128 100

129 15.5 11.3 16.9




127 0.0 4.0 6.0#

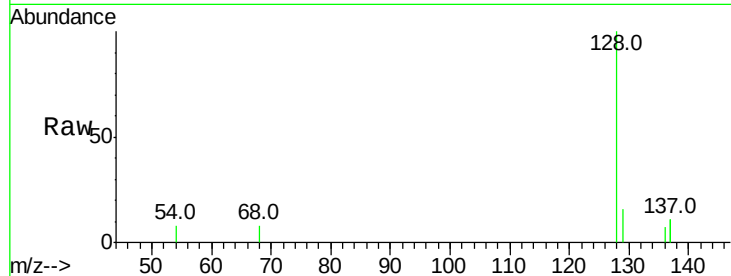

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

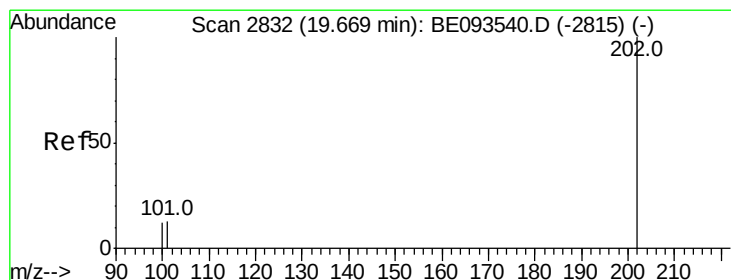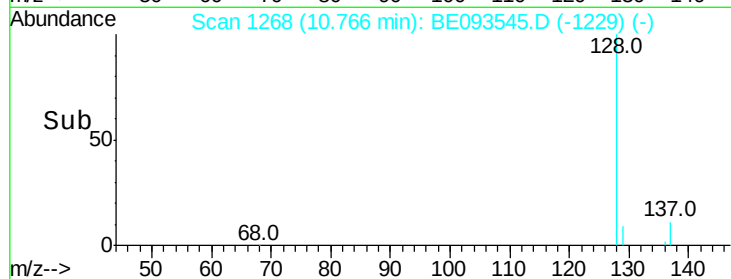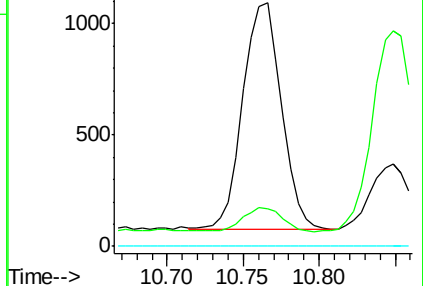

#17

Pyrene

Concen: 0.025 ng/ul

RT: 19.67 min Scan# 2832

Delta R.T. -0.00 min

Lab File: BE093545.D

Acq: 24 Jul 2017 19:18


Tgt Ion:202 Resp: 2218

Ion Ratio Lower Upper

202 100

101 19.4 18.2 27.4

100 25.9 15.6 23.4#

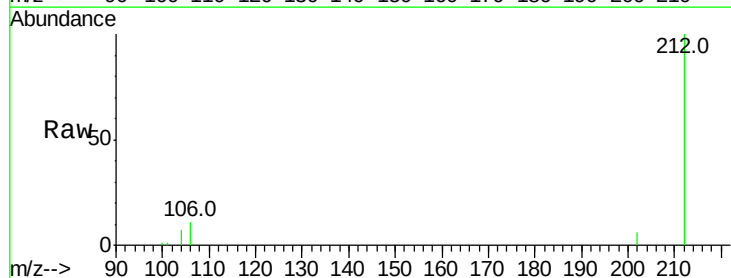

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

