

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072417\
 Data File : BE093546.D
 Acq On : 24 Jul 2017 19:57
 Operator : SJ/JU
 Sample : I4214-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B89

Quant Time: Jul 25 01:24:09 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 18:07:15 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3013	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16407	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	11420	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	30719	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	218840	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	8507	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	29230	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.52	166	3016	0.063	ng/ul#	19
17) Pyrene	19.64	202	4034	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072417\
Data File : BE093546.D
Acq On : 24 Jul 2017 19:57
Operator : SJ/JU
Sample : I4214-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0B89

Quant Time: Jul 25 01:24:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 18:07:15 2017
Response via : Initial Calibration

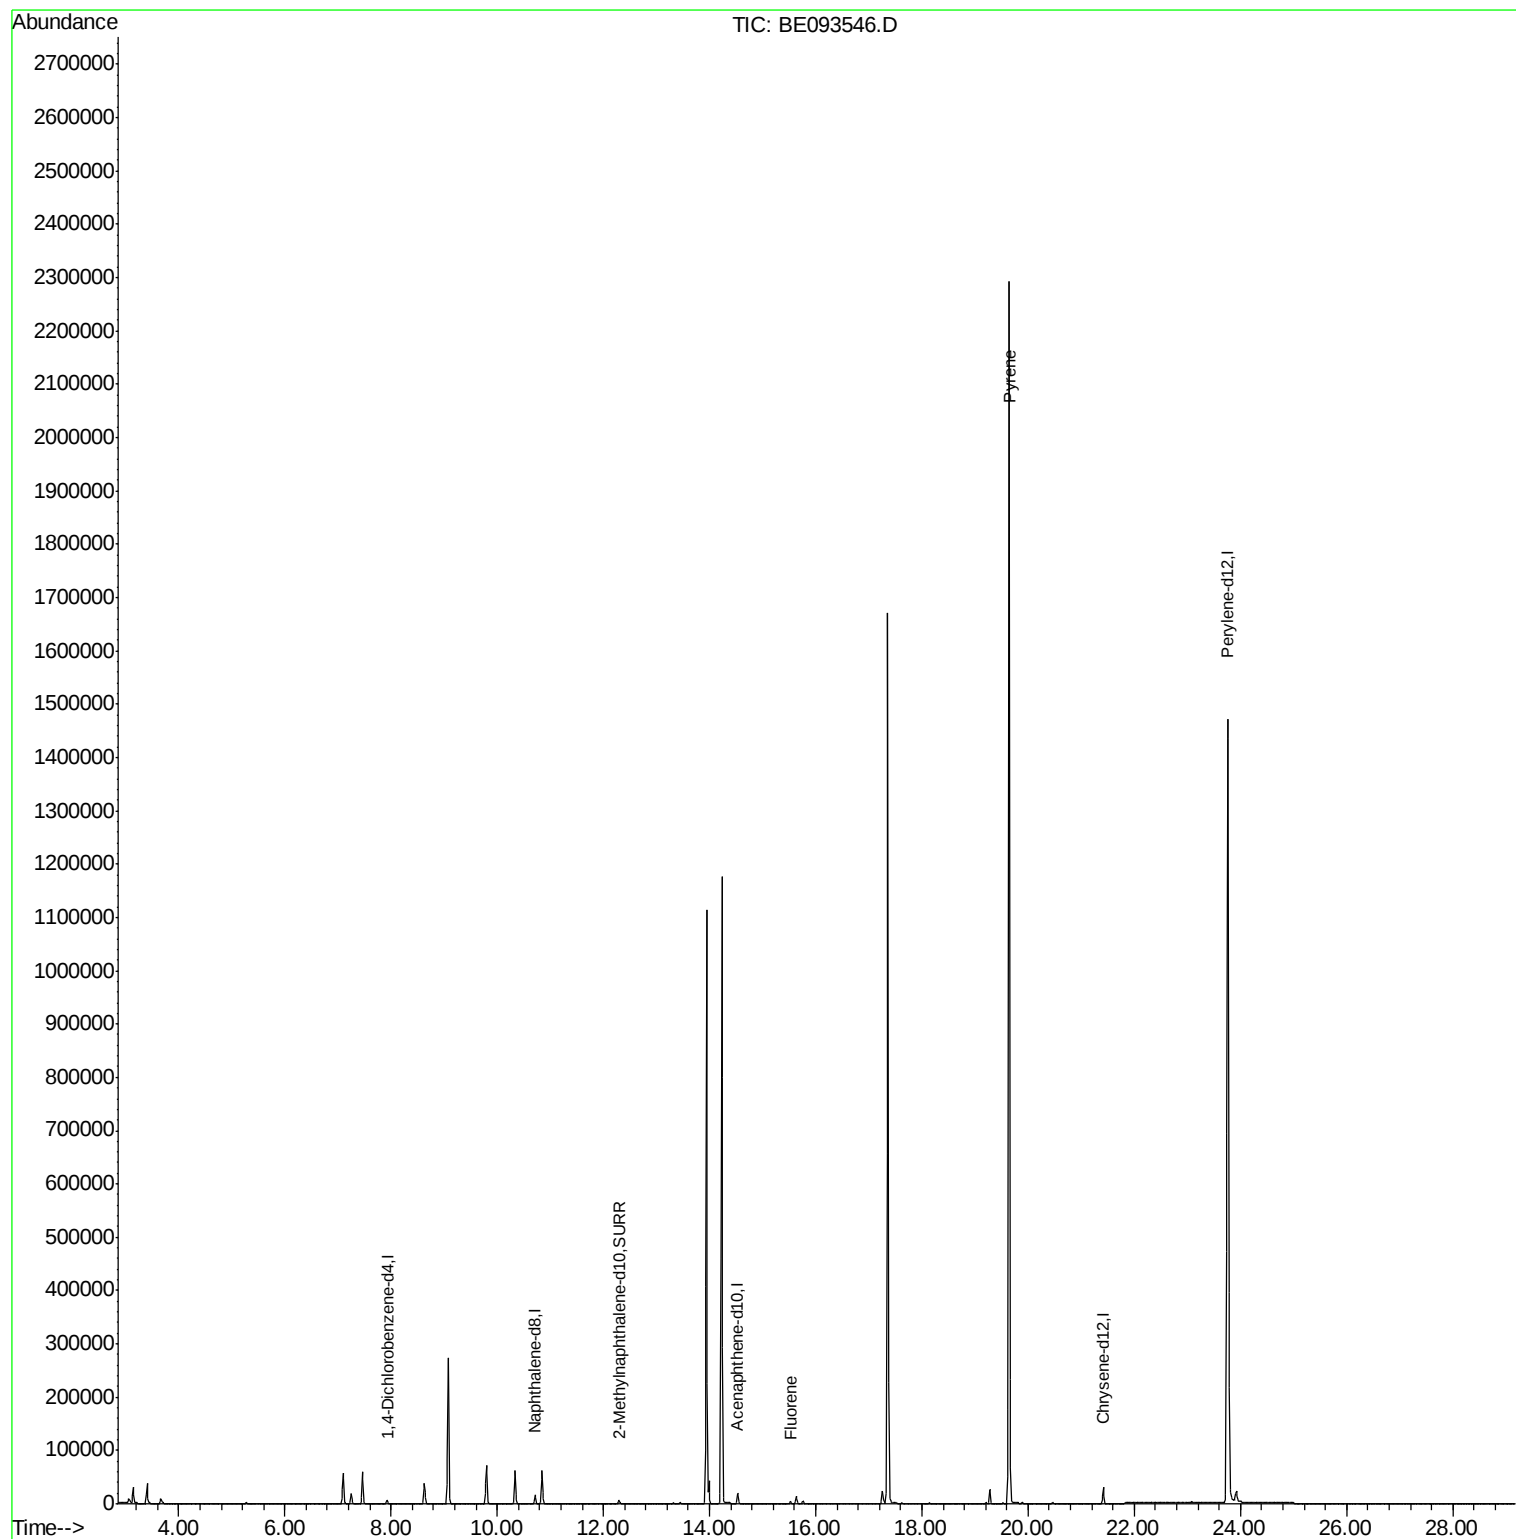

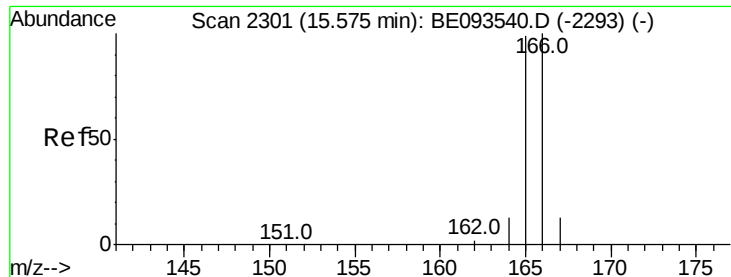

#9

Fluorene

Concen: 0.063 ng/ul

RT: 15.52 min Scan# 2293

Delta R.T. -0.05 min

Lab File: BE093546.D

Acq: 24 Jul 2017 19:57

Instrument :

BNA_E

ClientSampleId :

C0B89


Tot Ion:166 Resp: 3016

Ion Ratio Lower Upper

166 100

165 6.0 73.4 110.2#




167 35.0 14.6 22.0#

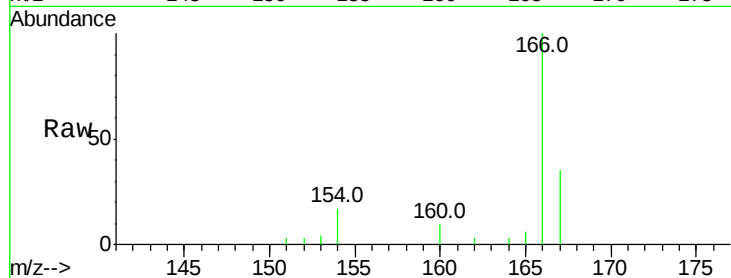

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

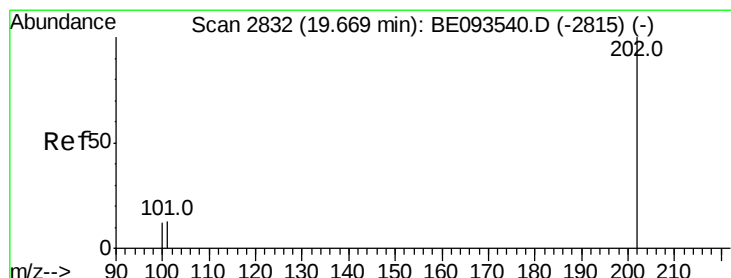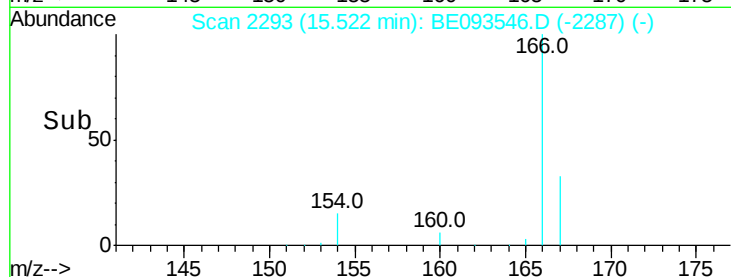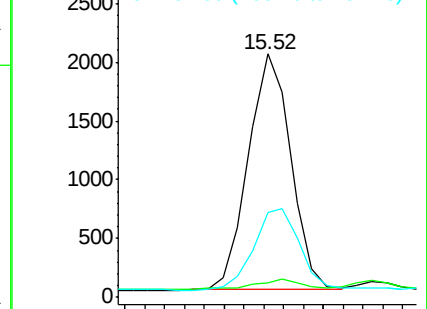

#17

Pyrene

Concen: 0.045 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.03 min

Lab File: BE093546.D

Acq: 24 Jul 2017 19:57


Tgt Ion:202 Resp: 4034

Ion Ratio Lower Upper

202 100

101 163.8 18.2 27.4#

100 911.6 15.6 23.4#

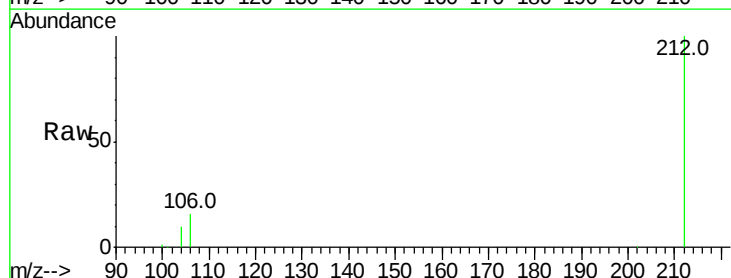

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

