


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
Data File : BE093537.D
Acq On : 24 Jul 2017 14:22
Operator : SJ/JU
Sample : PB100766BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK66

Manual Integrations
APPROVED

Sohil
7/25/2017 5:32:30 PM

Quant Time: Jul 24 15:45:23 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 13:14:05 2017
Response via : Initial Calibration

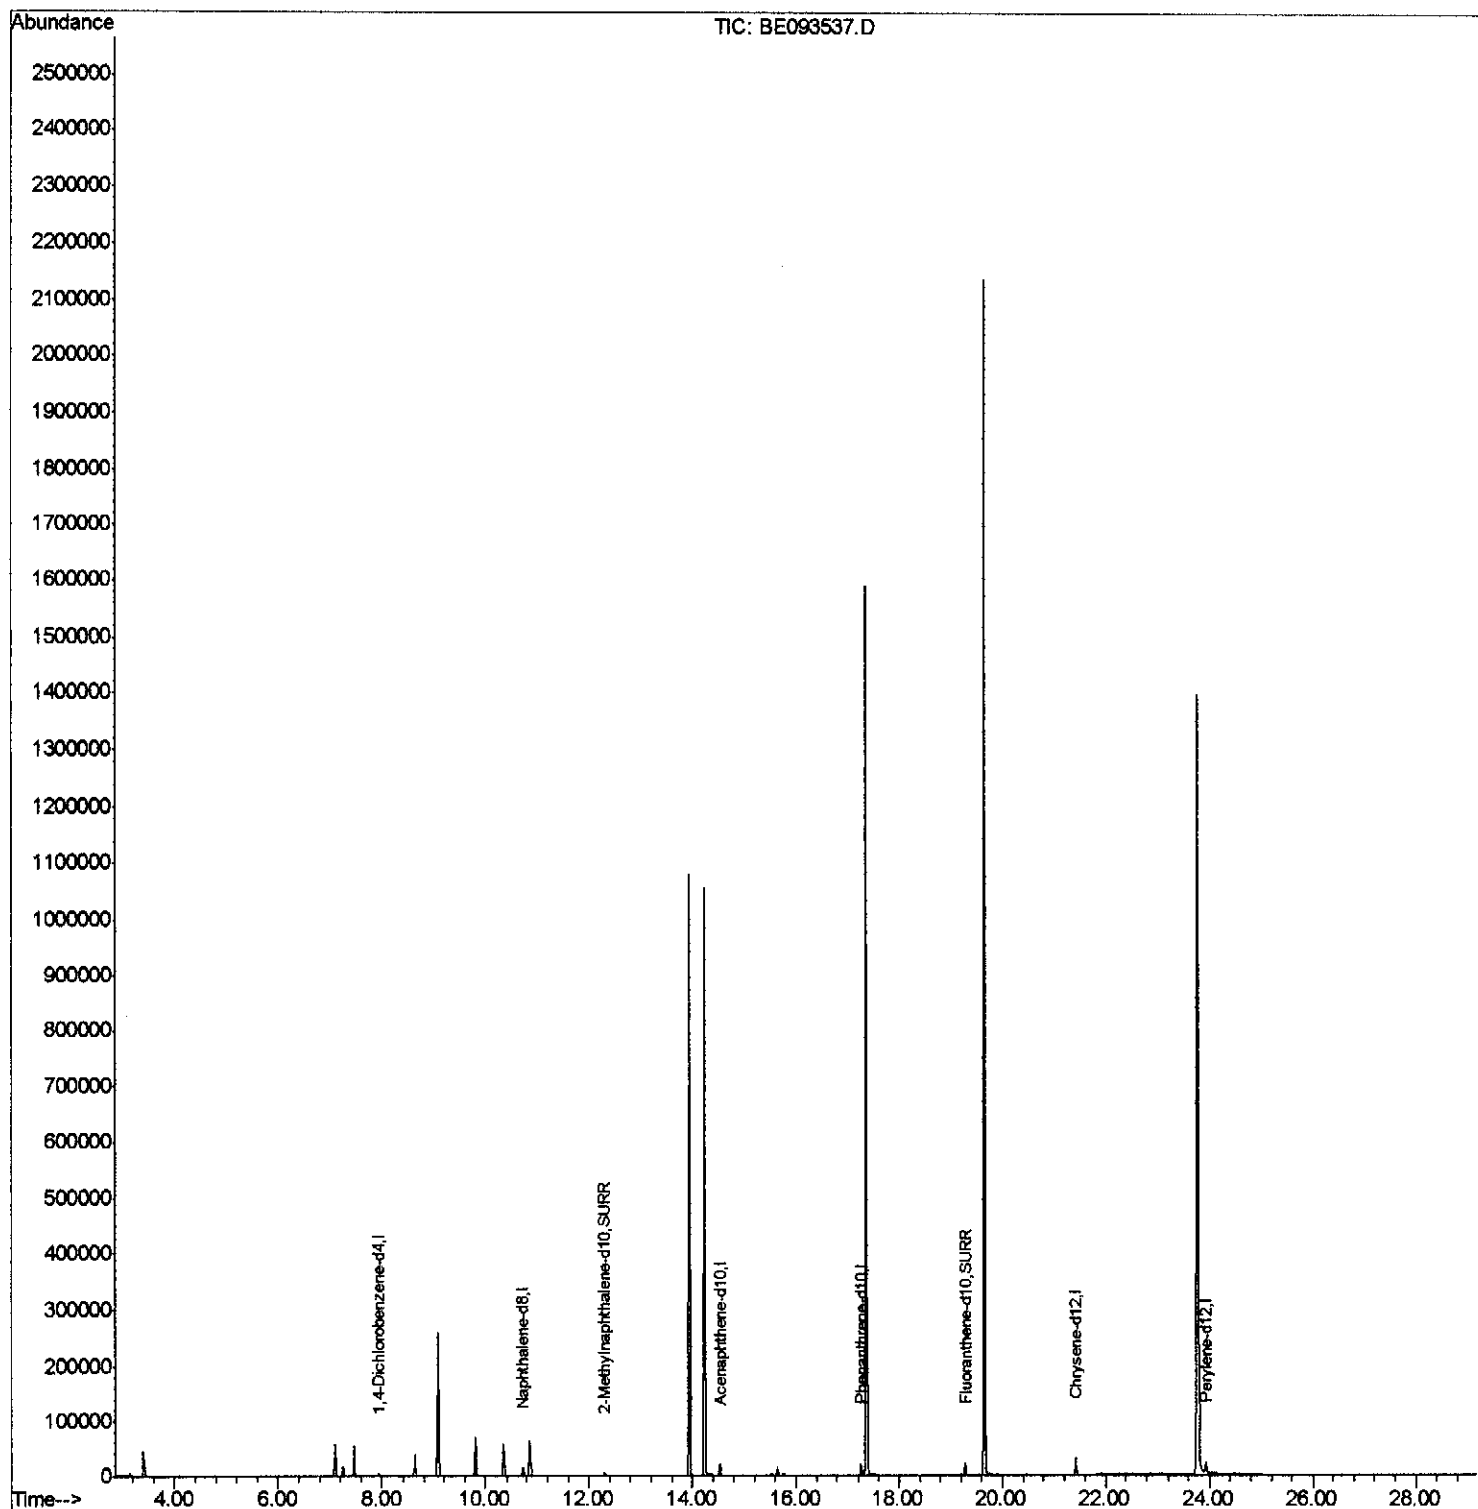




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
Data File : BE093537.D
Acq On : 24 Jul 2017 14:22
Operator : SJ/JU
Sample : PB100766BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK66

Manual Integrations
APPROVED

Sohil
7/25/2017 5:32:30 PM

Quant Time: Jul 24 15:42:16 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 13:14:05 2017
Response via : Initial Calibration

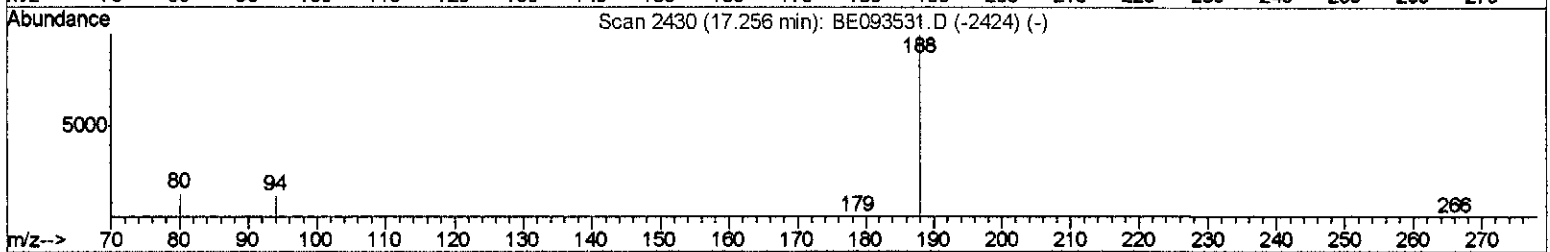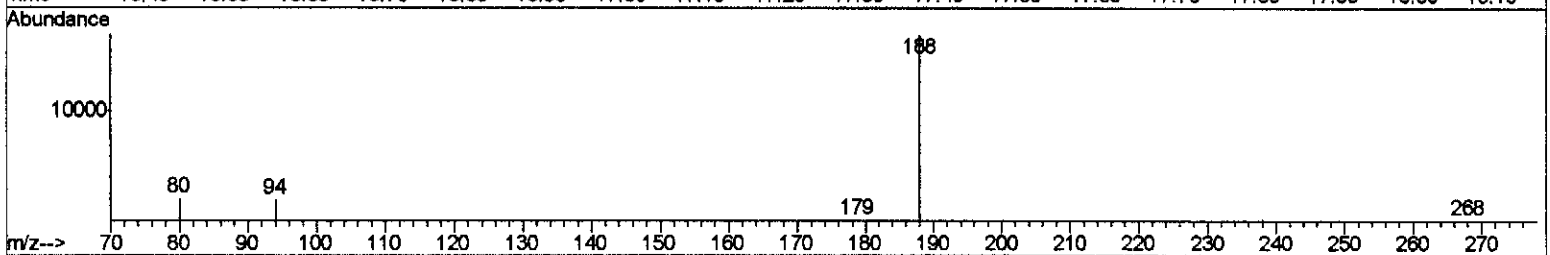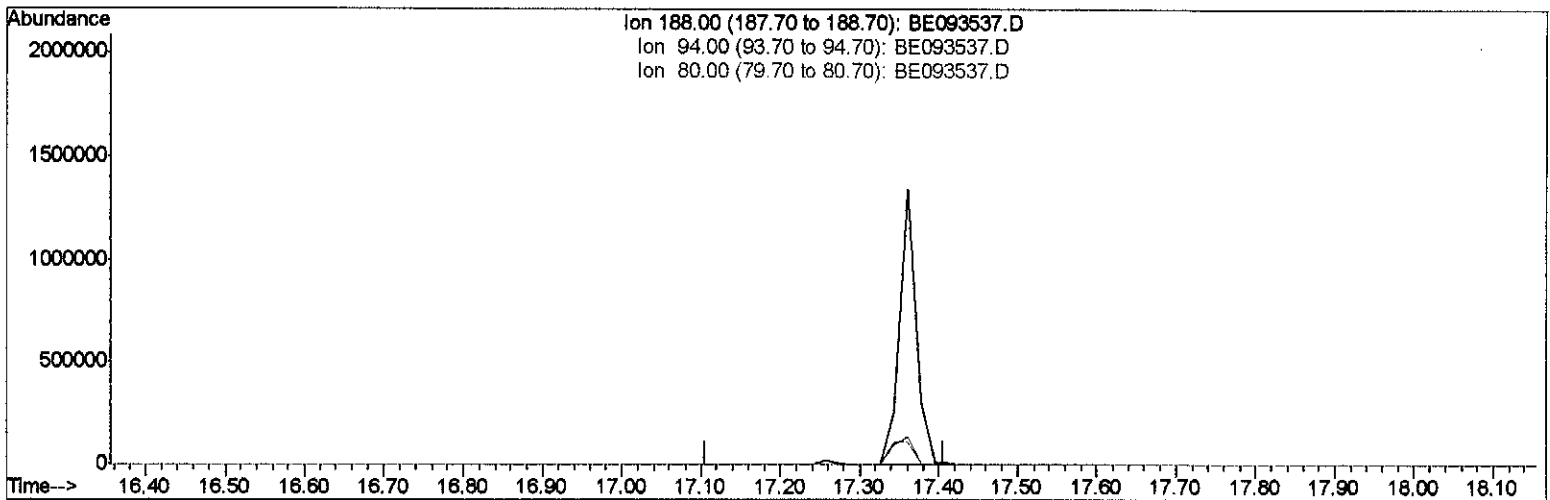

TIC: BE093537.D

(10) Phenanthrene-d10 (I)

17.256min (-17.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
Data File : BE093537.D
Acq On : 24 Jul 2017 14:22
Operator : SJ/JU
Sample : PB100766BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK66

Manual Integrations
APPROVED

Sohil
7/25/2017 5:32:30 PM

Quant Time: Jul 24 15:42:16 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 13:14:05 2017
Response via : Initial Calibration

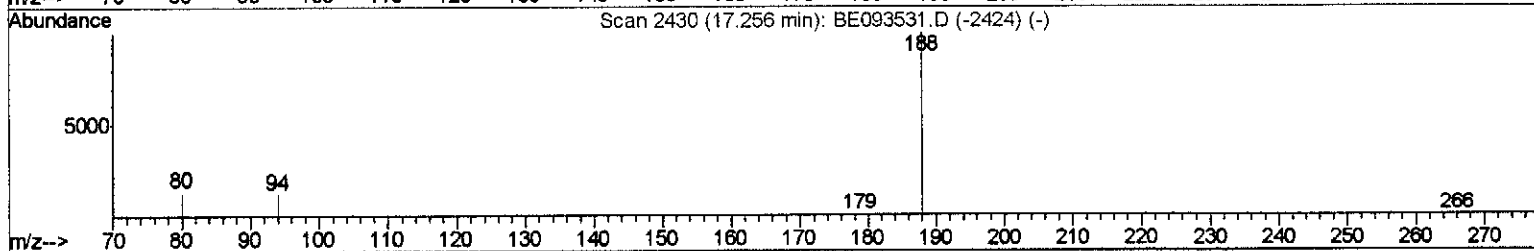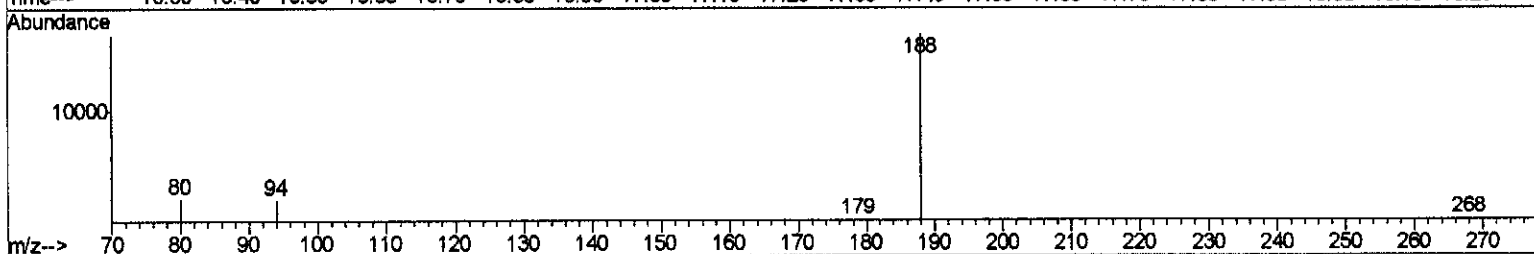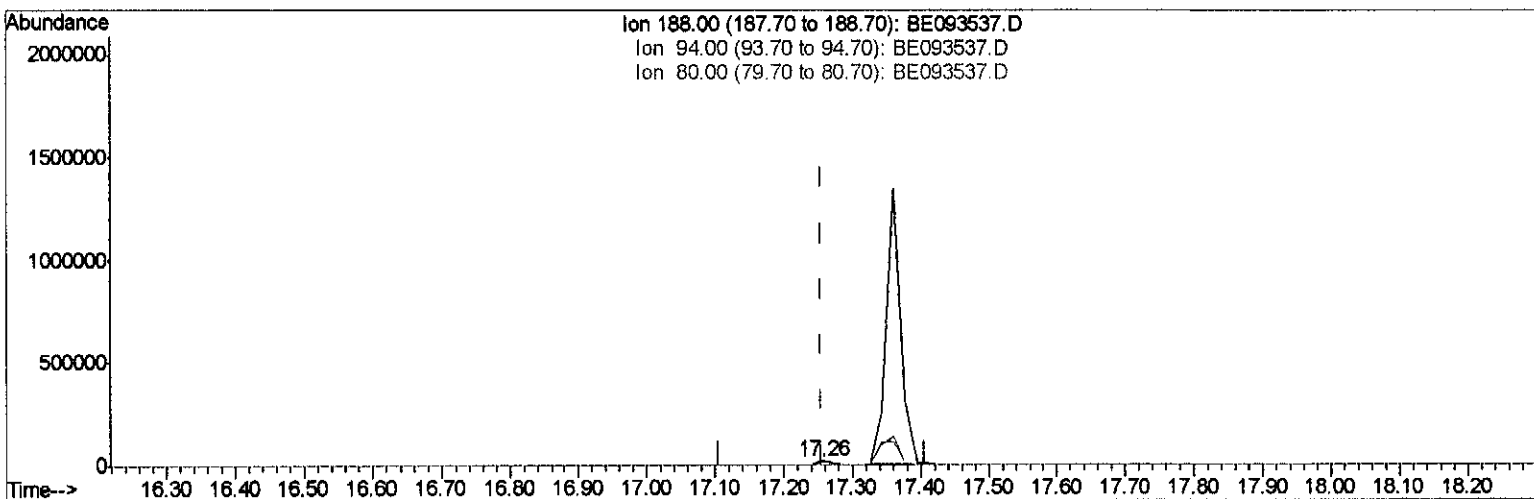

TIC: BE093537.D

(10) Phenanthrene-d10 (I)

17.256min (-0.000) 0.40ng/ul m

response 27349

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.42
80.00	11.80	11.98
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
 Data File : BE093537.D
 Acq On : 24 Jul 2017 14:22
 Operator : SJ/JU
 Sample : PB100766BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK66

Manual Integrations
 APPROVED

Sohil
 7/25/2017 5:32:30 PM

Quant Time: Jul 24 15:44:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 13:14:05 2017
 Response via : Initial Calibration

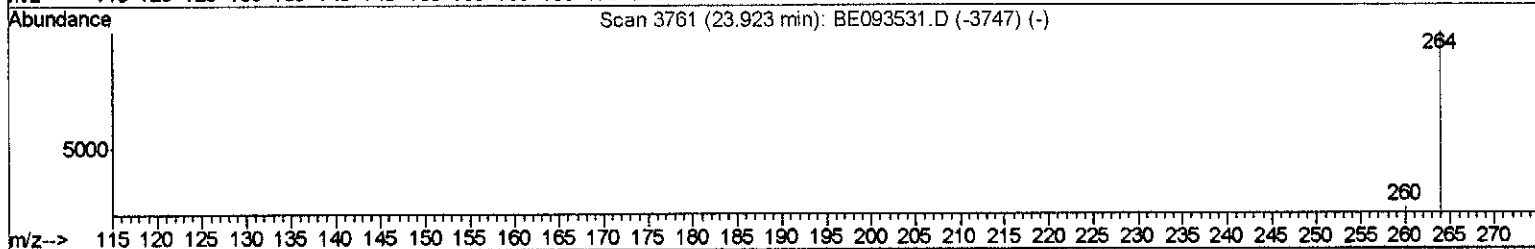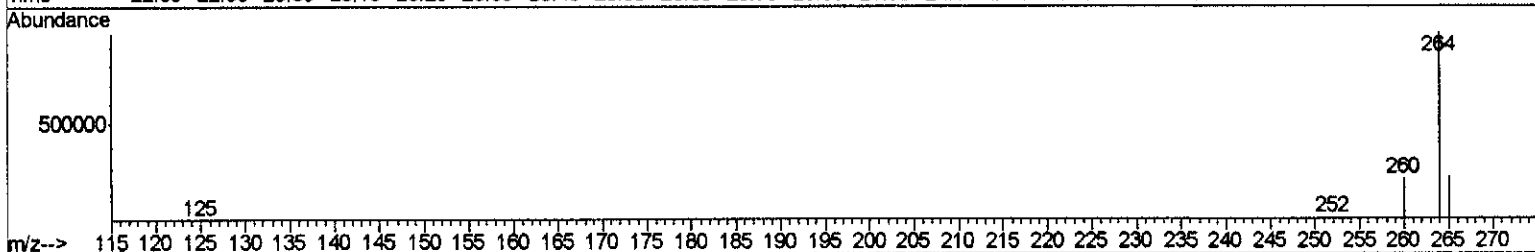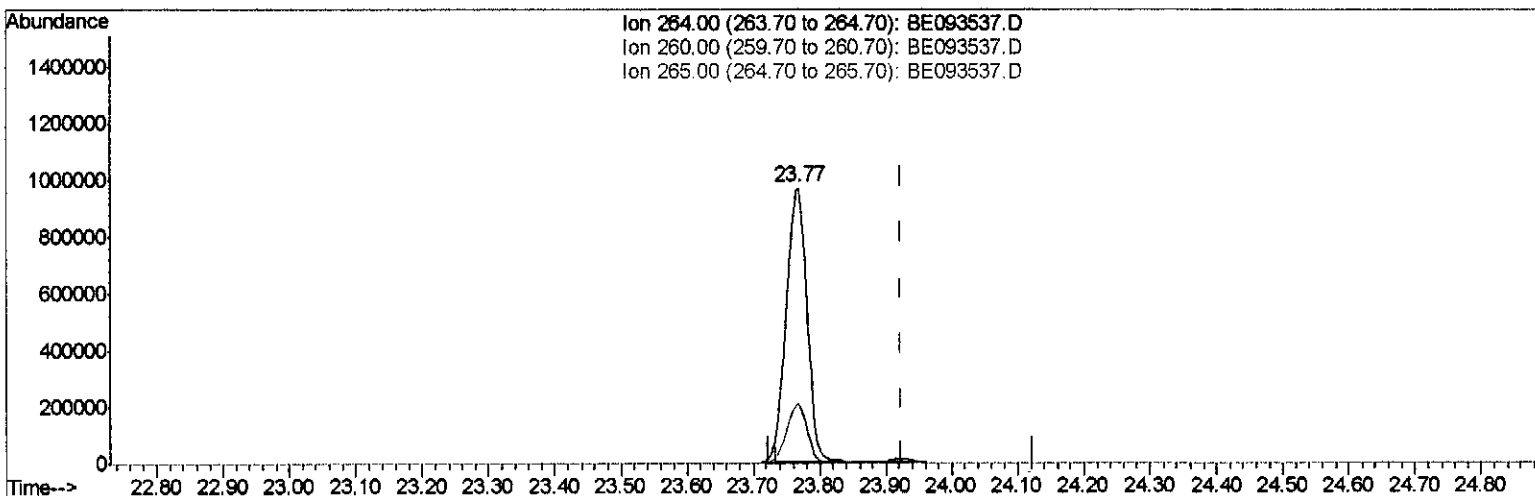

TIC: BE093537.D

(20) Perylene-d12 (I)

23.768min (-0.155) 0.40ng/ui

response 2060303

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.17#
265.00	103.50	21.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
 Data File : BE093537.D
 Acq On : 24 Jul 2017 14:22
 Operator : SJ/JU
 Sample : PB100766BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK66

Manual Integrations
 APPROVED

Sohil
 7/25/2017 5:32:30 PM

Quant Time: Jul 24 15:44:15 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 13:14:05 2017
 Response via : Initial Calibration

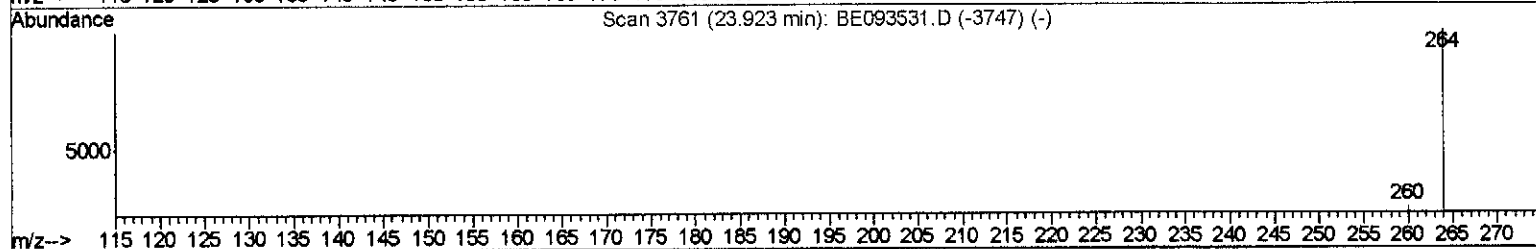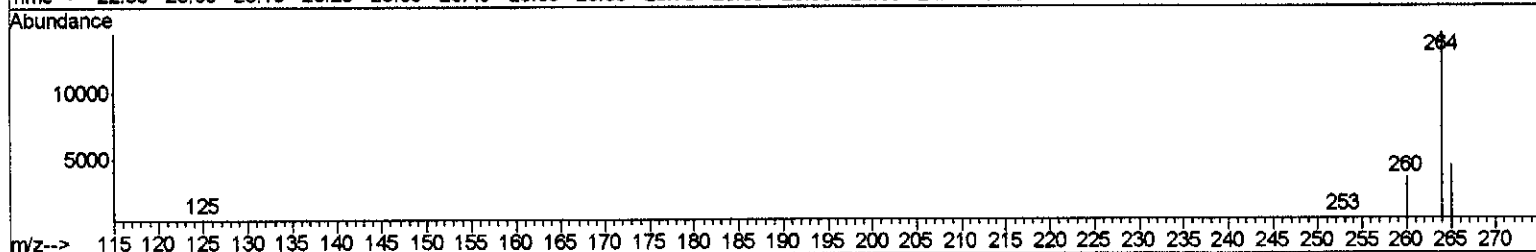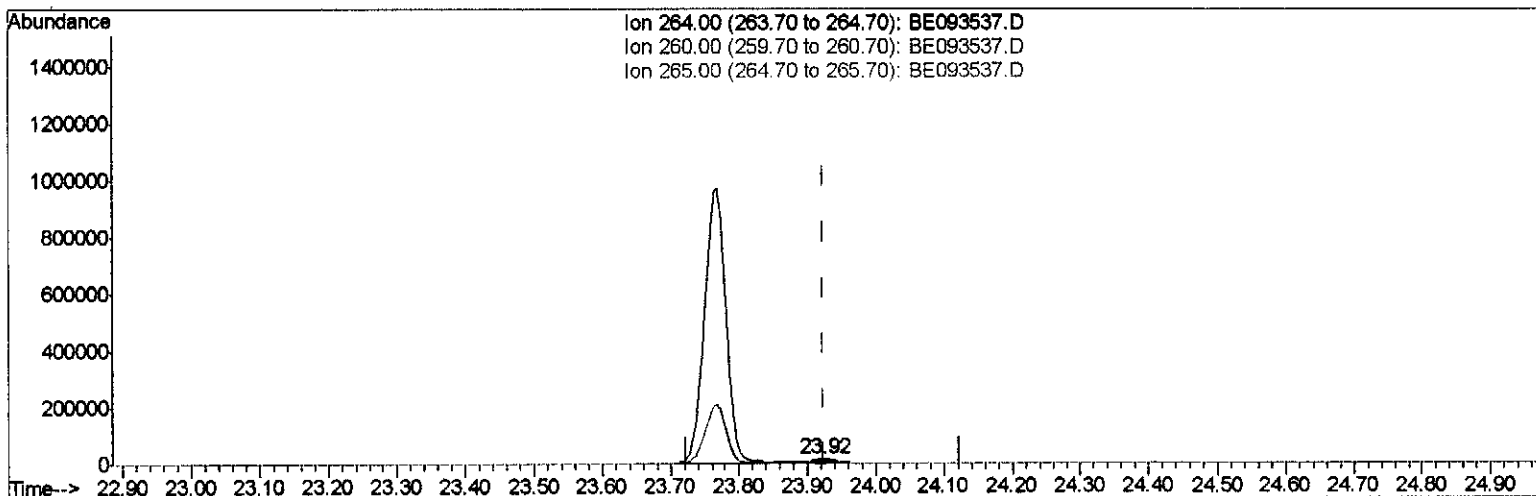

(20) Perylene-d12 (I)

23.923min (-0.000) 0.40ng/ul m

response 24380

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.32#
265.00	103.50	30.21#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
Data File : BE093537.D
Acq On : 24 Jul 2017 14:22
Operator : SJ/JU
Sample : PB100766BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK66

Manual Integrations
APPROVED

Sohil
7/25/2017 5:32:30 PM

Quant Time: Jul 24 15:45:23 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 13:14:05 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	3111	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16164	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	10987	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	27349m>	0.40	ng/ul	>0.00
16) Chrysene-d12	21.42	240	29872	0.40	ng/ul	0.00
20) Perylene-d12	23.92	264	24380m>	0.40	ng/ul	>0.00

July 8/8/17
July 8/8/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.30	152	8140	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	26268	0.30	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed