

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
 Data File : BE093545.D
 Acq On : 24 Jul 2017 19:18
 Operator : SJ/JU
 Sample : I4214-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0B76

Manual Integrations
 APPROVED

Sohil
 7/25/2017 5:33:04 PM

Quant Time: Jul 25 02:25:19 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 18:07:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	3012	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16246	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	11234	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	28241m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	30232	0.40	ng/ul	0.00
20) Perylene-d12	23.92	264	26439m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	8343	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	29079	0.33	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.77	128	1791	0.045	ng/ul#	93
15) Fluoranthene	19.31	202	2249	0.023	ng/ul	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072417\
Data File : BE093545.D
Acq On : 24 Jul 2017 19:18
Operator : SJ/JU
Sample : I4214-03
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
C0B76

Manual Integrations
APPROVED

Sohil
7/25/2017 5:33:04 PM

Quant Time: Jul 25 02:25:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 18:07:15 2017
Response via : Initial Calibration

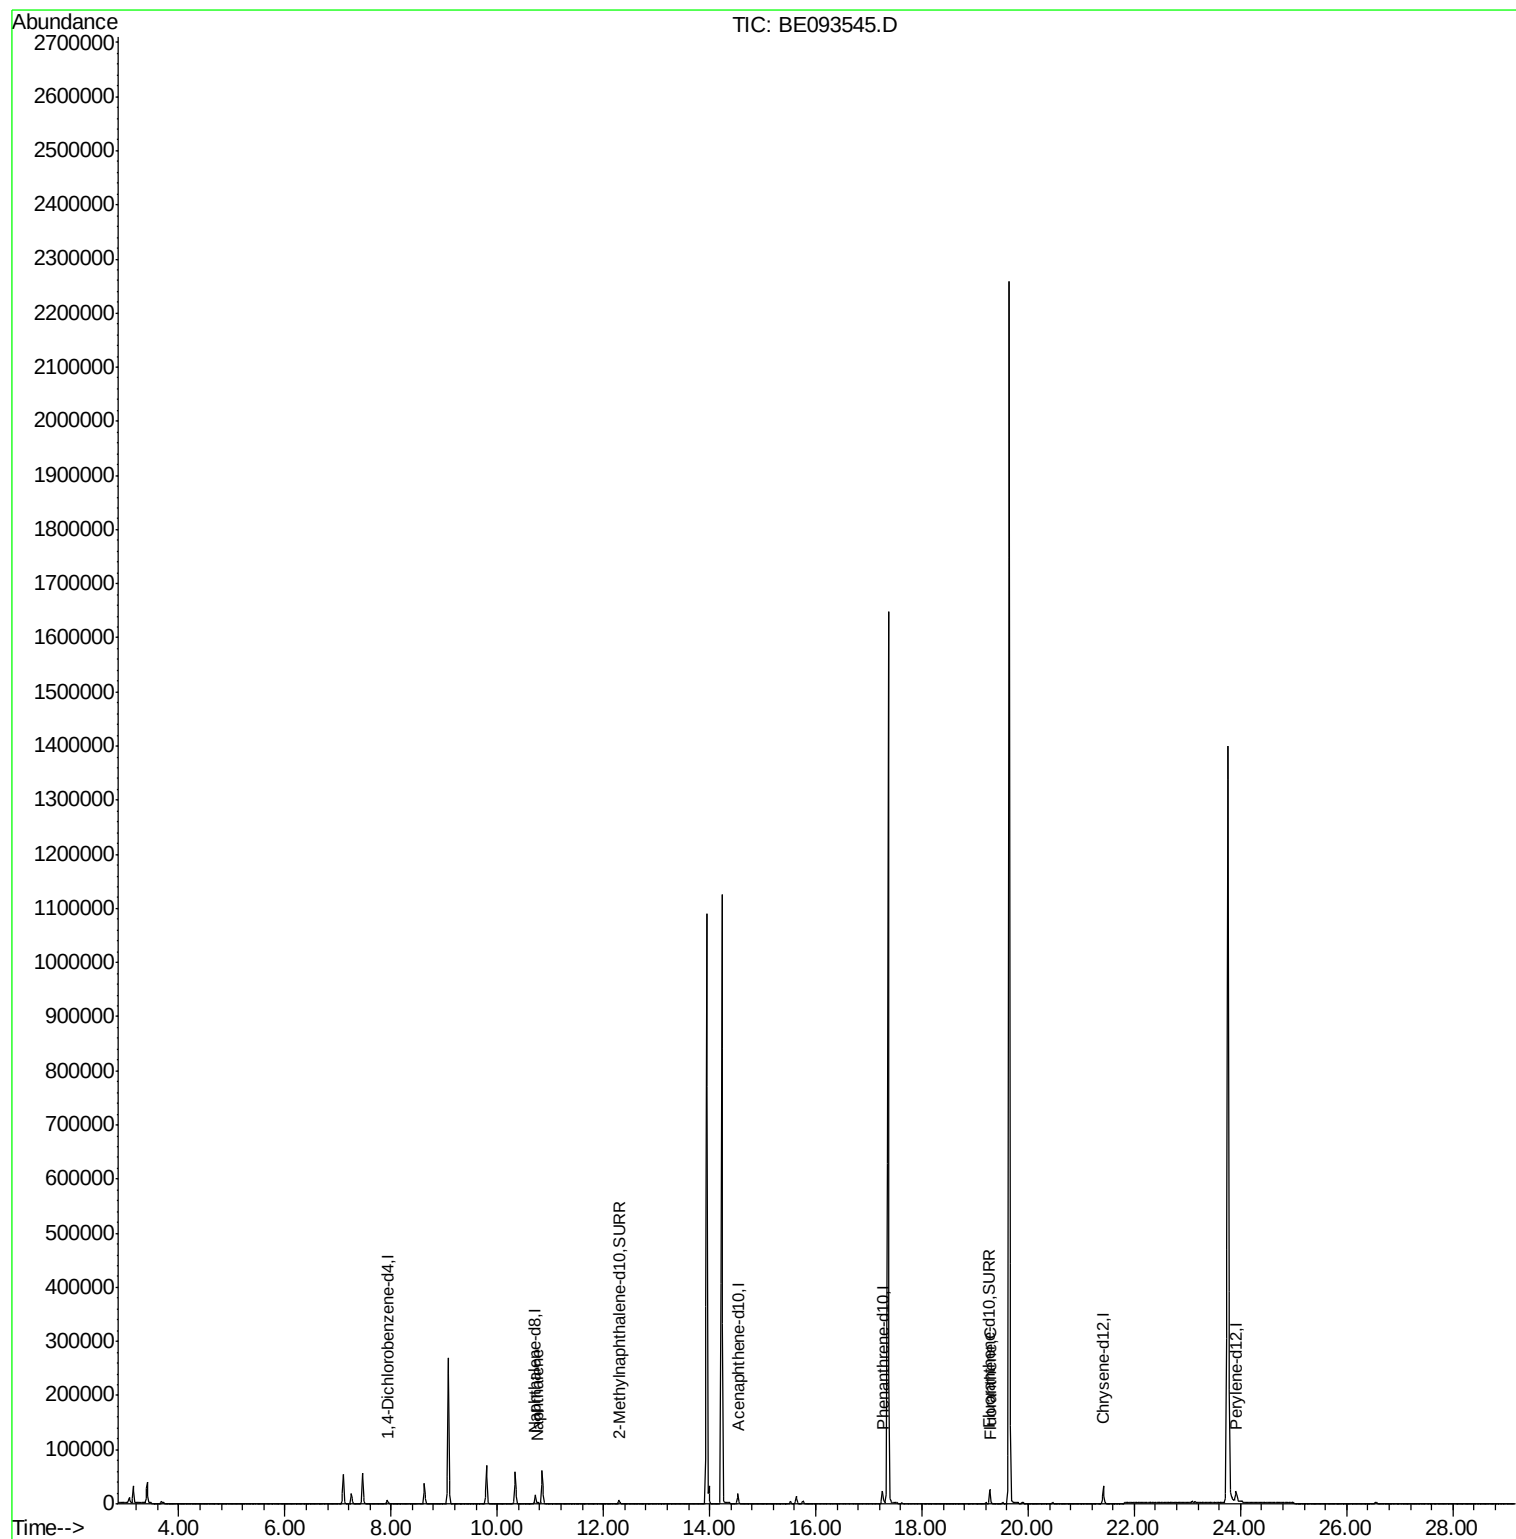

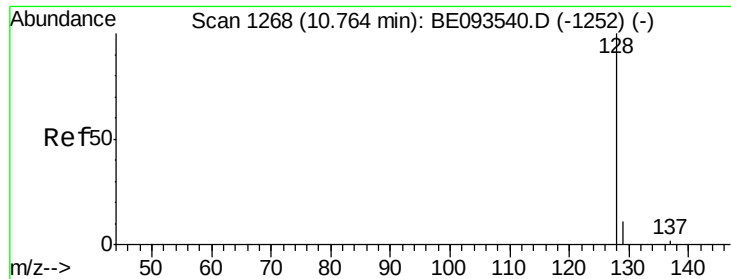

#3

Naphthalene

Concen: 0.045 ng/ul

RT: 10.77 min Scan# 1268

Delta R.T. 0.00 min

Lab File: BE093545.D

Acq: 24 Jul 2017 19:18

Instrument :

BNA_E





ClientSampled :

C0B76

Tgt Ion:	128	Resp:	1791
Ion Ratio	Lower	Upper	
128	100		
129	15.5	11.3	16.9
127	0.0	4.0	6.0#

Manual Integrations
APPROVED

Sohil
7/25/2017 5:33:04 PM

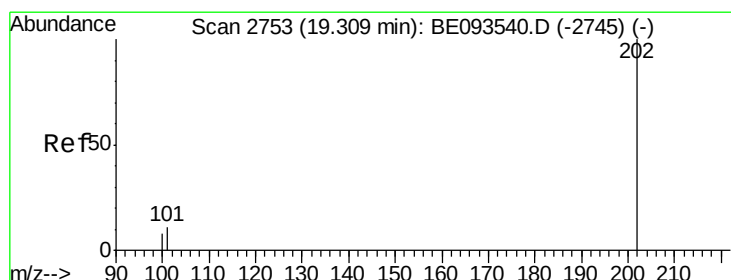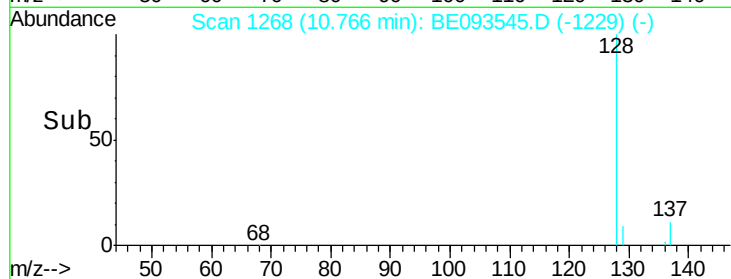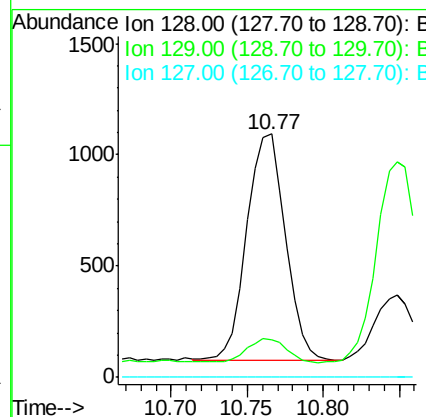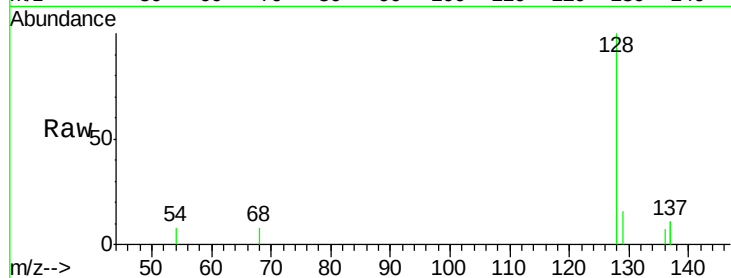

#15

Fluoranthene

Concen: 0.023 ng/ul

RT: 19.31 min Scan# 2753

Delta R.T. -0.00 min

Lab File: BE093545.D

Acq: 24 Jul 2017 19:18

Tgt Ion:	202	Resp:	2249
Ion Ratio	Lower	Upper	
202	100		
101	14.3	0.0	30.3
100	12.5	0.0	39.5

