

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE072418\
 Data File : BE097094.D
 Acq On : 25 Jul 2018 5:42
 Operator : SJ/JU
 Sample : J4073-04DL 2X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE109D2-071618DL

Quant Time: Jul 25 07:40:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE072418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 24 13:24:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1419	0.40	ng	0.00
7) Naphthalene-d8	10.15	136	6780	0.40	ng	0.00
13) Acenaphthene-d10	14.01	164	3988	0.40	ng	0.00
19) Phenanthrene-d10	16.77	188	11728	0.40	ng	0.00
27) Chrysene-d12	20.97	240	12841	0.40	ng	-0.01
34) Perylene-d12	23.21	264	12436	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.05	112	174	0.04	ng	0.00
5) Phenol-d6	6.60	99	187	0.03	ng	0.00
8) Nitrobenzene-d5	8.53	82	1055	0.18	ng	0.00
11) 2-Methylnaphthalene-d10	11.73	152	1665	0.16	ng	0.00
14) 2,4,6-Tribromophenol	15.52	330	160	0.12	ng	0.00
15) 2-Fluorobiphenyl	12.63	172	3255	0.24	ng	0.00
25) Fluoranthene-d10	18.81	212	24206	0.21	ng	0.00
29) Terphenyl-d14	19.42	244	7066	0.29	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.09	88	3306	1.466	ng	Qvalue # 90
22) Pentachlorophenol	16.44	266	13	0.044	ng	99
32) Bis(2-ethylhexyl)phthalate	20.92	149	162895	3.204	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE072418\
Data File : BE097094.D
Acq On : 25 Jul 2018 5:42
Operator : SJ/JU
Sample : J4073-04DL 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE109D2-071618DL

Quant Time: Jul 25 07:40:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE072418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 24 13:24:10 2018
Response via : Initial Calibration

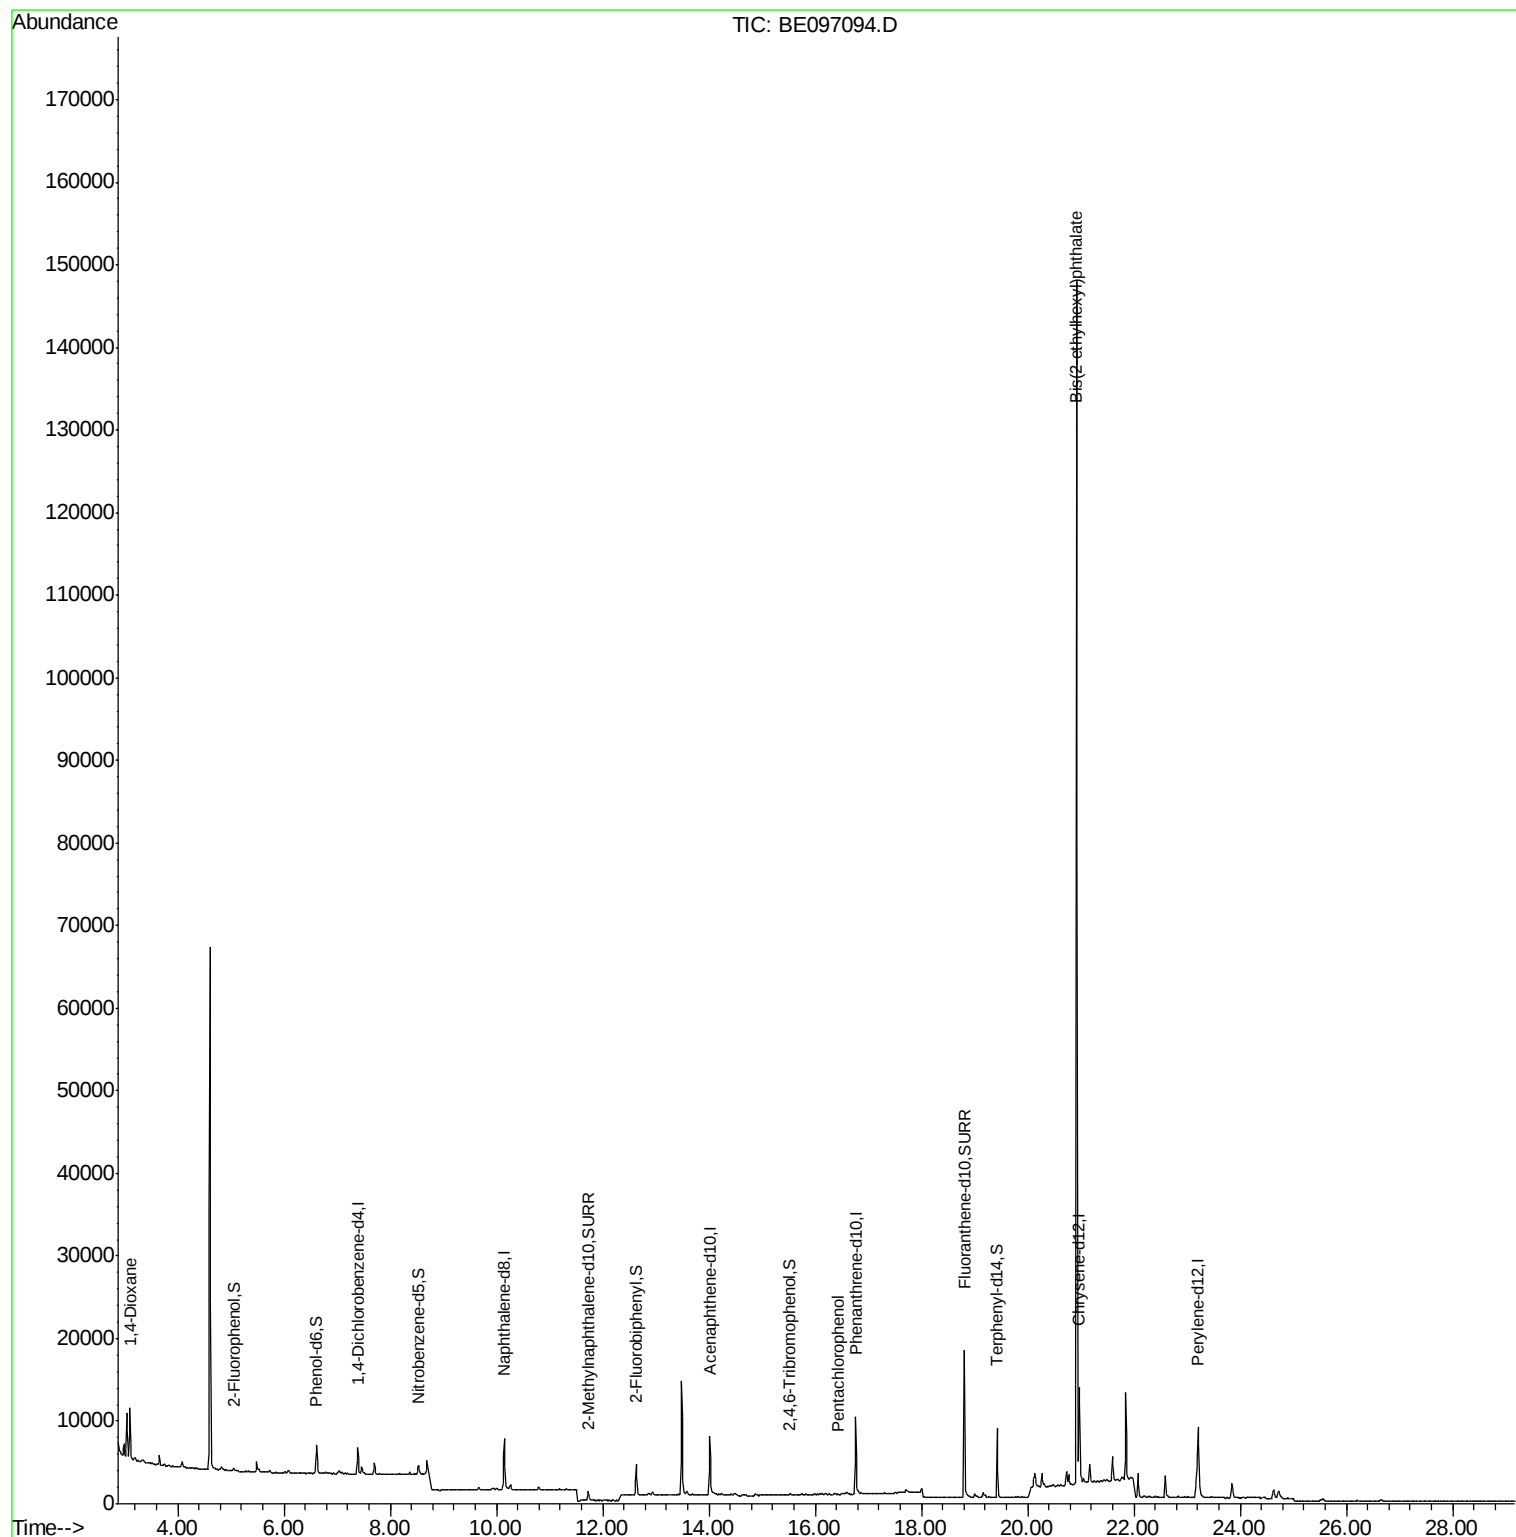



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.39 min Scan# 393

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL


Tot Ion:152 Resp: 1419

Ion Ratio Lower Upper

152 100

150 153.8 117.2 175.8




115 71.7 57.0 85.6

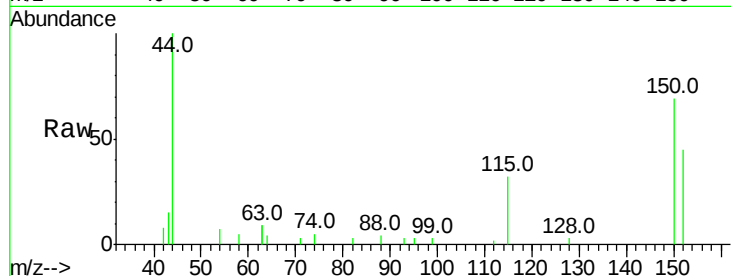

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

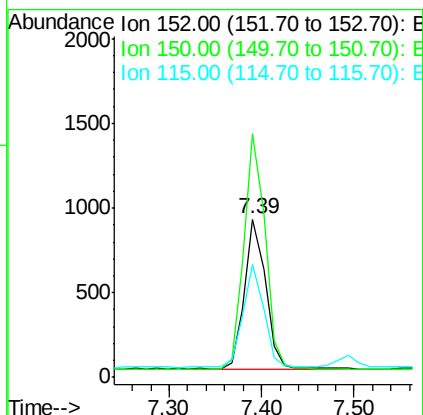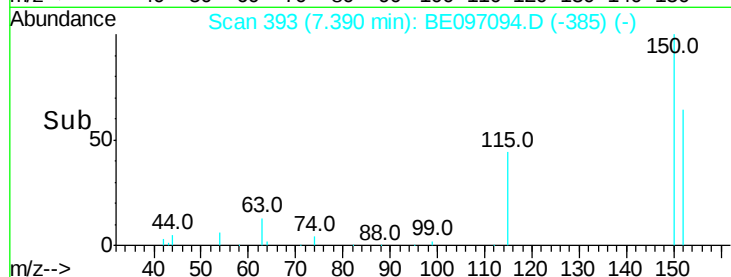

#2

1,4-Dioxane

Concen: 1.466 ng

RT: 3.09 min Scan# 20

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42


Tgt Ion: 88 Resp: 3306

Ion Ratio Lower Upper

88 100

58 84.6 63.2 94.8



43 40.2 41.2 61.8#




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

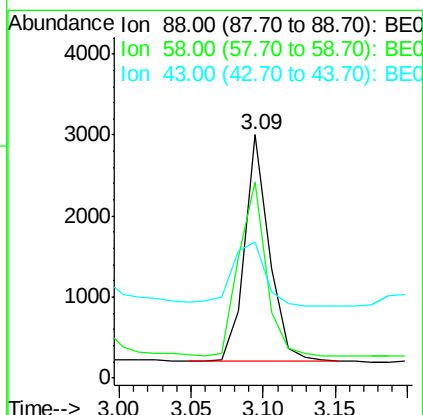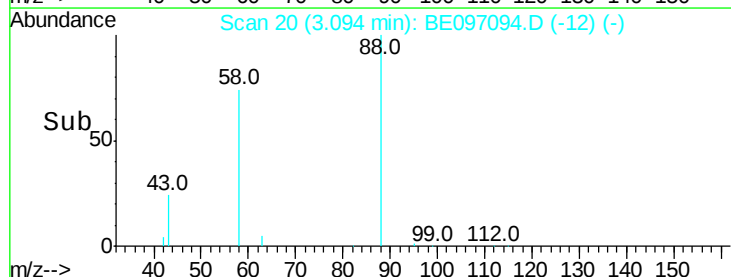

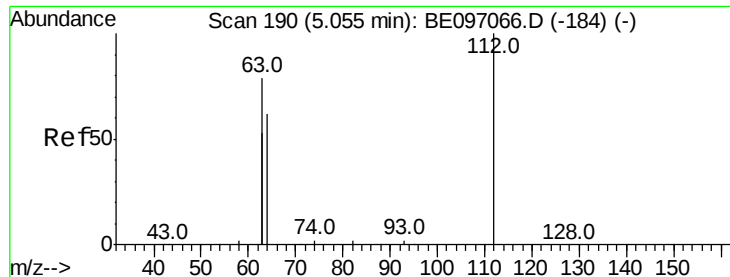

#4

2-Fluorophenol

Concen: 0.044 ng

RT: 5.05 min Scan# 190

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL


Tot Ion:112 Resp: 174

Ion Ratio Lower Upper

112 100

64 87.4 60.1 90.1

63 152.3 116.8 175.2



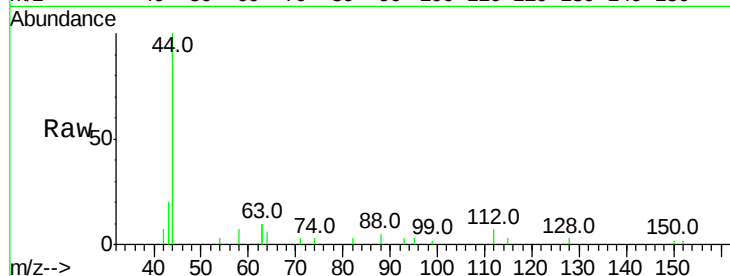


Abundance Ion 112.00 (111.70 to 112.70): BE097066.D (-184) (-)

Ion 64.00 (63.70 to 64.70): BE097066.D (-184) (-)

Ion 63.00 (62.70 to 63.70): BE097066.D (-184) (-)

Time-->

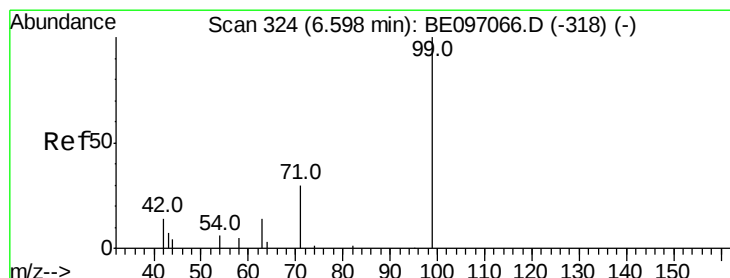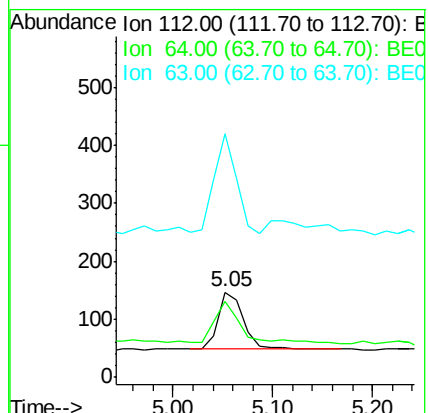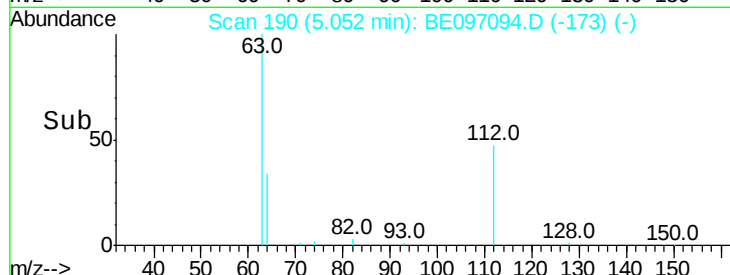

#5

Phenol-d6

Concen: 0.032 ng

RT: 6.60 min Scan# 324

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42


Tgt Ion: 99 Resp: 187

Ion Ratio Lower Upper

99 100

42 107.0 20.2 30.2#

71 75.9 28.4 42.6#


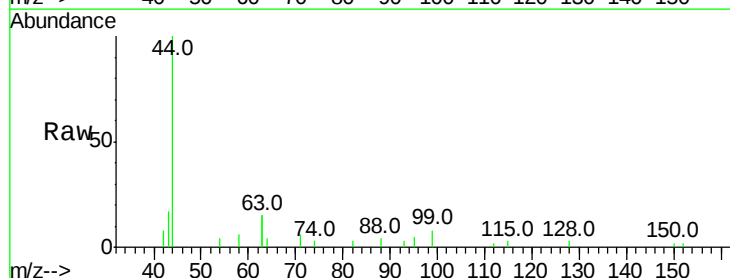



Abundance Ion 99.00 (98.70 to 99.70): BE097066.D (-318) (-)

Ion 42.00 (41.70 to 42.70): BE097066.D (-318) (-)

Ion 71.00 (70.70 to 71.70): BE097066.D (-318) (-)

Time-->

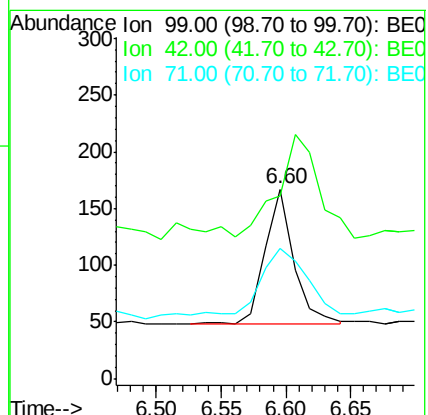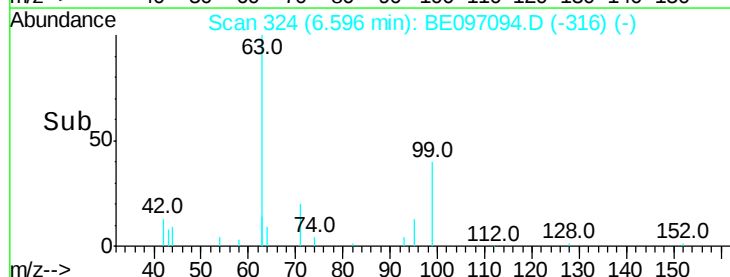

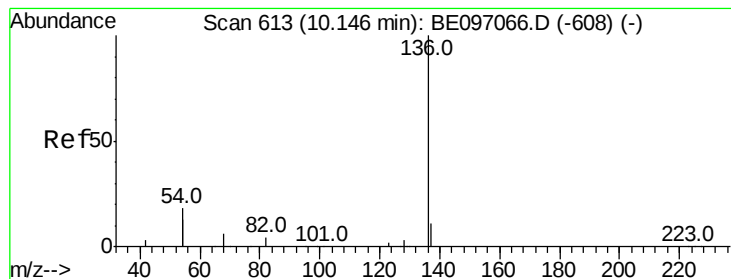

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.15 min Scan# 613

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL

Tot Ion:136 Resp: 6780


Ion Ratio Lower Upper

136 100

137 12.1 9.5 14.3

54 36.6 29.1 43.7

68 7.2 6.2 9.2



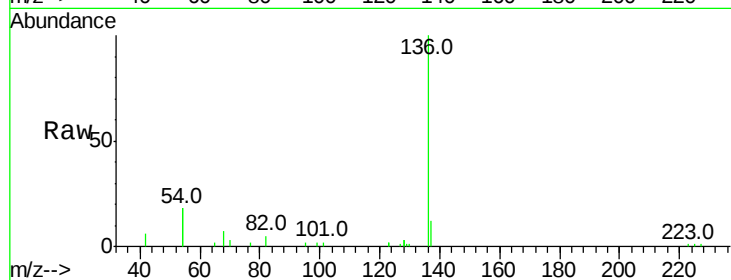


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

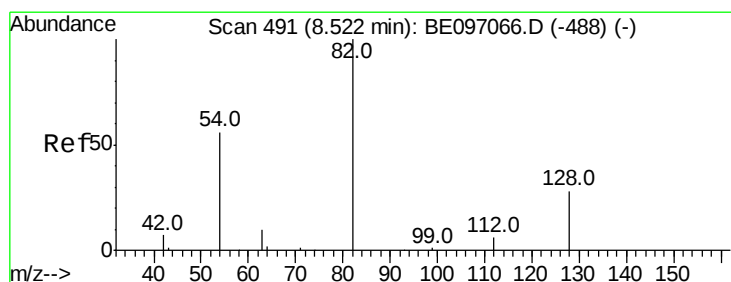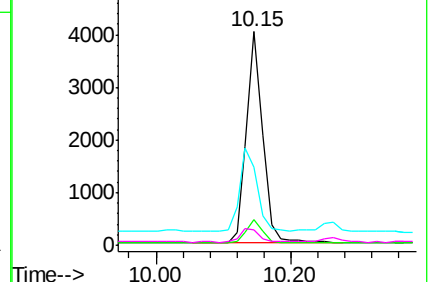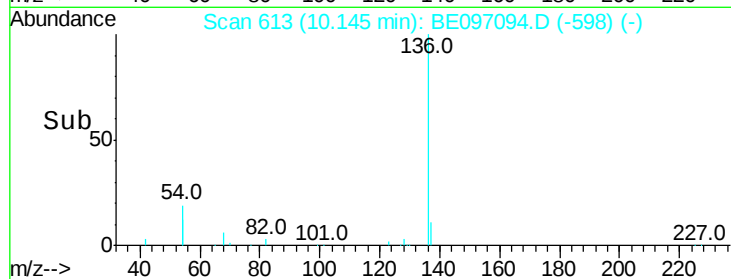

#8

Nitrobenzene-d5

Concen: 0.179 ng

RT: 8.53 min Scan# 492

Delta R.T. 0.01 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42


Tgt Ion: 82 Resp: 1055

Ion Ratio Lower Upper

82 100

128 42.6 24.0 36.0#



54 56.9 40.0 60.0

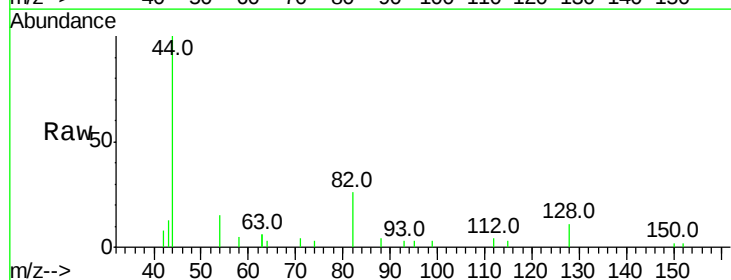


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



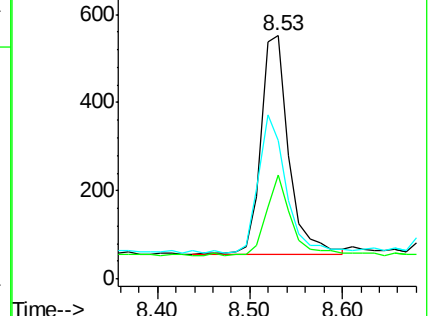
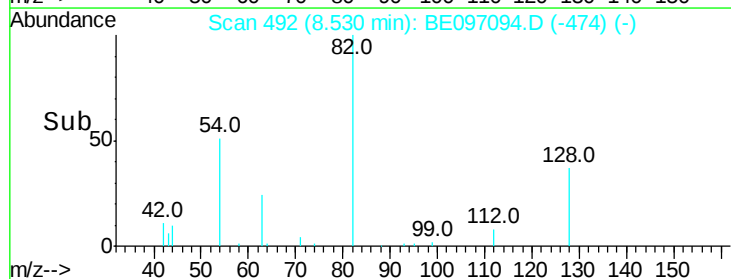


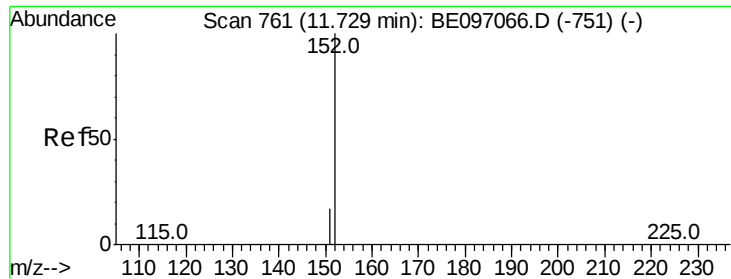

#11
2-Methylnaphthalene-d10
Concen: 0.164 ng
RT: 11.73 min Scan# 761
Delta R.T. -0.00 min
Lab File: BE097094.D
Acq: 25 Jul 2018 5:42




Instrument :
BNA_E
ClientSampleId :
RE109D2-071618DL


Tot Ion:152 Resp: 1665
Ion Ratio Lower Upper
152 100
151 19.7 15.4 23.0

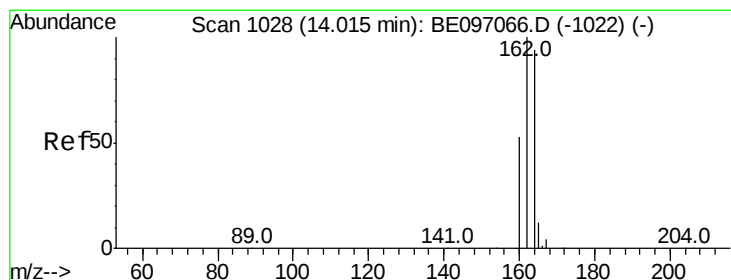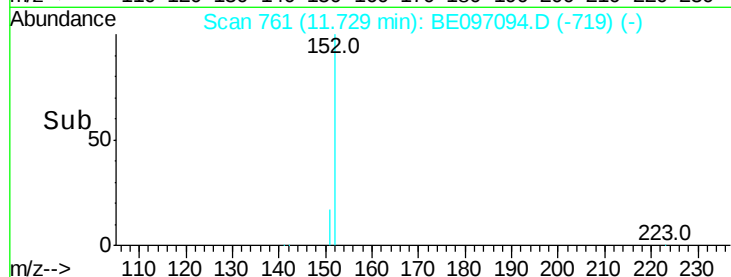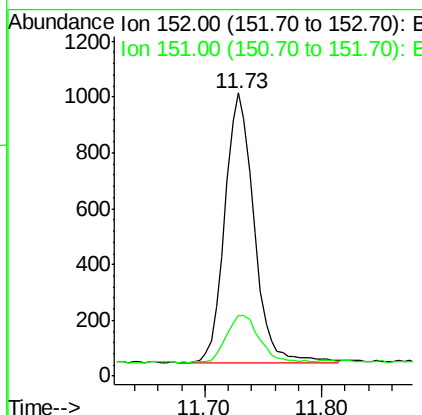

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.01 min Scan# 1028
Delta R.T. -0.00 min
Lab File: BE097094.D
Acq: 25 Jul 2018 5:42

Tgt Ion:164 Resp: 3988
Ion Ratio Lower Upper
164 100
162 106.7 83.1 124.7
160 55.0 37.1 55.7


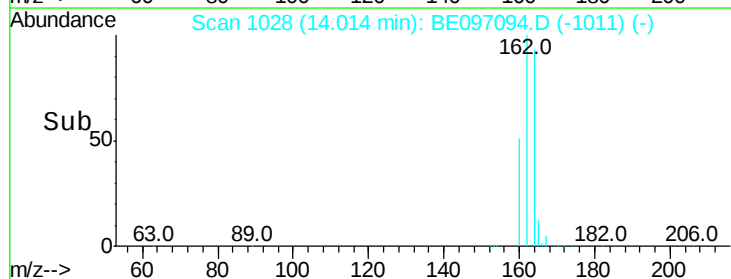
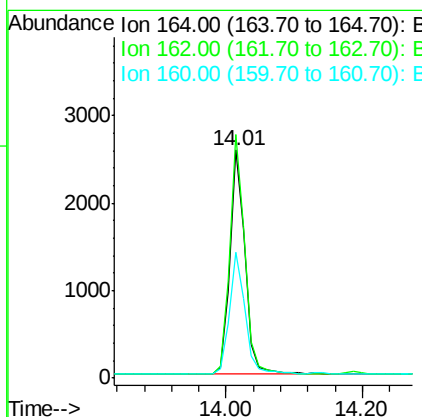
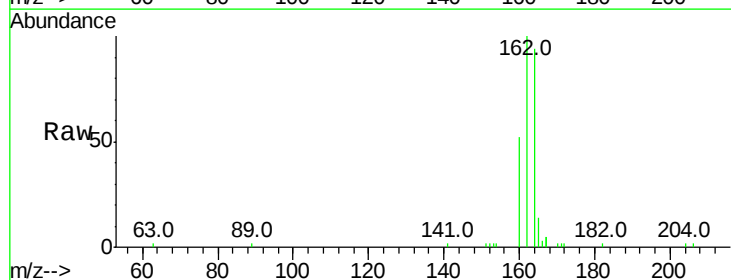


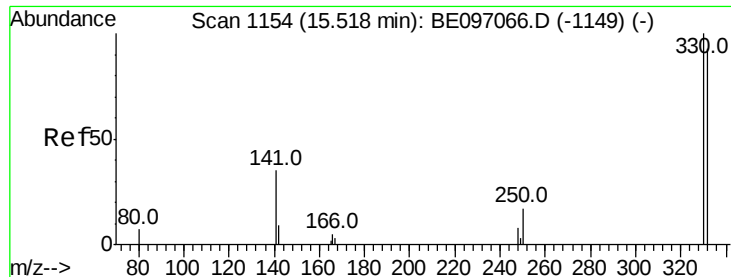

#14
 2,4,6-Tribromophenol
 Concen: 0.122 ng
 RT: 15.52 min Scan# 1154
 Delta R.T. 0.00 min
 Lab File: BE097094.D
 Acq: 25 Jul 2018 5:42




Instrument :
 BNA_E
 ClientSampleId :
 RE109D2-071618DL


Tot Ion:330 Resp: 160
 Ion Ratio Lower Upper
 330 100
 332 98.8 152.7 229.1#
 141 38.8 33.7 50.5

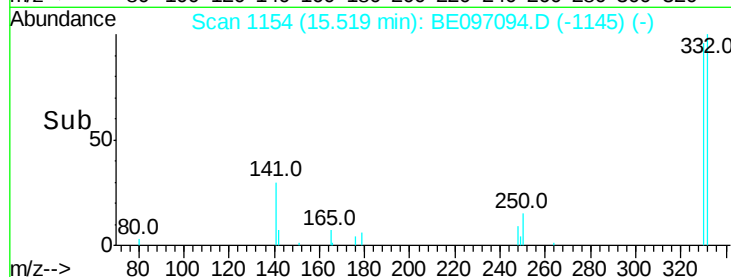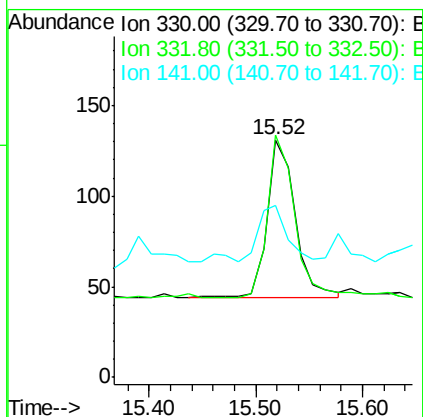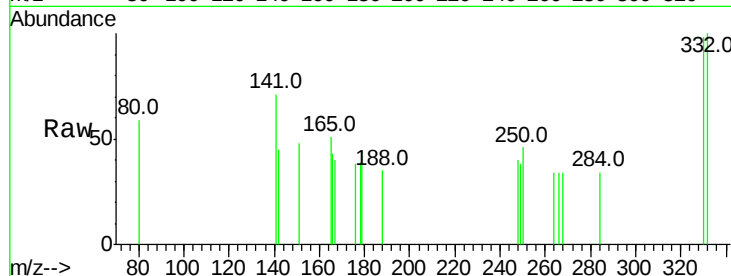

#15
 2-Fluorobiphenyl
 Concen: 0.236 ng
 RT: 12.63 min Scan# 908
 Delta R.T. -0.00 min
 Lab File: BE097094.D
 Acq: 25 Jul 2018 5:42

Tgt Ion:172 Resp: 3255
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.9 44.9
 170 25.2 21.8 32.8

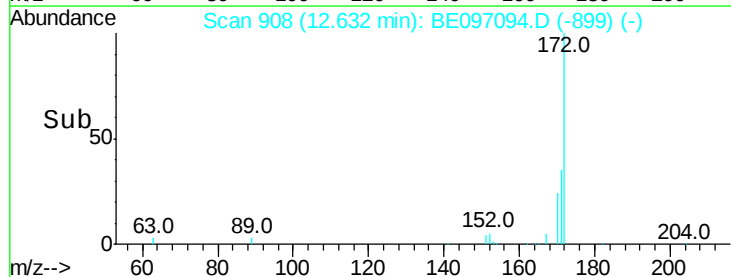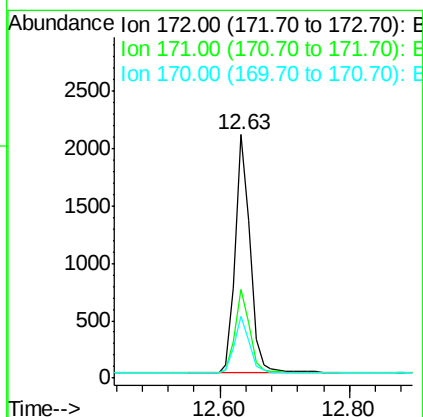

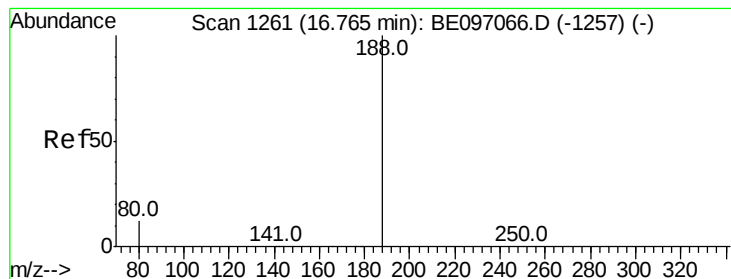

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.77 min Scan# 1261

Delta R.T. 0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL


Tot Ion:188 Resp: 11728

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 11.1 3.6 5.4#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

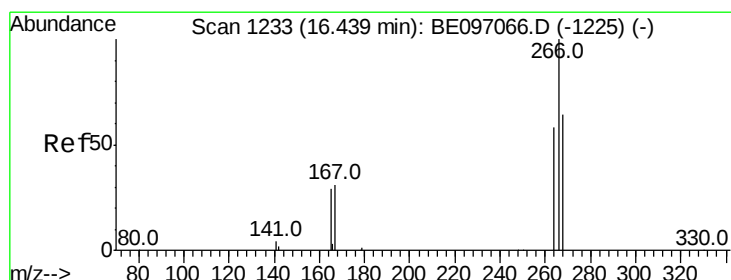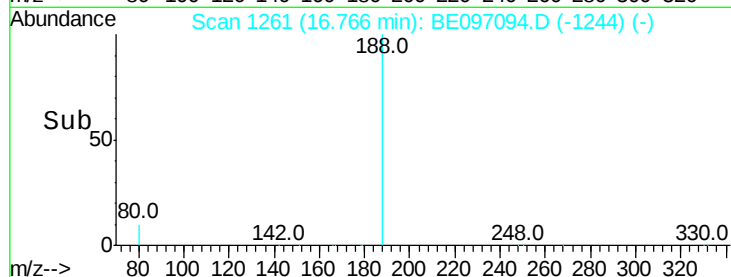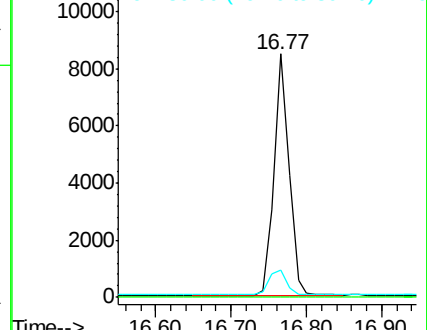

#22

Pentachlorophenol

Concen: 0.044 ng

RT: 16.44 min Scan# 1233

Delta R.T. 0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42


Tgt Ion:266 Resp: 13

Ion Ratio Lower Upper

266 100

264 92.3 72.5 108.7



268 92.3 73.8 110.6




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

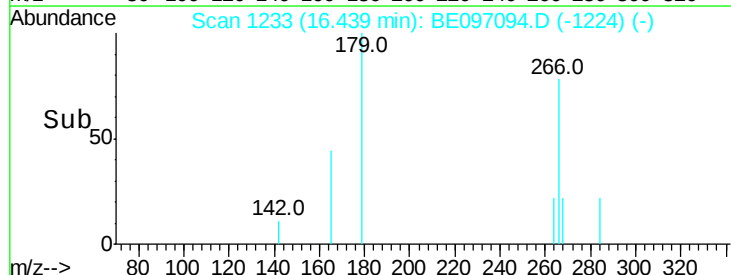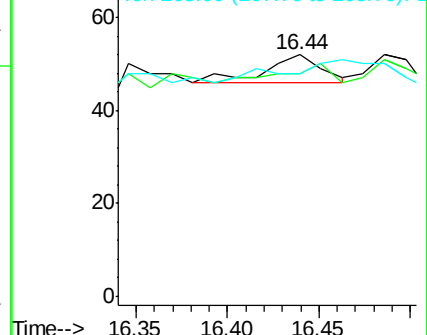

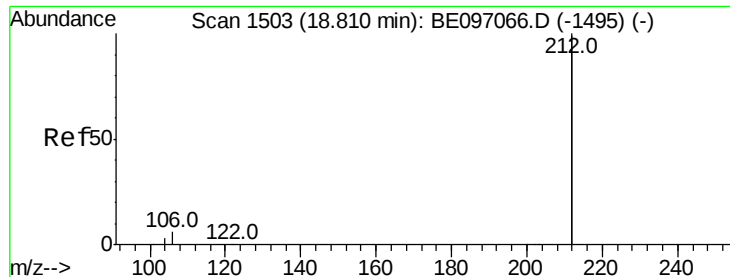

#25

Fluoranthene-d10

Concen: 0.206 ng

RT: 18.81 min Scan# 1503

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL


Tot Ion:212 Resp: 24206

Ion Ratio Lower Upper

212 100

106 3.0 2.8 4.2




104 1.8 1.6 2.4

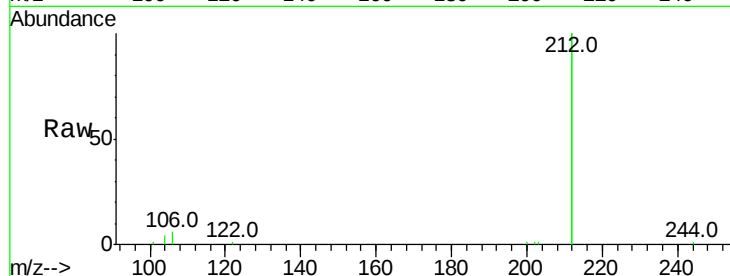

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

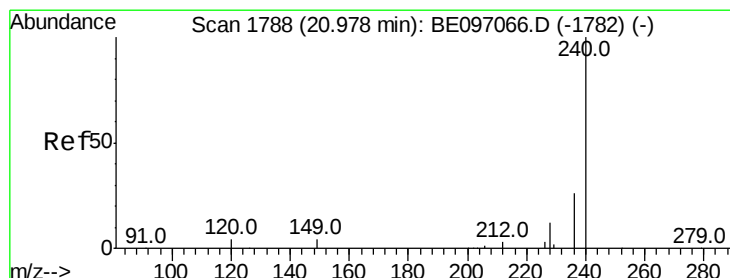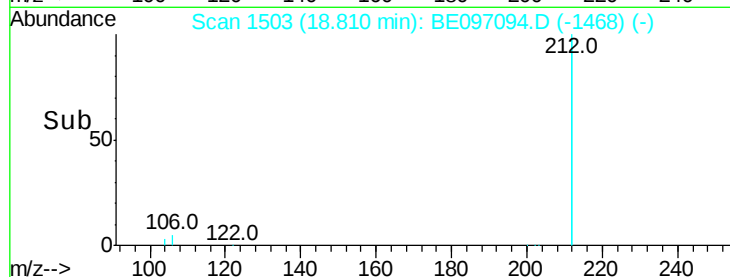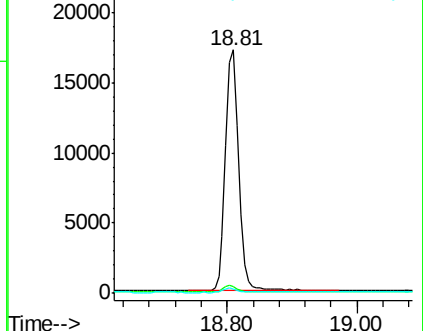

#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.97 min Scan# 1787

Delta R.T. -0.01 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42


Tgt Ion:240 Resp: 12841

Ion Ratio Lower Upper

240 100

120 14.6 5.5 8.3#



236 28.4 20.7 31.1

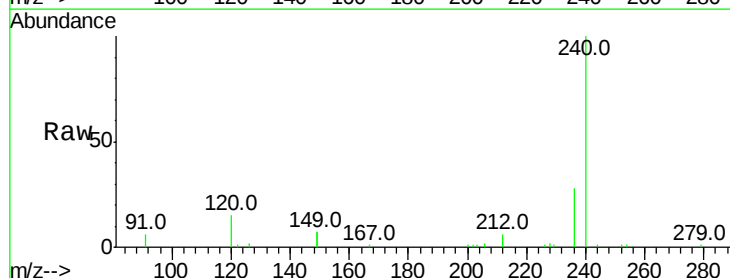


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

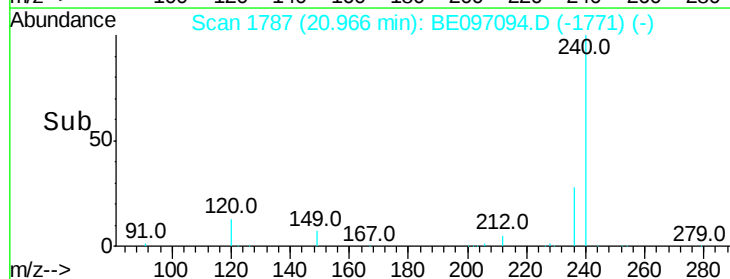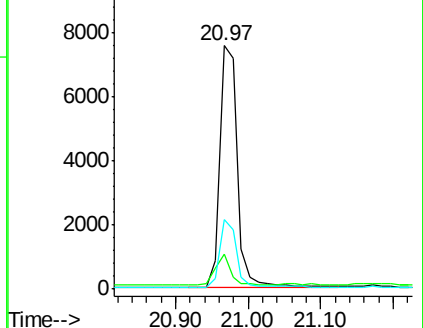

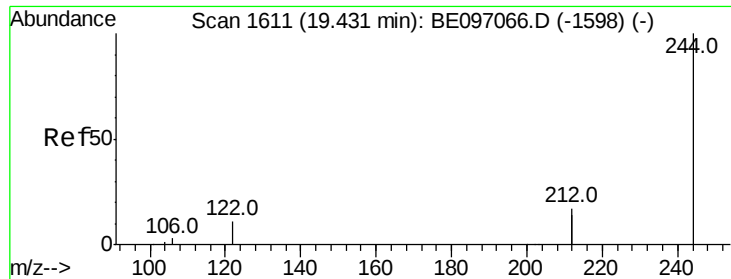

#29

Terphenyl-d14

Concen: 0.286 ng

RT: 19.42 min Scan# 1610

Delta R.T. -0.01 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL





Tot Ion:244 Resp: 7066

Ion Ratio Lower Upper

244 100

212 34.6 25.4 38.0

122 12.1 8.1 12.1#

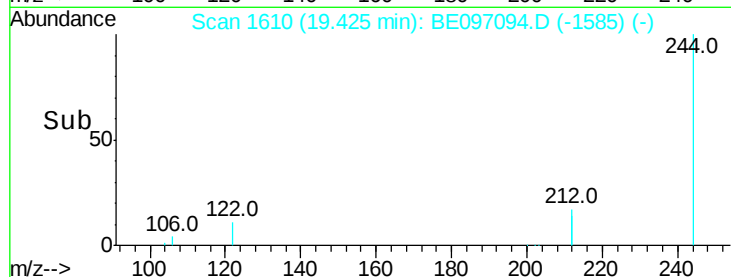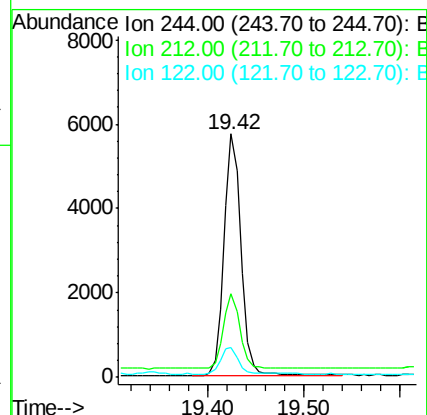

#32

Bis(2-ethylhexyl)phthalate

Concen: 3.204 ng

RT: 20.92 min Scan# 1783

Delta R.T. 0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42




Tgt Ion:149 Resp: 162895




Ion Ratio Lower Upper

149 100

167 6.5 5.4 8.0

279 0.9 0.7 1.1

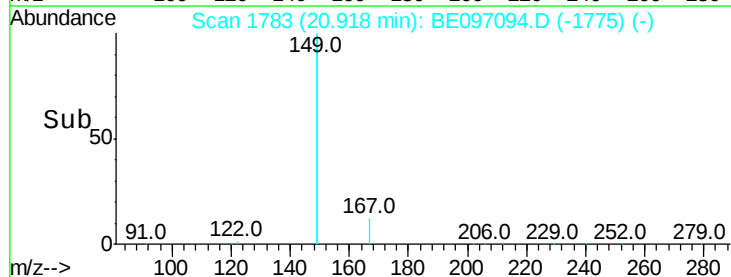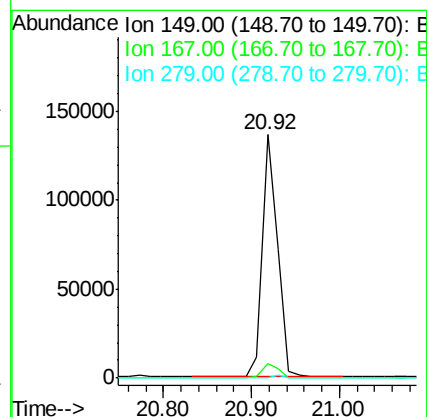

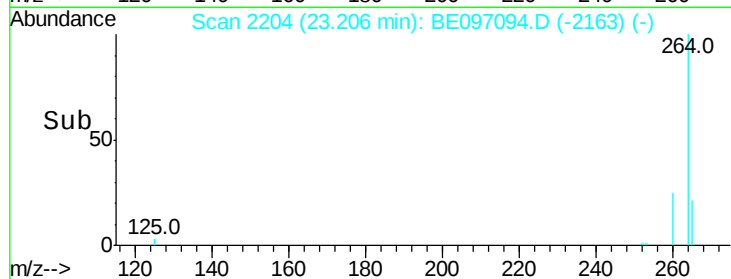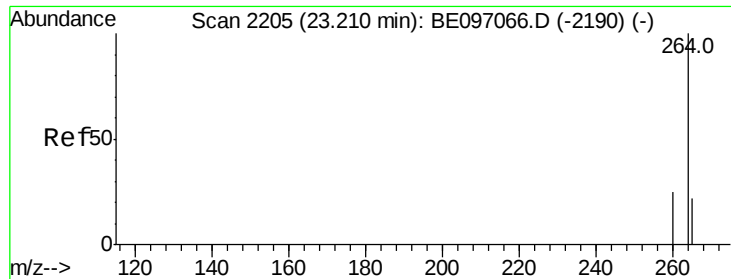

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.21 min Scan# 2204

Delta R.T. -0.00 min

Lab File: BE097094.D

Acq: 25 Jul 2018 5:42

Instrument :

BNA_E

ClientSampleId :

RE109D2-071618DL

Tot Ion:264 Resp: 12436

Ion Ratio Lower Upper

264 100

260 25.8 20.5 30.7

265 24.9 22.8 34.2

