
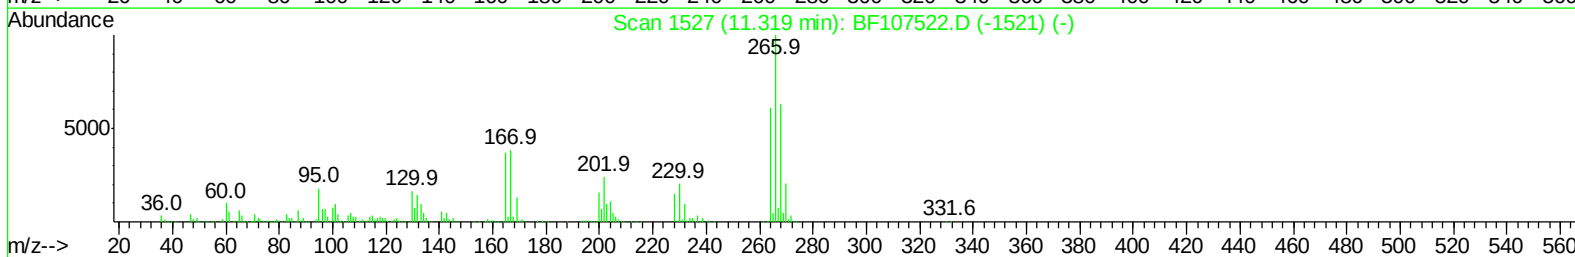
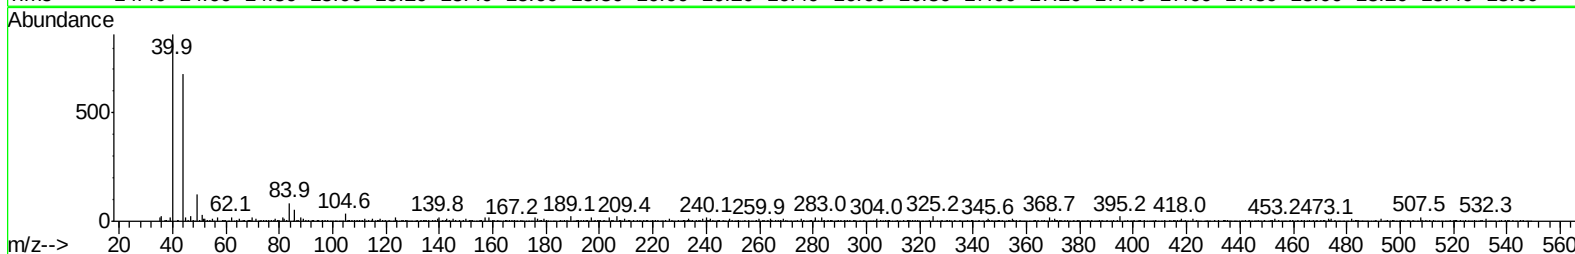


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE072418\
Data File : BE097071.D
Acq On : 24 Jul 2018 14:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 09:20:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

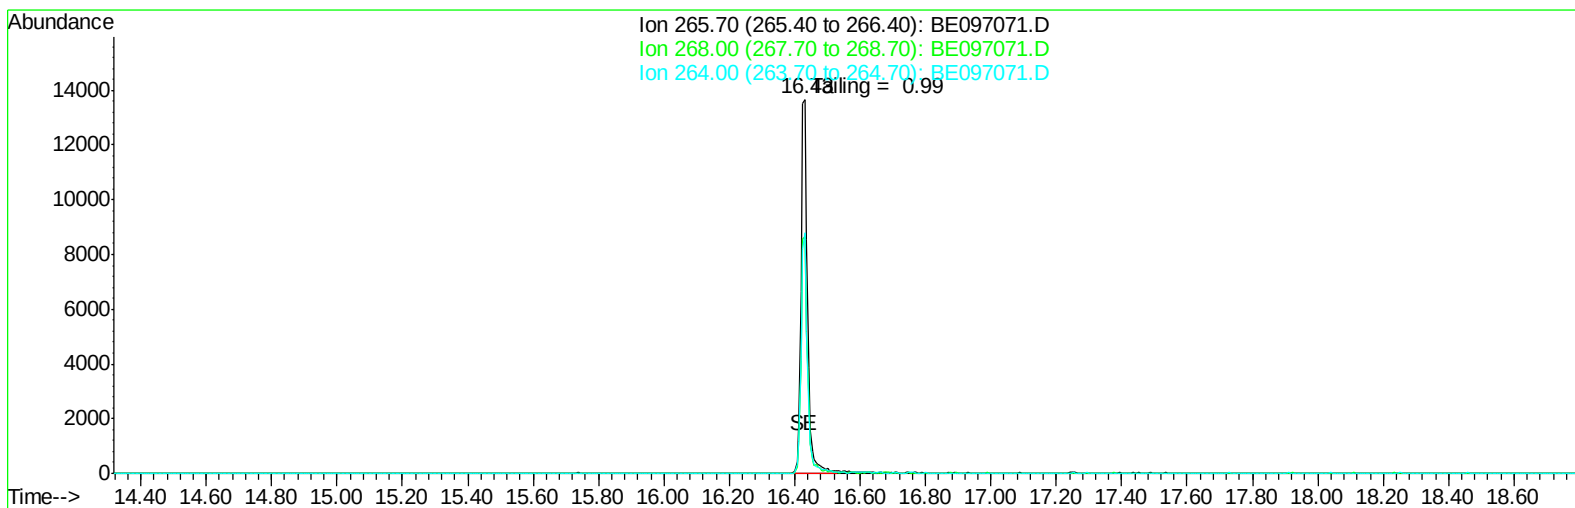

TIC: BE097071.D

(69) Pentachlorophenol (C)




11.336min (+0.018) 68.67ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	85.71#
264.00	61.90	214.29#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE072418\
Data File : BE097071.D
Acq On : 24 Jul 2018 14:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 09:20:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

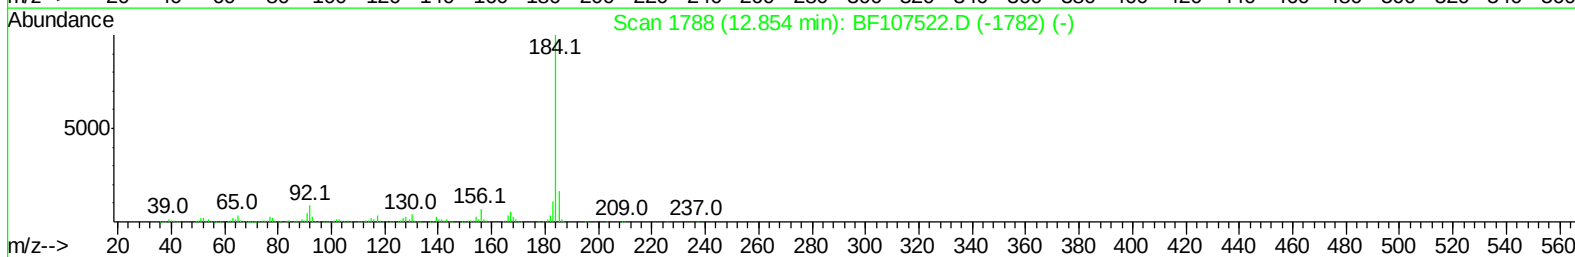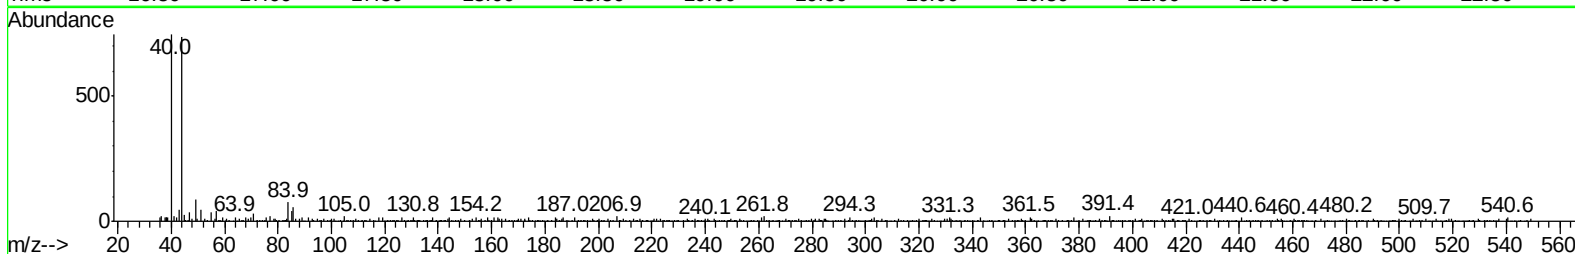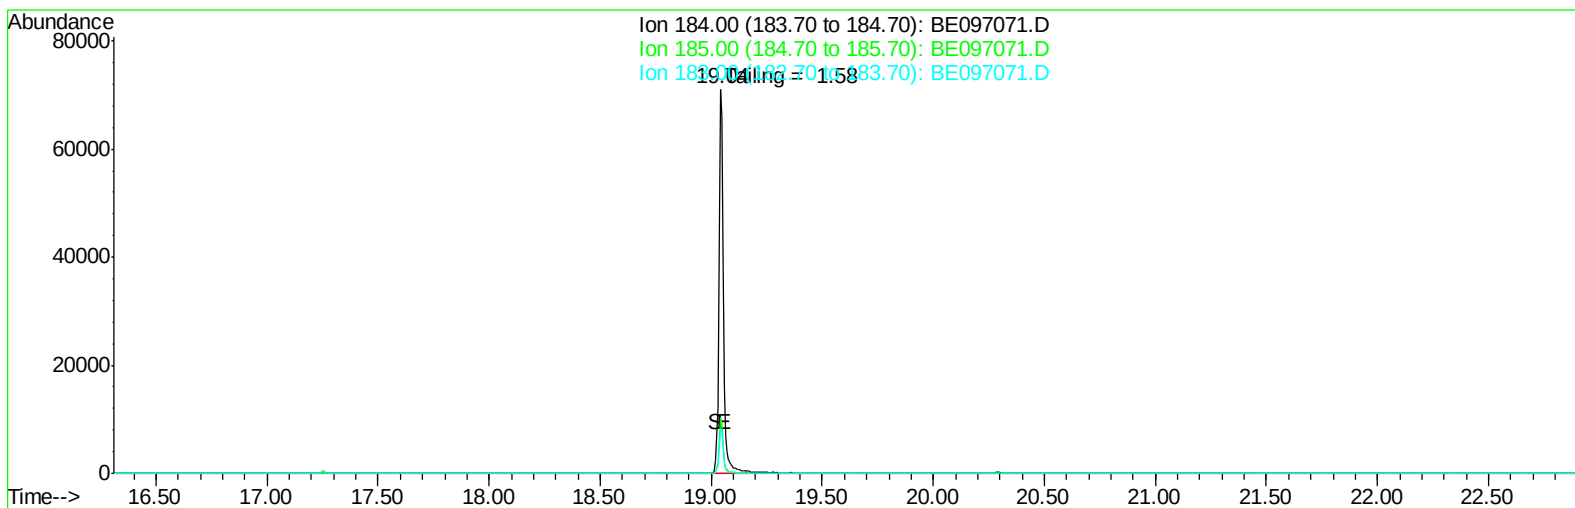

TIC: BE097071.D

(76) Benzidine

12.864min (+0.010) 84.33ng

response 17

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	31.82#
183.00	11.60	0.00#
0.00	0.00	0.00