


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072418\
 Data File : BE097063.D
 Acq On : 24 Jul 2018 8:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 10:49:28 2018

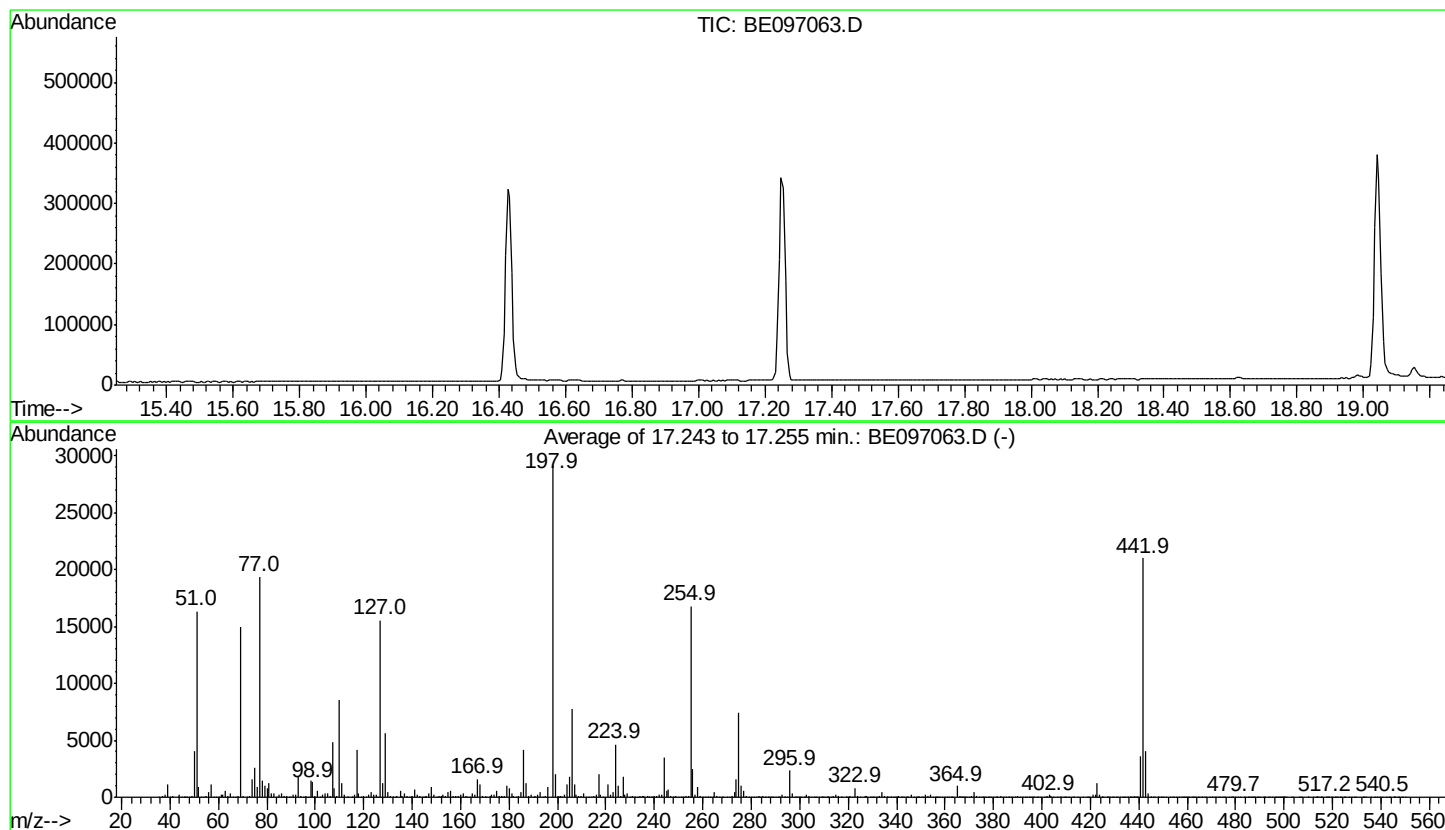

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.1	16349	PASS
68	69	0.00	2	1.1	160	PASS
69	198	0.00	100	51.4	14995	PASS
70	69	0.00	2	0.6	88	PASS
127	198	10	80	53.3	15543	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29146	PASS
199	198	5	9	6.9	2000	PASS
275	198	10	60	25.7	7478	PASS
365	198	1	100	3.4	979	PASS
441	198	0.01	100	12.4	3617	PASS
442	198	50	100	72.1	21021	PASS
443	442	15	24	19.2	4034	PASS