


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072418\  
Data File : BE097071.D  
Acq On : 24 Jul 2018 14:05  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE072418.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jul 31 10:49:28 2018

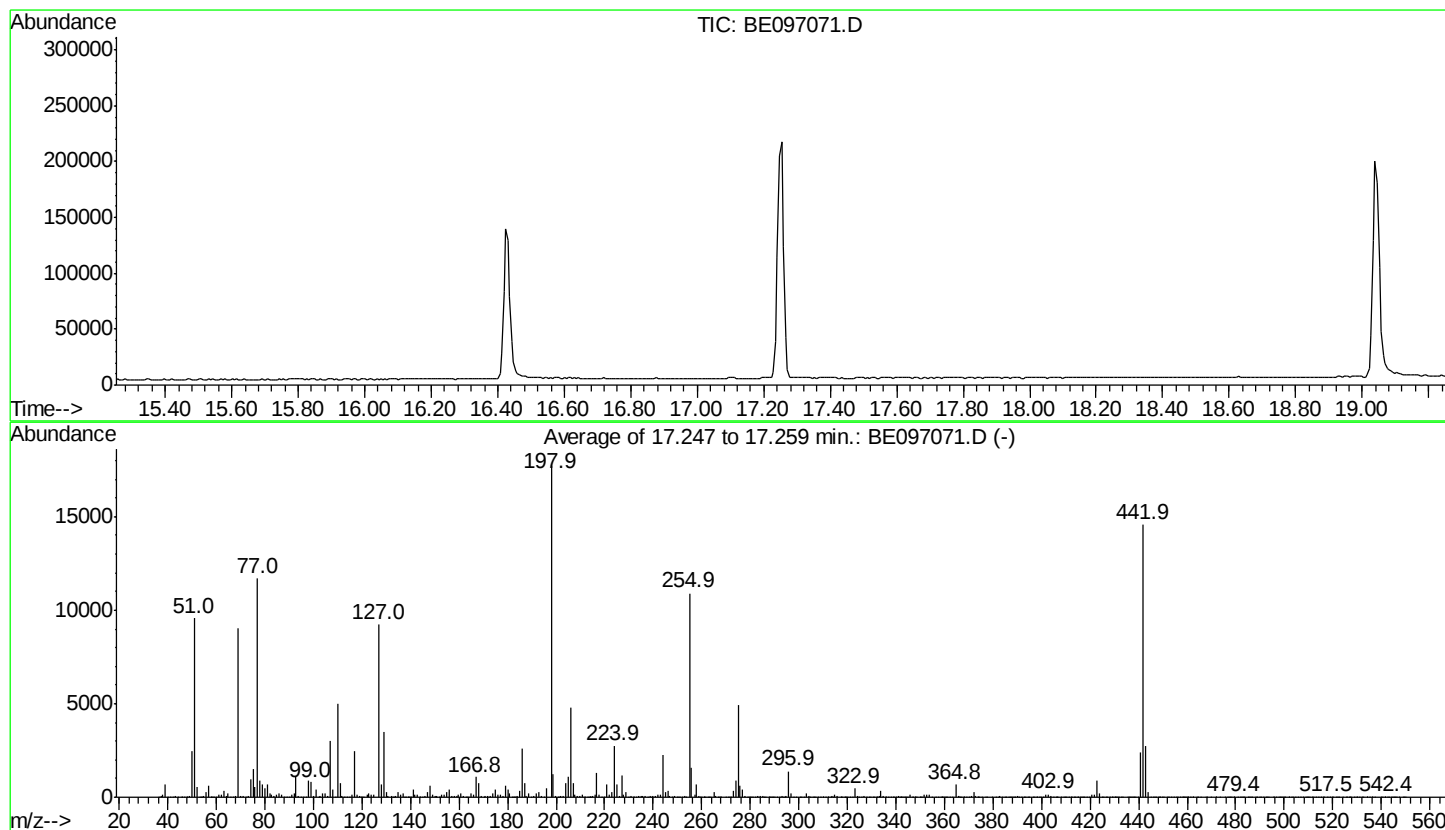

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 53.9      | 9562    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 88      | PASS             |
| 69          | 198          | 0.00         | 100          | 51.0      | 9046    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.9       | 79      | PASS             |
| 127         | 198          | 10           | 80           | 52.0      | 9227    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 17730   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 1207    | PASS             |
| 275         | 198          | 10           | 60           | 27.9      | 4952    | PASS             |
| 365         | 198          | 1            | 100          | 3.8       | 677     | PASS             |
| 441         | 198          | 0.01         | 100          | 13.5      | 2396    | PASS             |
| 442         | 198          | 50           | 100          | 82.1      | 14562   | PASS             |
| 443         | 442          | 15           | 24           | 19.0      | 2762    | PASS             |