


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072418\
 Data File : BE097088.D
 Acq On : 25 Jul 2018 1:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 10:49:28 2018

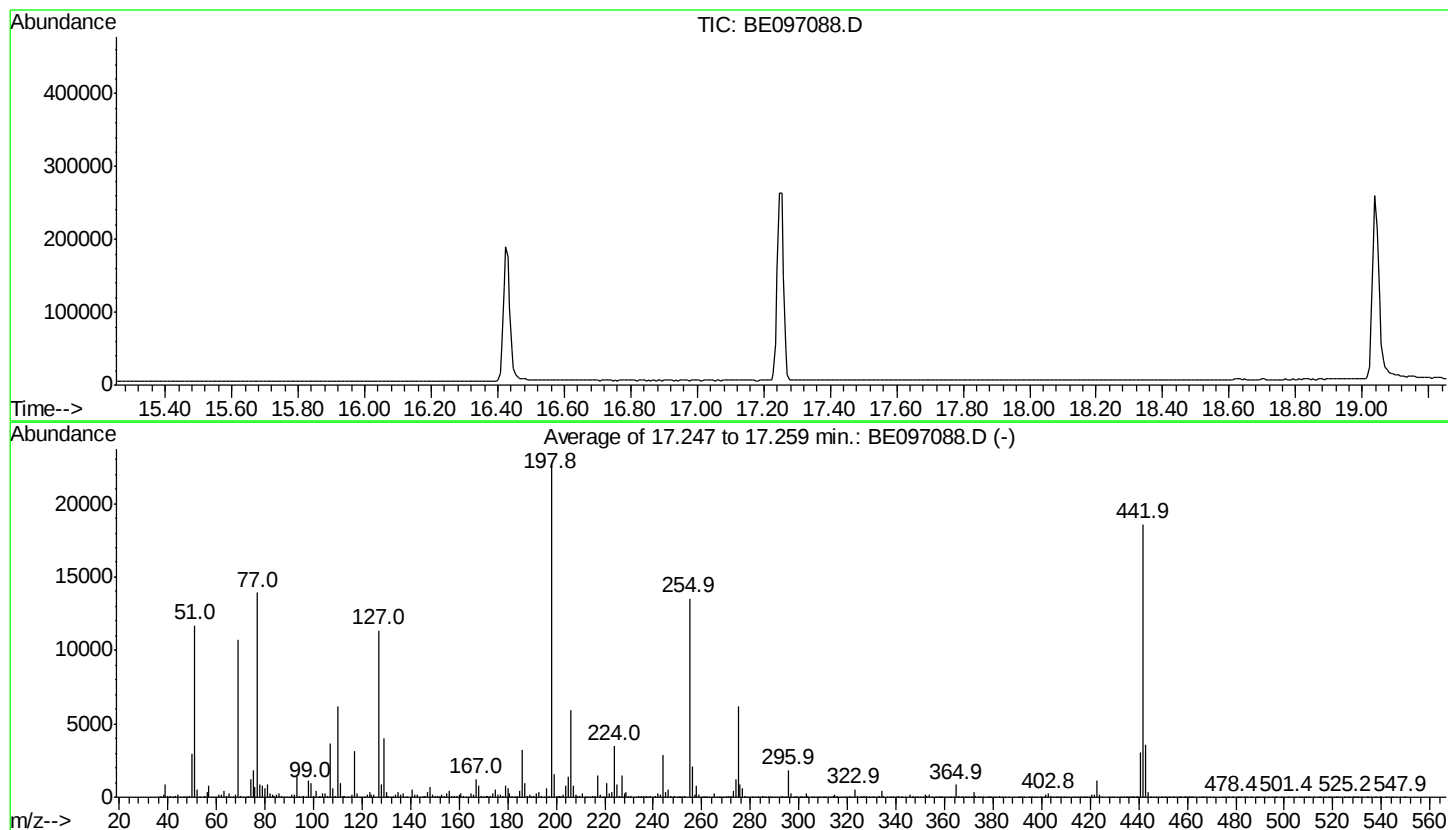

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	11714	PASS
68	69	0.00	2	1.7	184	PASS
69	198	0.00	100	47.5	10732	PASS
70	69	0.00	2	0.7	71	PASS
127	198	10	80	50.2	11339	PASS
197	198	0.00	2	0.3	63	PASS
198	198	100	100	100.0	22583	PASS
199	198	5	9	7.1	1602	PASS
275	198	10	60	27.3	6172	PASS
365	198	1	100	3.8	850	PASS
441	198	0.01	100	13.4	3030	PASS
442	198	50	100	82.4	18611	PASS
443	442	15	24	19.4	3606	PASS