

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
 Data File : BE093594.D
 Acq On : 26 Jul 2017 1:35
 Operator : SJ/JU
 Sample : I4373-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA0

Quant Time: Jul 26 05:47:19 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 05:32:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	2731	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	14374	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	9411	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	22567	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1618186	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6581	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	20825	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.52	166	2241	0.057	ng/ul#	19
17) Pyrene	19.64	202	2762	0.042	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093594.D
Acq On : 26 Jul 2017 1:35
Operator : SJ/JU
Sample : I4373-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA0

Quant Time: Jul 26 05:47:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

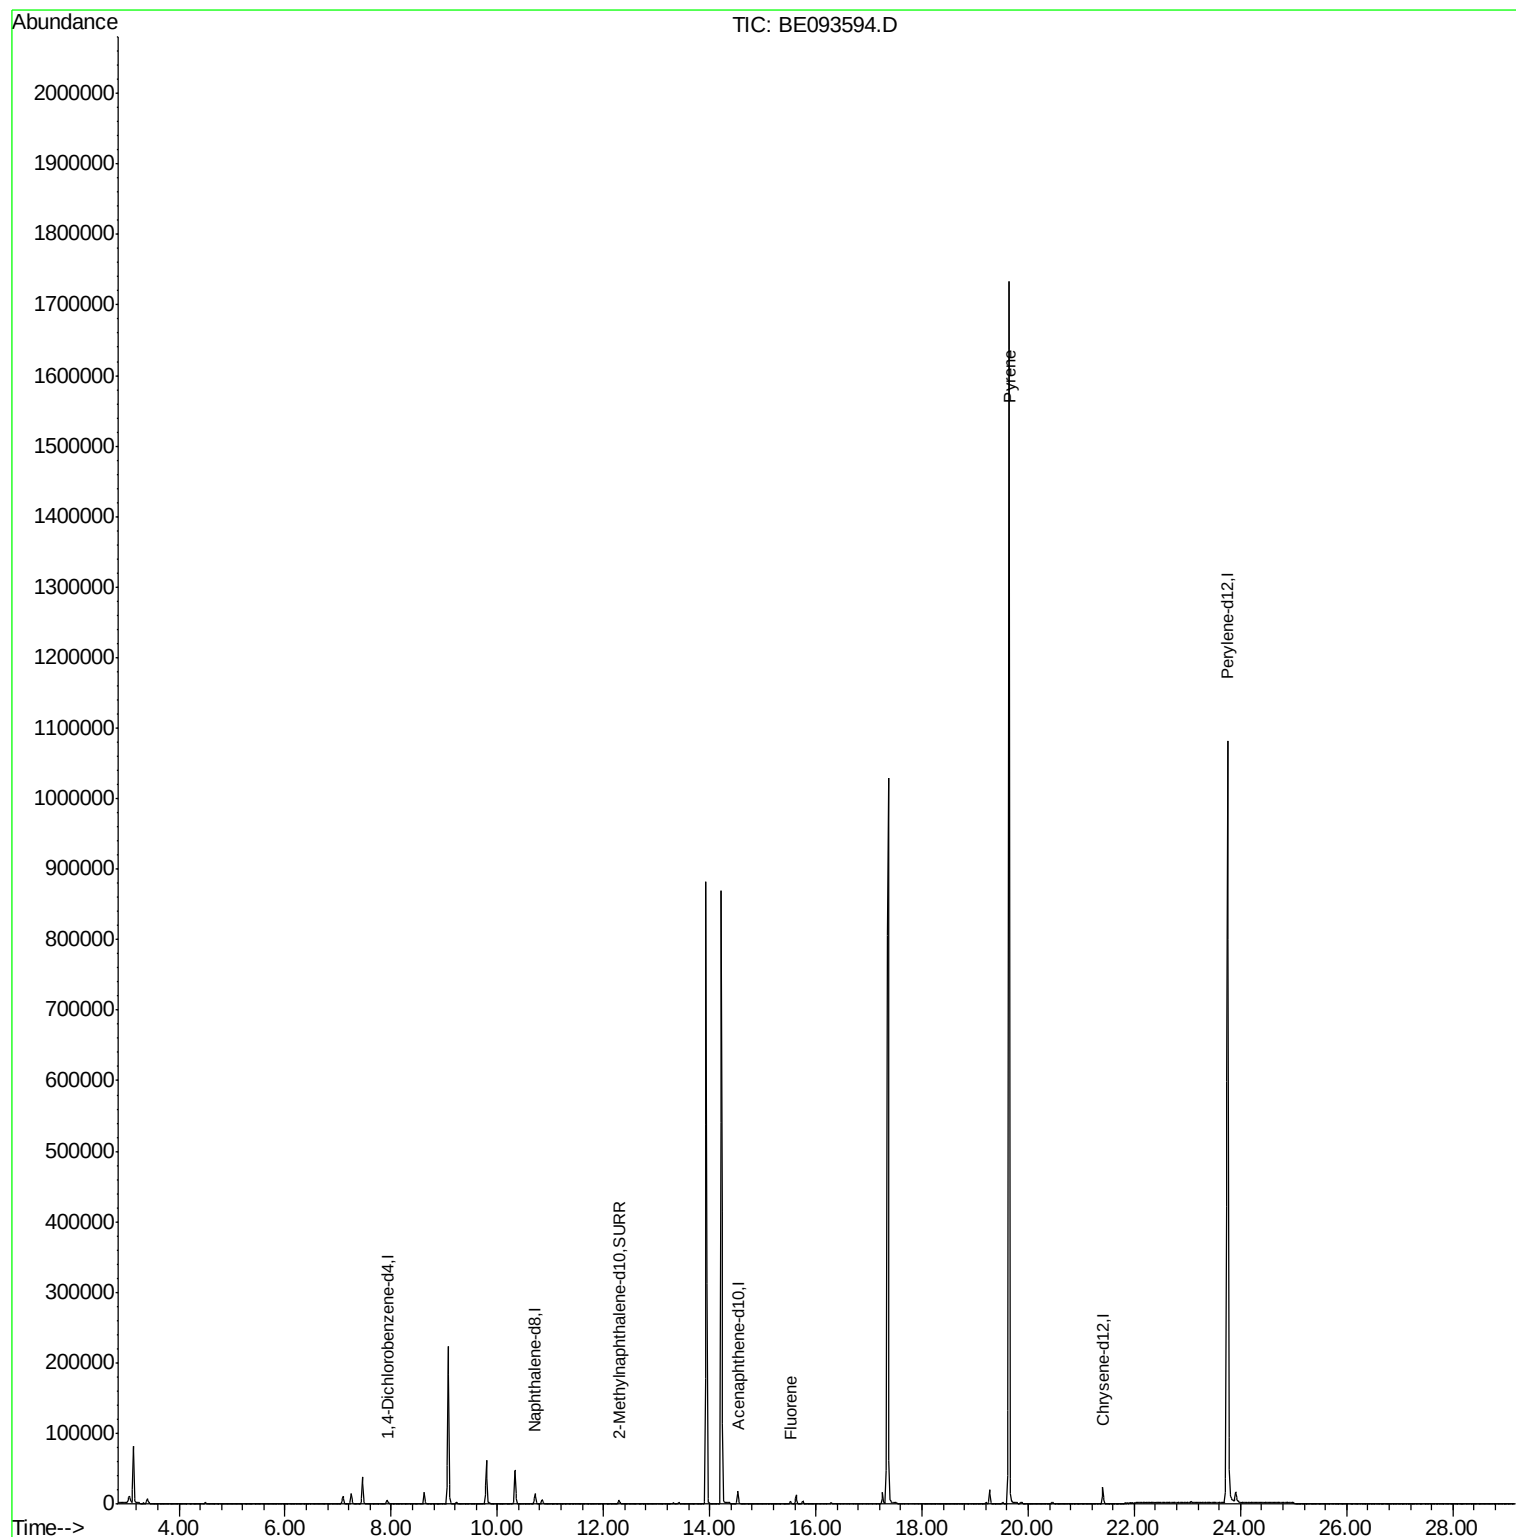

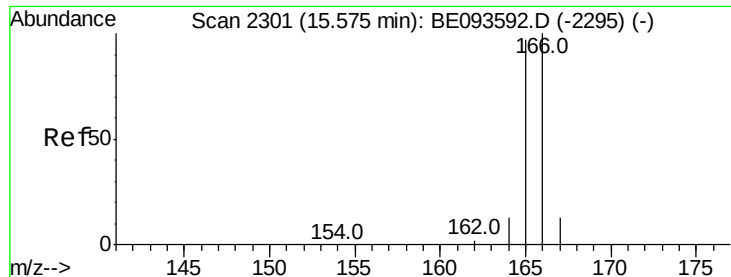

#9

Fluorene

Concen: 0.057 ng/ul

RT: 15.52 min Scan# 2294

Delta R.T. -0.05 min

Lab File: BE093594.D

Acq: 26 Jul 2017 1:35

Instrument :

BNA_E

ClientSampleId :

C0AA0


Tot Ion:166 Resp: 2241

Ion Ratio Lower Upper

166 100

165 7.2 73.4 110.2#


167 37.7 14.6 22.0#

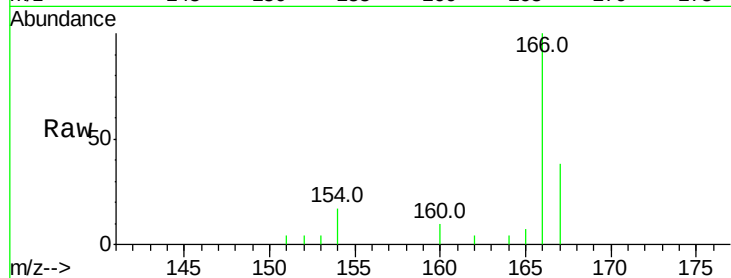



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

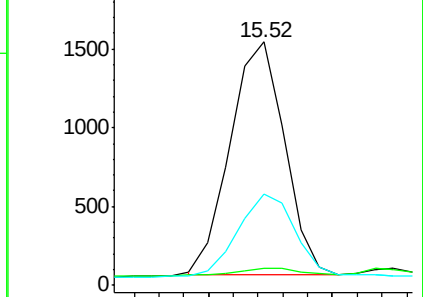

Time-->

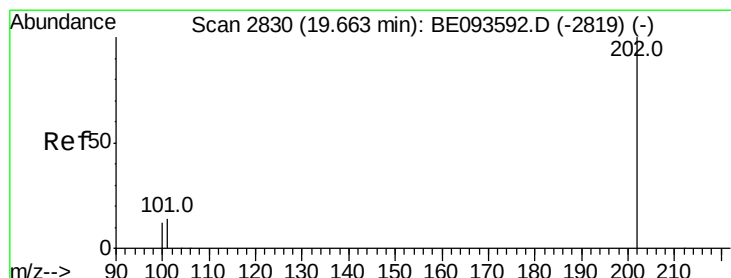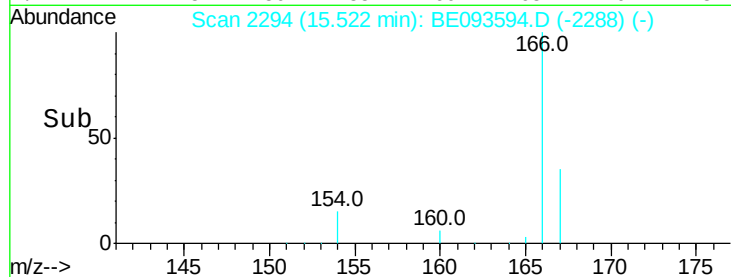

#17

Pyrene

Concen: 0.042 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.02 min

Lab File: BE093594.D

Acq: 26 Jul 2017 1:35


Tgt Ion:202 Resp: 2762

Ion Ratio Lower Upper

202 100

101 166.4 18.2 27.4#


100 901.3 15.6 23.4#

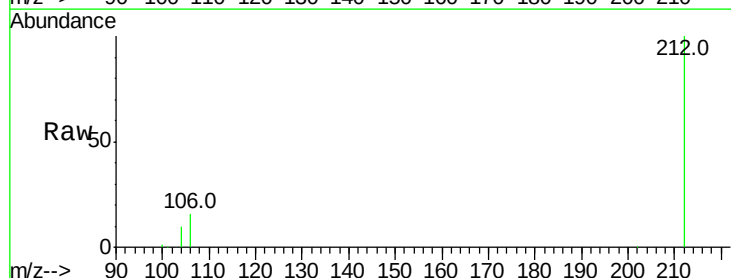

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

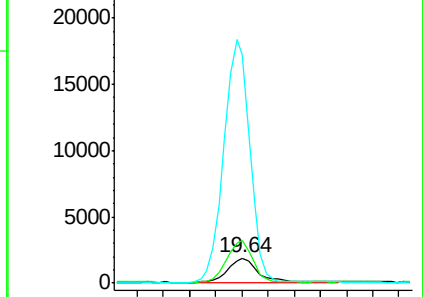

Time-->

