

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
 Data File : BE093595.D
 Acq On : 26 Jul 2017 2:13
 Operator : SJ/JU
 Sample : I4373-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Quant Time: Jul 26 05:47:27 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 05:32:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2620	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	13797	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	9051	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	21934	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1407737	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	5720	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	18372	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	2568	0.040	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093595.D
Acq On : 26 Jul 2017 2:13
Operator : SJ/JU
Sample : I4373-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Quant Time: Jul 26 05:47:27 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

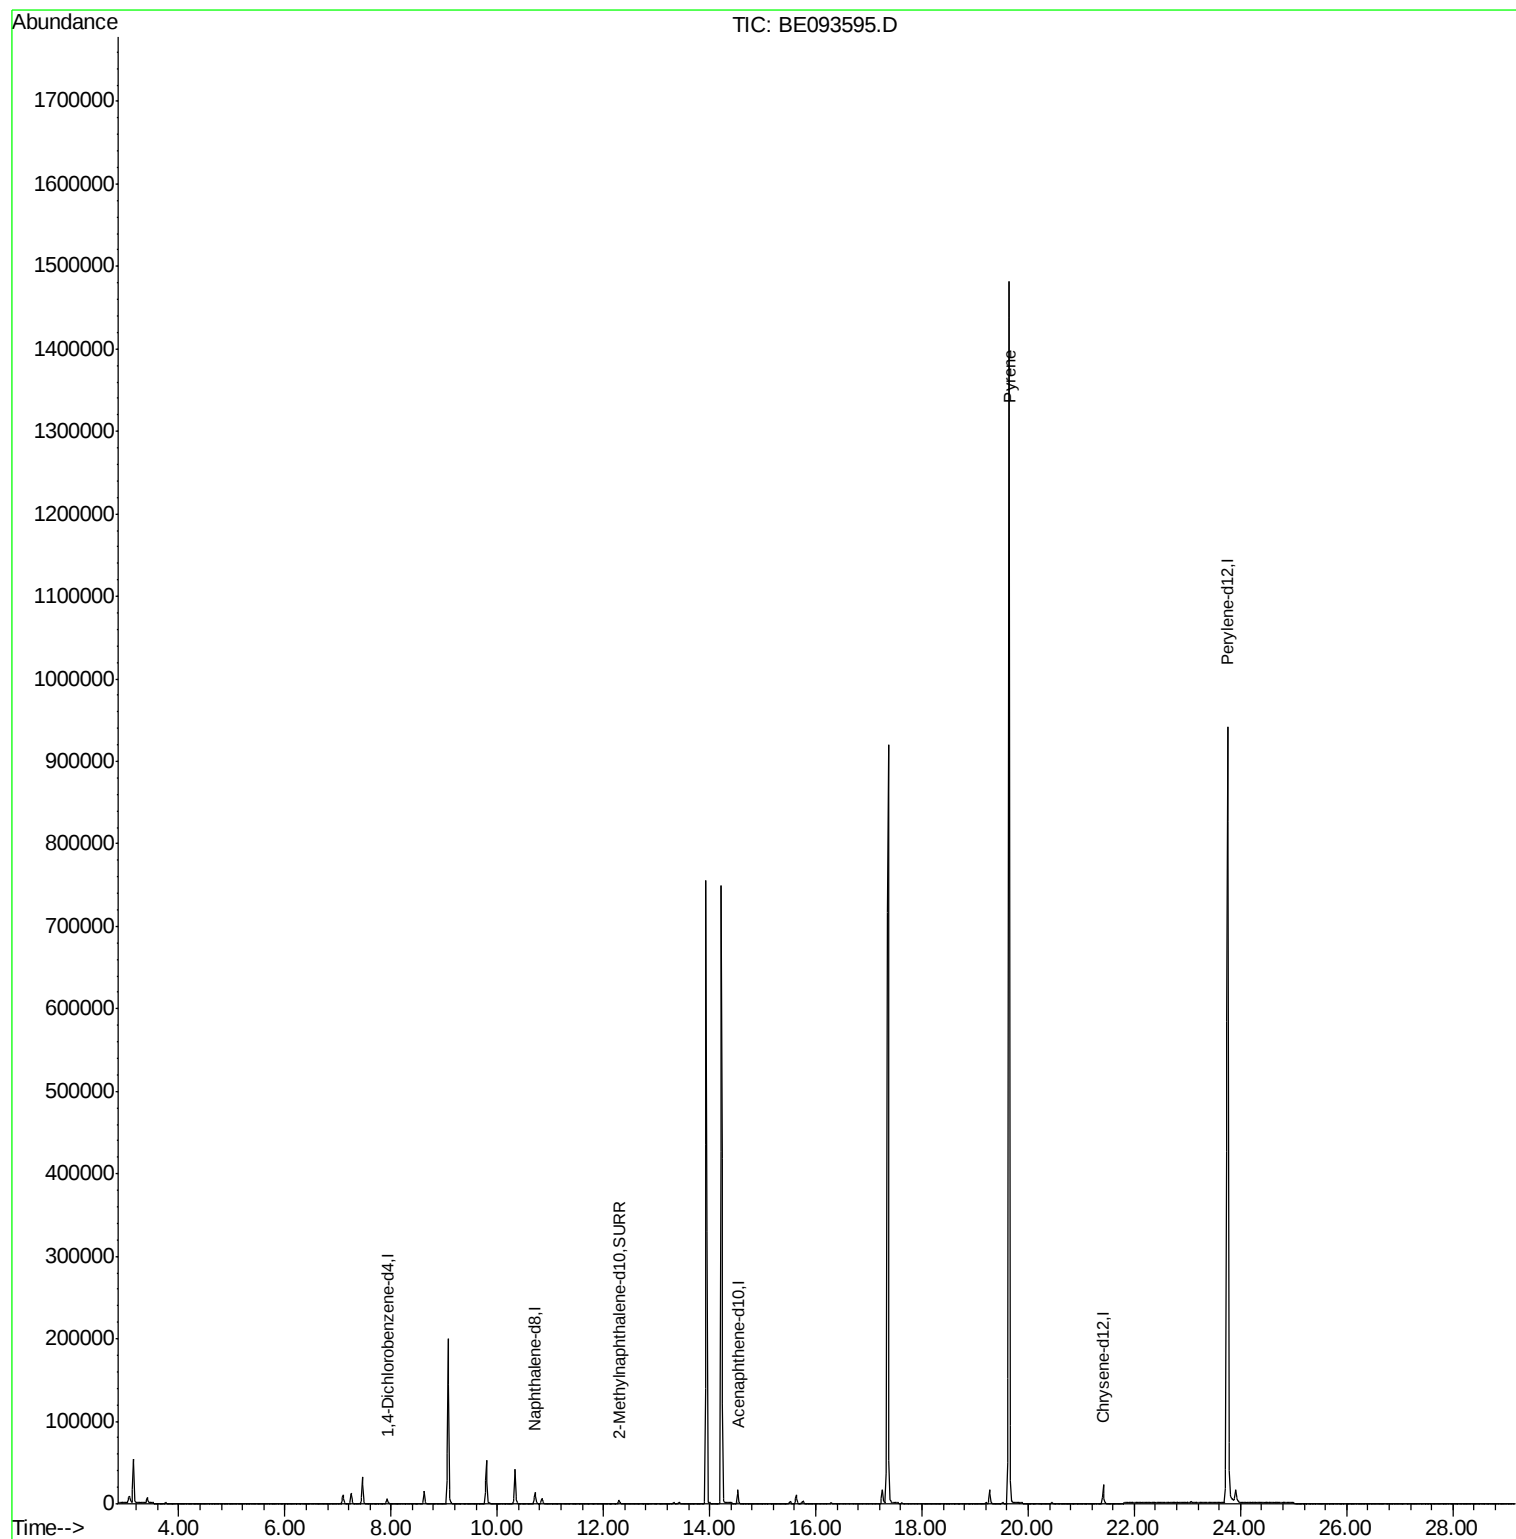


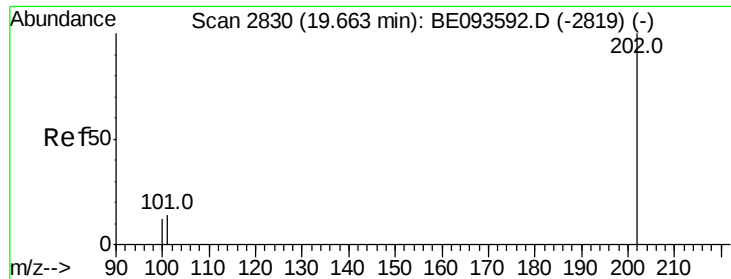

#17
 Pvrene
 Concen: 0.040 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.02 min
 Lab File: BE093595.D
 Acq: 26 Jul 2017 2:13

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Tot Ion: 202 Resp: 2568
 Ion Ratio Lower Upper
 202 100
 101 161.1 18.2 27.4#
 100 846.0 15.6 23.4#

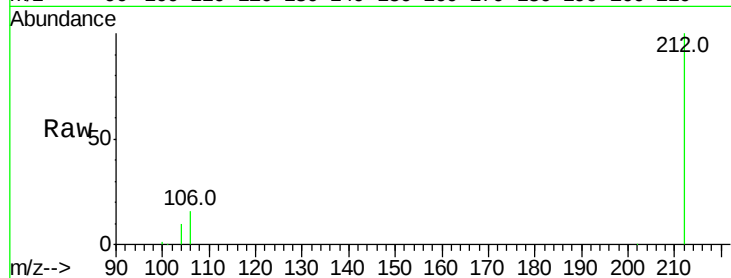

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BE

