

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
 Data File : BE093596.D
 Acq On : 26 Jul 2017 2:49
 Operator : SJ/JU
 Sample : I4373-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA2

Quant Time: Jul 26 05:47:33 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 05:32:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3089	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16378	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10496	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	26139	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1550165	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6411	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	21974	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	2780	0.036	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093596.D
Acq On : 26 Jul 2017 2:49
Operator : SJ/JU
Sample : I4373-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA2

Quant Time: Jul 26 05:47:33 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

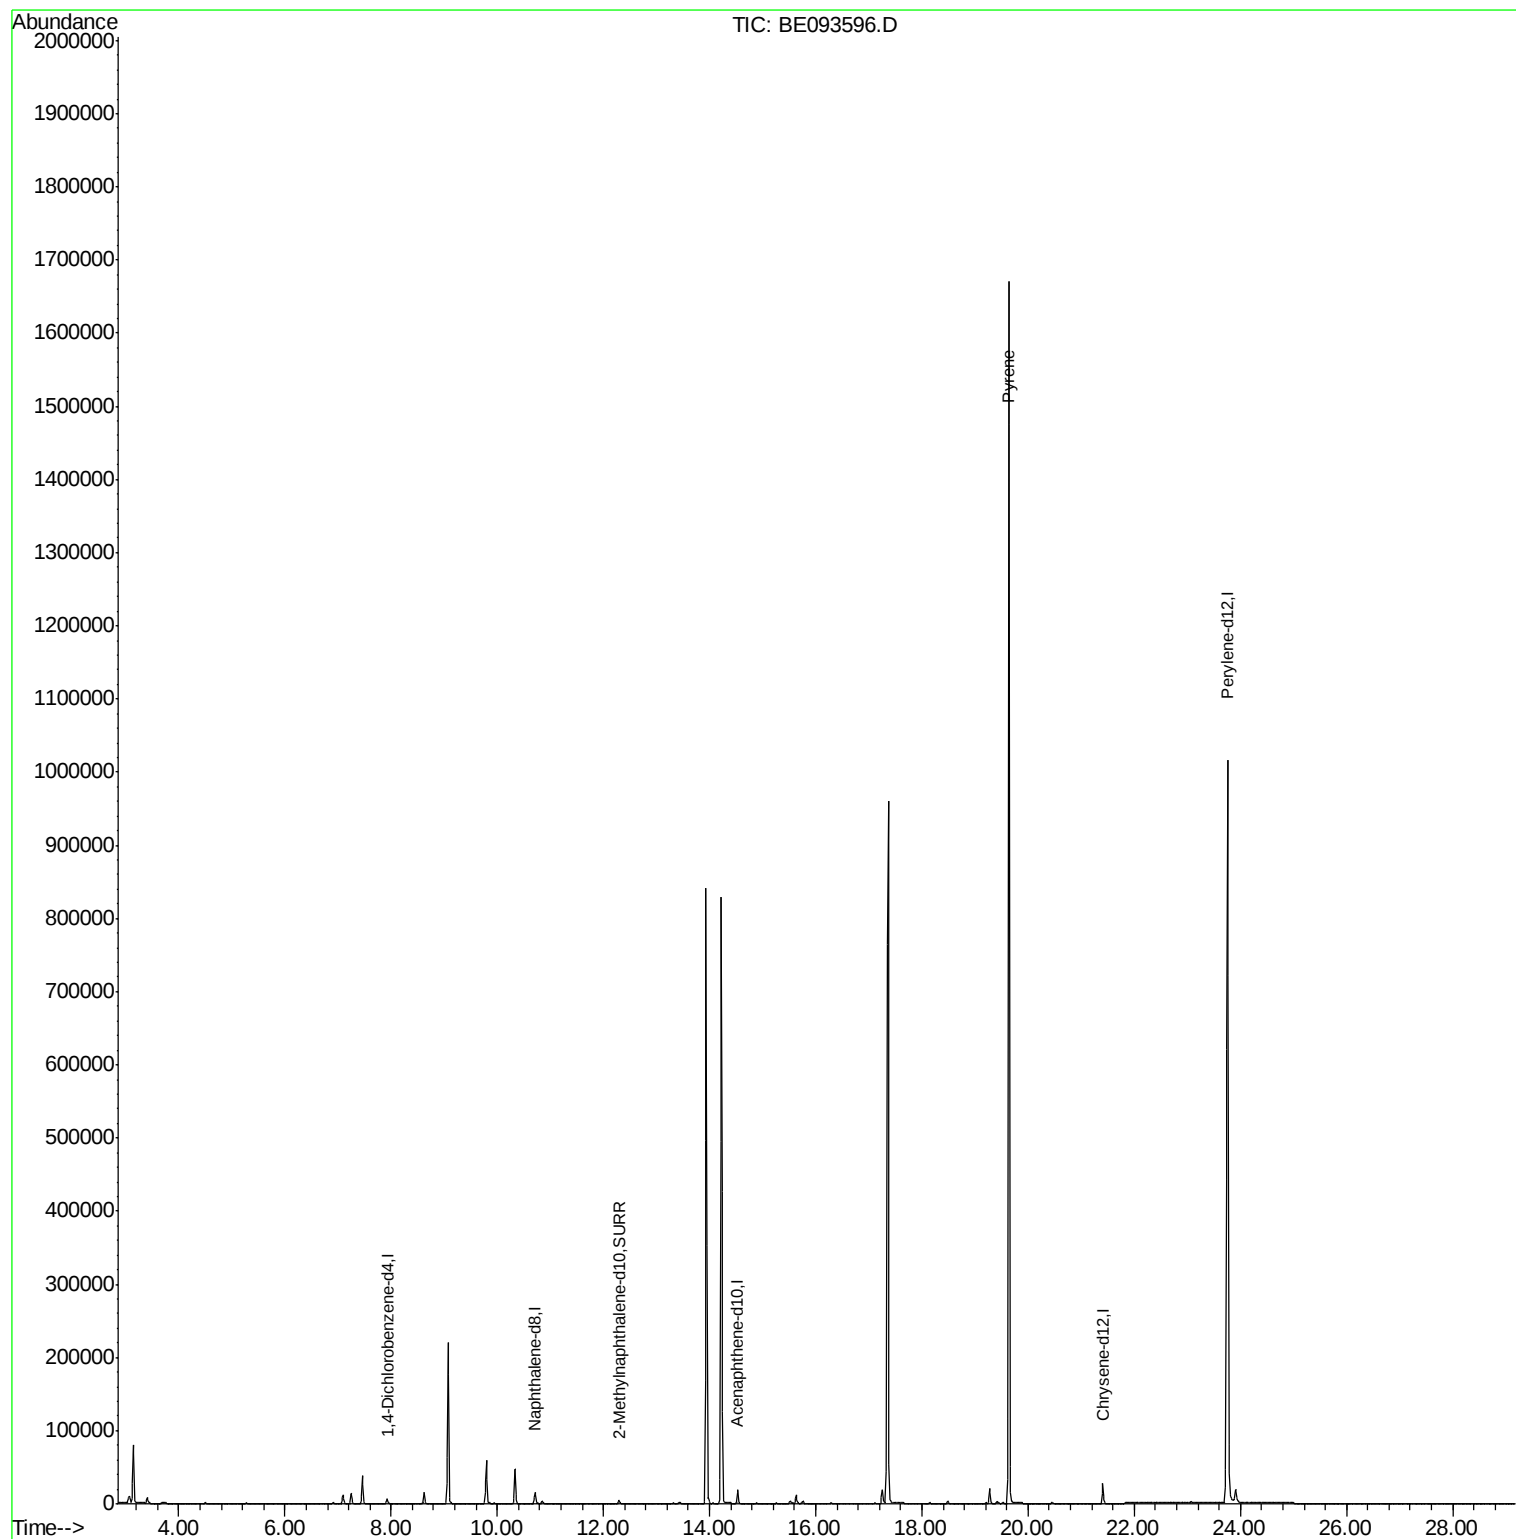

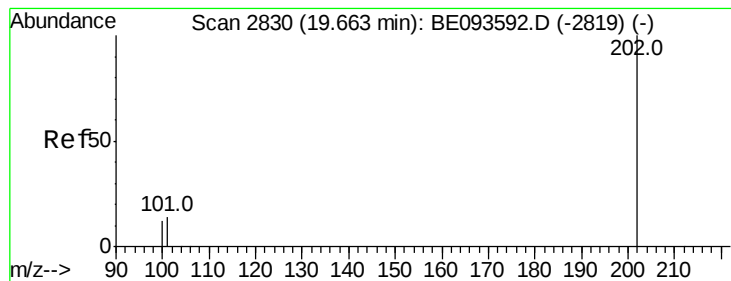

#17

Pvrene

Concen: 0.036 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.02 min

Lab File: BE093596.D

Acq: 26 Jul 2017 2:49

Instrument :

BNA_E

ClientSampleId :

C0AA2


Tot Ion:202 Resp: 2780

Ion Ratio Lower Upper

202 100

101 167.2 18.2 27.4#

100 916.4 15.6 23.4#

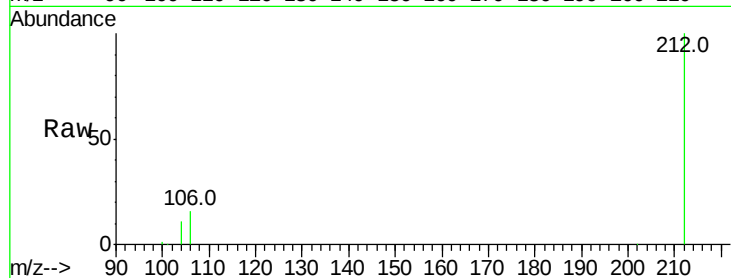

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

