


Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093595.D
Acq On : 26 Jul 2017 2:13
Operator : SJ/JU
Sample : I4373-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
7/26/2017 5:56:17 PM

Quant Time: Jul 26 06:04:42 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

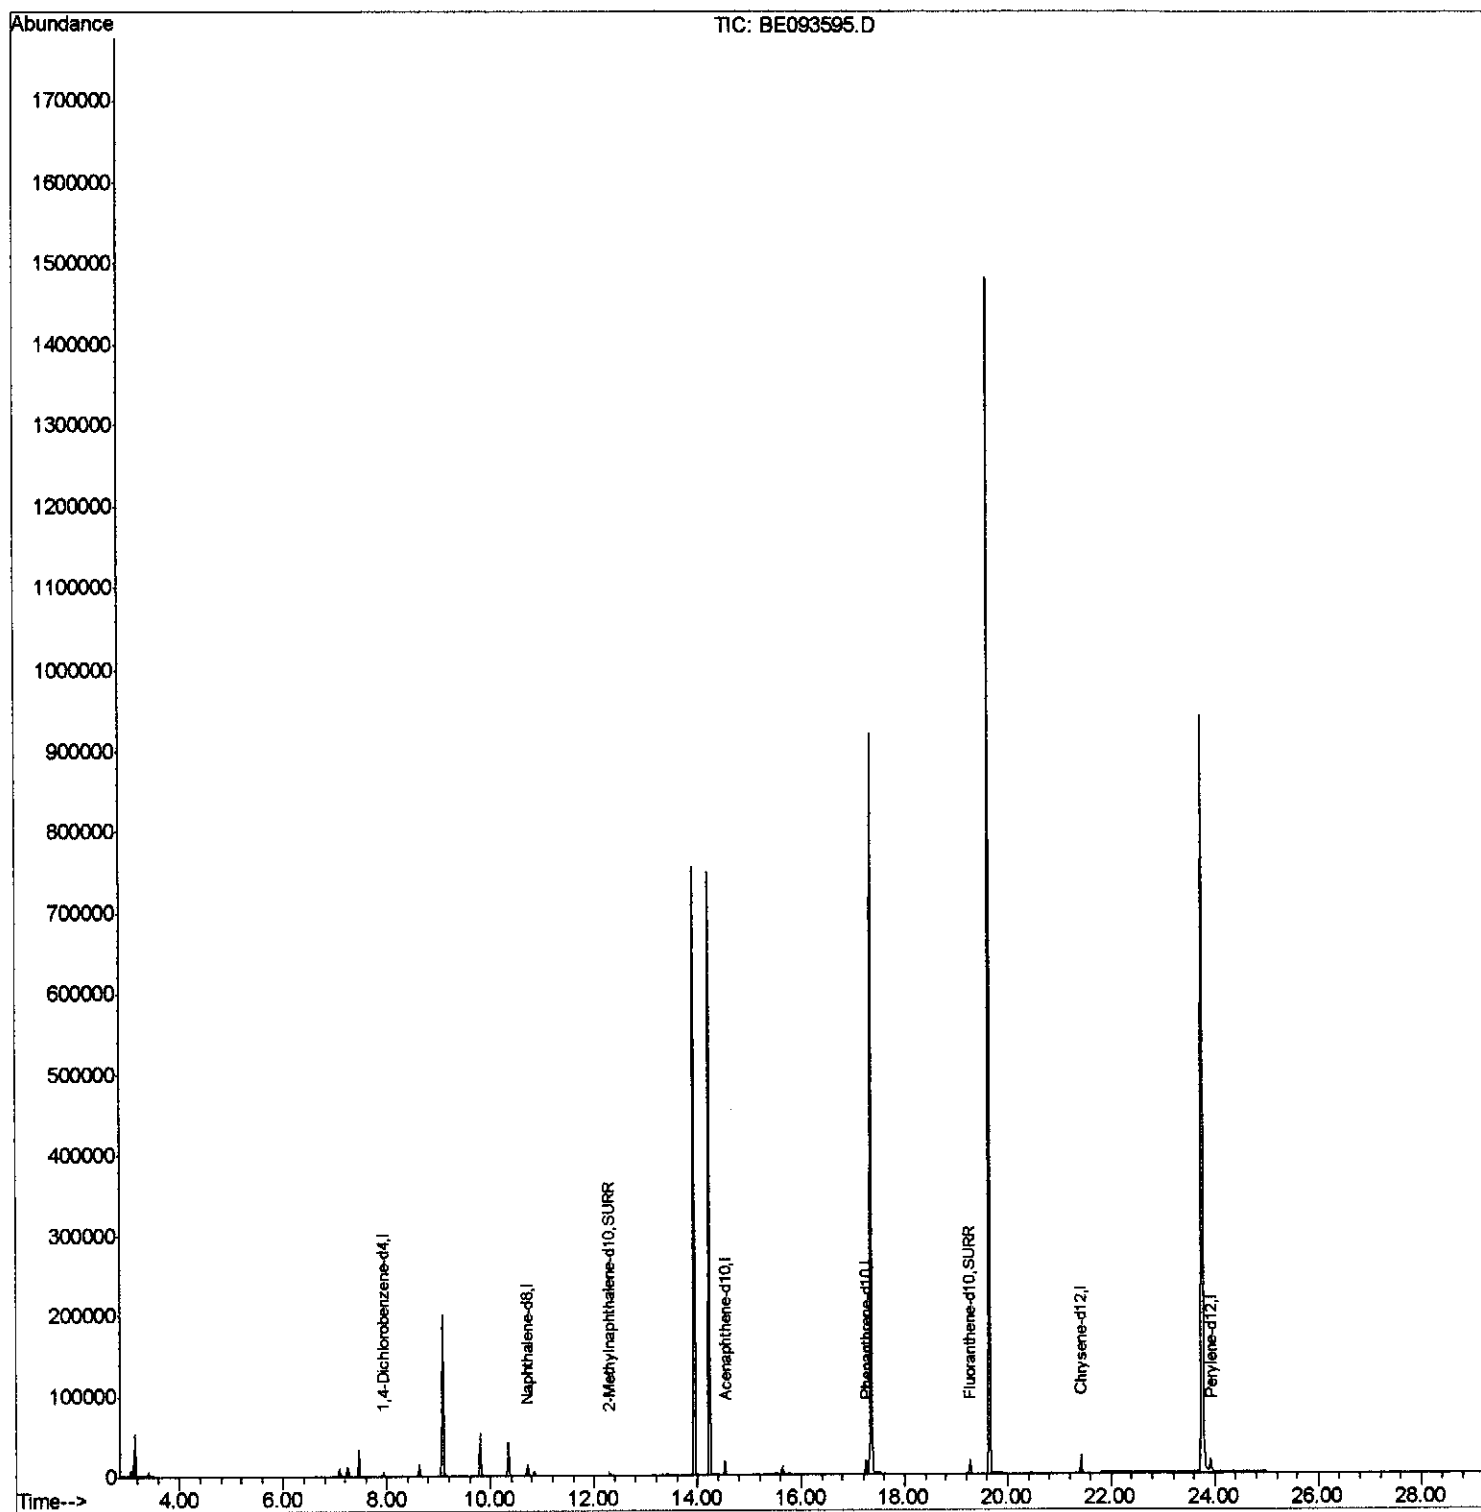




Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093595.D
Acq On : 26 Jul 2017 2:13
Operator : SJ/JU
Sample : I4373-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
7/26/2017 5:56:17 PM

Quant Time: Jul 26 05:47:27 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

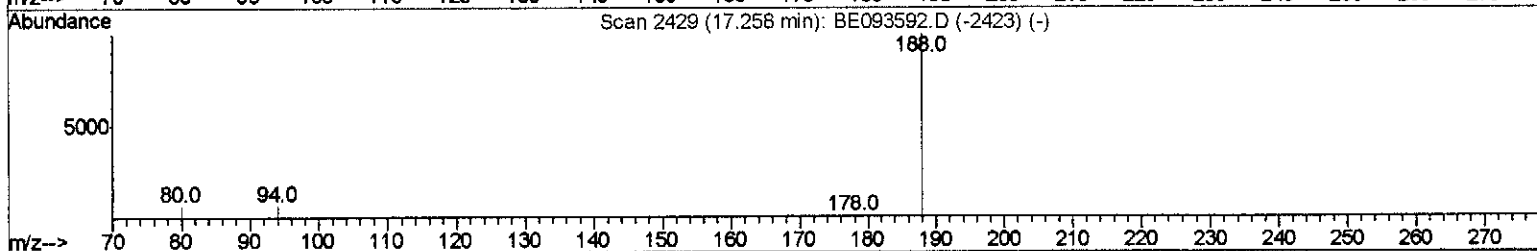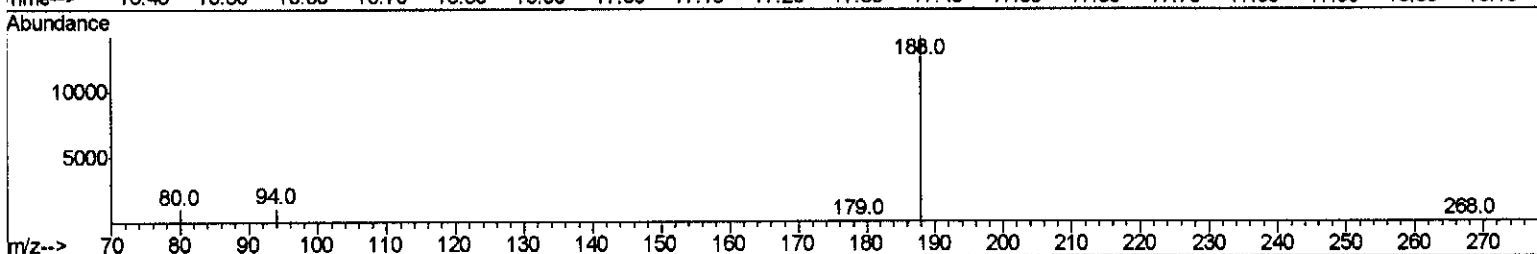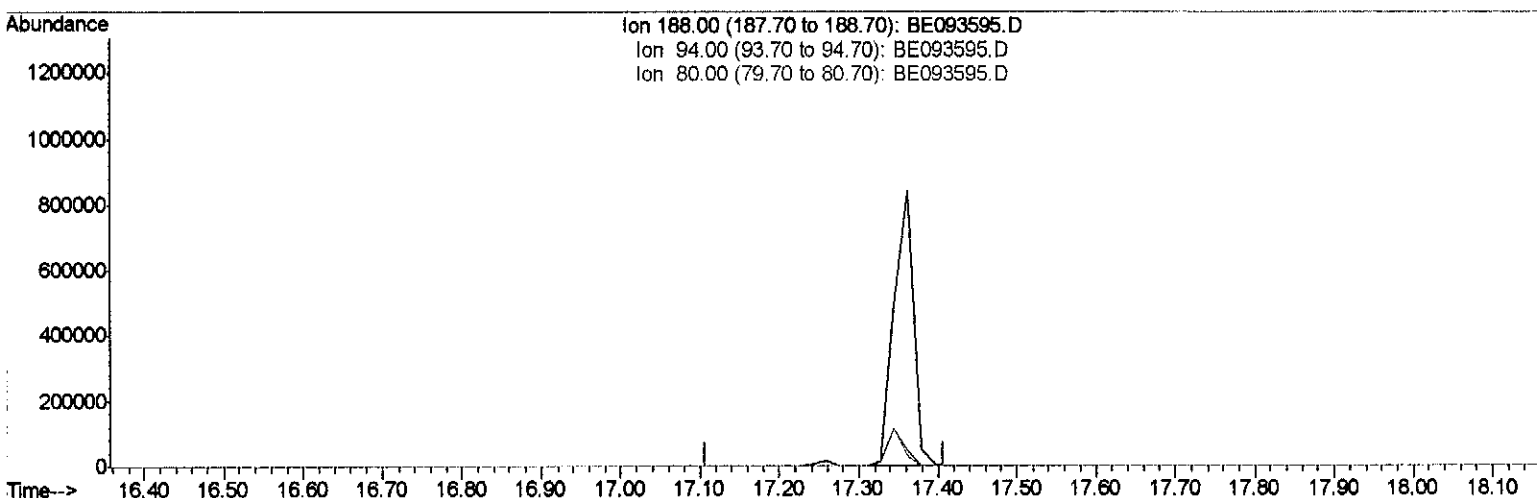

TIC: BE093595.D

(10) Phenanthrene-d10 (I)

17.258min (-17.258) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093595.D
Acq On : 26 Jul 2017 2:13
Operator : SJ/JU
Sample : I4373-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
7/26/2017 5:56:17 PM

Quant Time: Jul 26 05:47:27 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

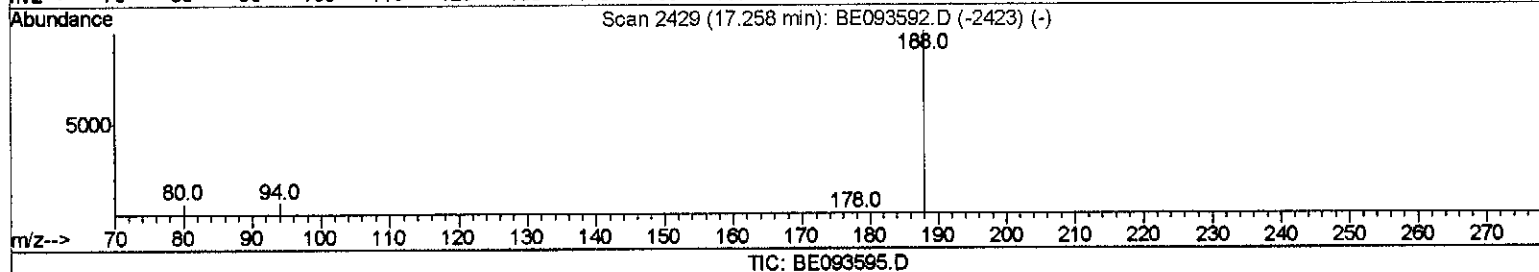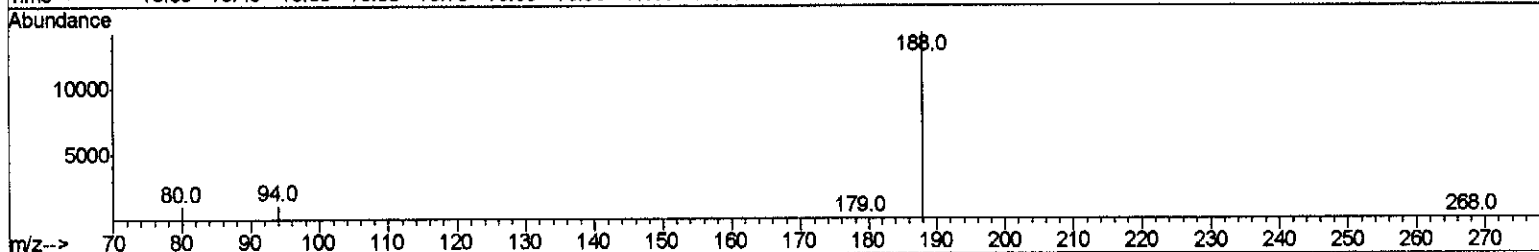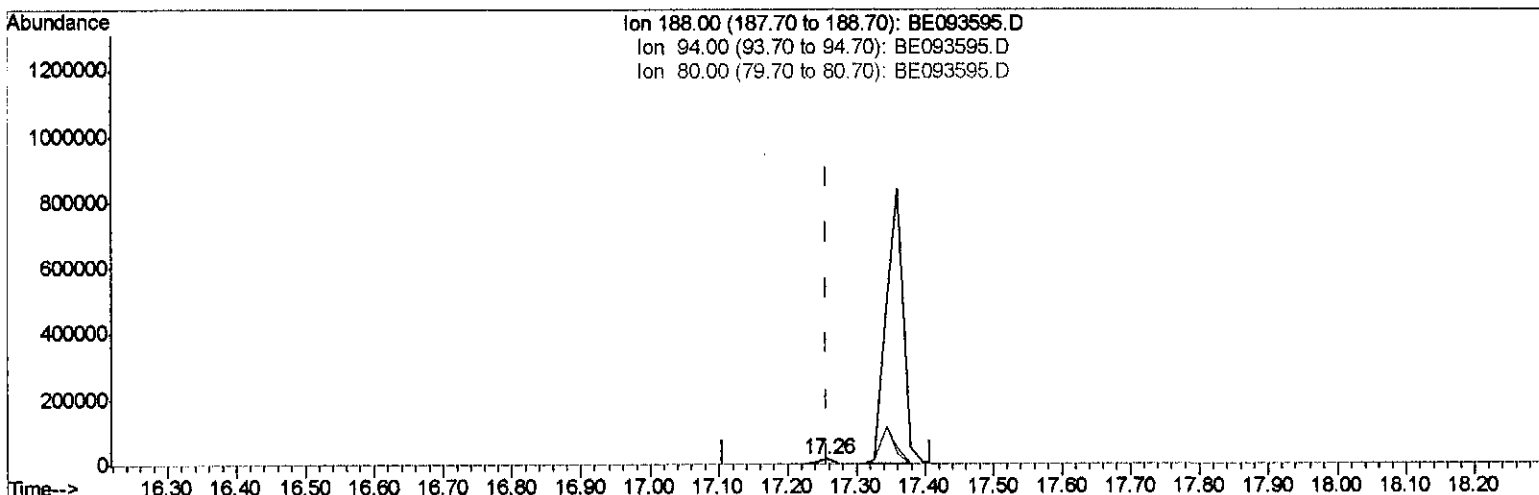

TIC: BE093595.D

(10) Phenanthrene-d10 (I)

17.257min (-0.001) 0.40ng/ul m SJ 8/8/17

response 20585

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.43#
80.00	11.80	6.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
 Data File : BE093595.D
 Acq On : 26 Jul 2017 2:13
 Operator : SJ/JU
 Sample : I4373-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 7/26/2017 5:56:17 PM

Quant Time: Jul 26 06:02:56 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 05:32:22 2017
 Response via : Initial Calibration

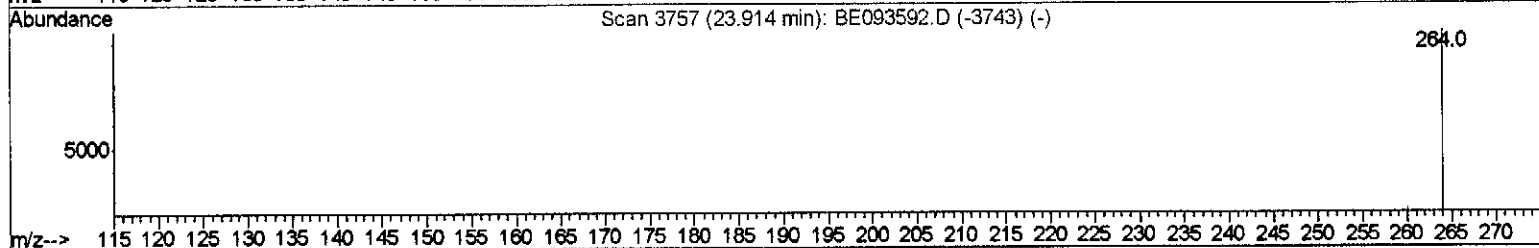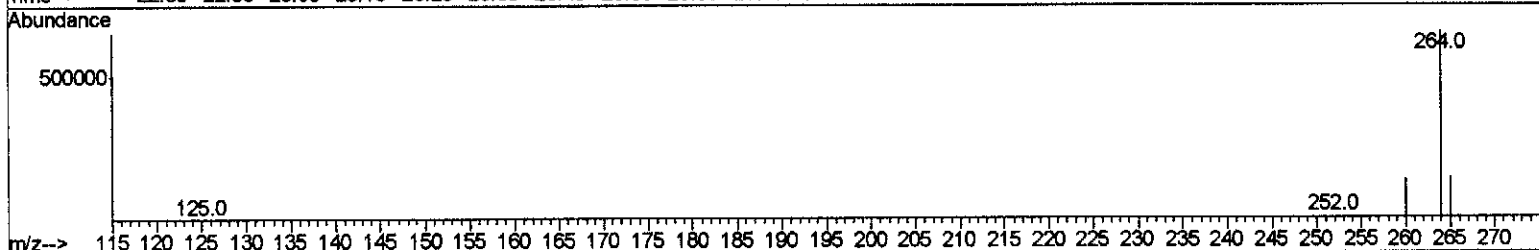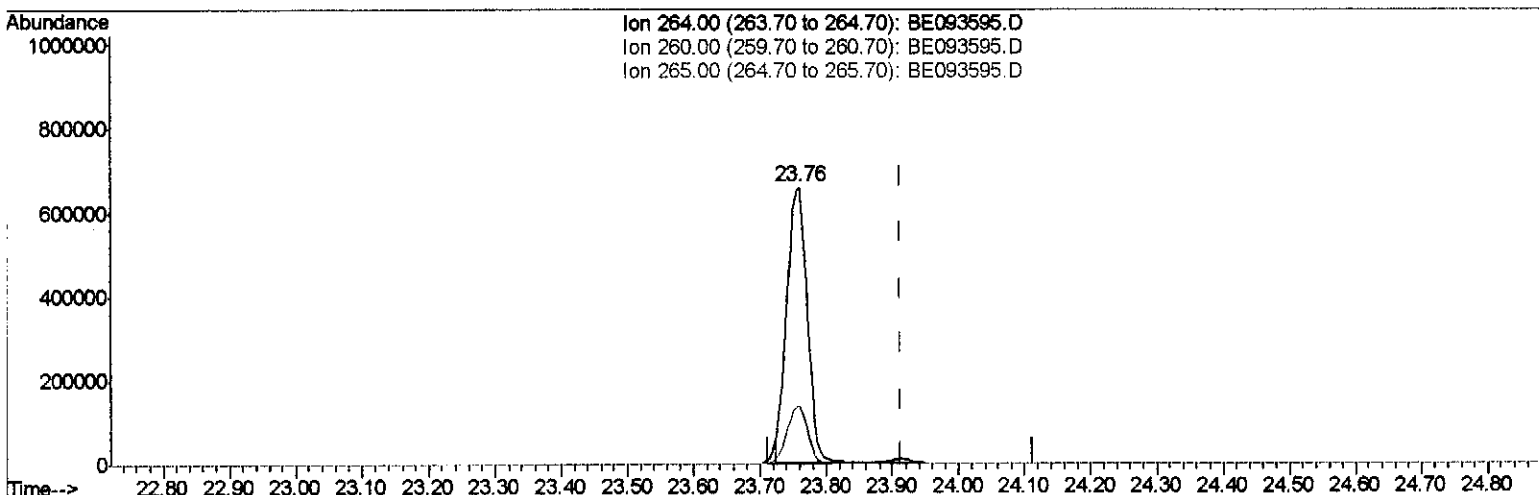

TIC: BE093595.D

(20) Perylene-d12 (I)
 23.760min (-0.154) 0.40ng/ul
 response 1407737

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.79#
266.00	103.50	21.56#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
 Data File : BE093595.D
 Acq On : 26 Jul 2017 2:13
 Operator : SJ/JU
 Sample : I4373-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 7/26/2017 5:56:17 PM

Quant Time: Jul 26 06:02:56 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 05:32:22 2017
 Response via : Initial Calibration

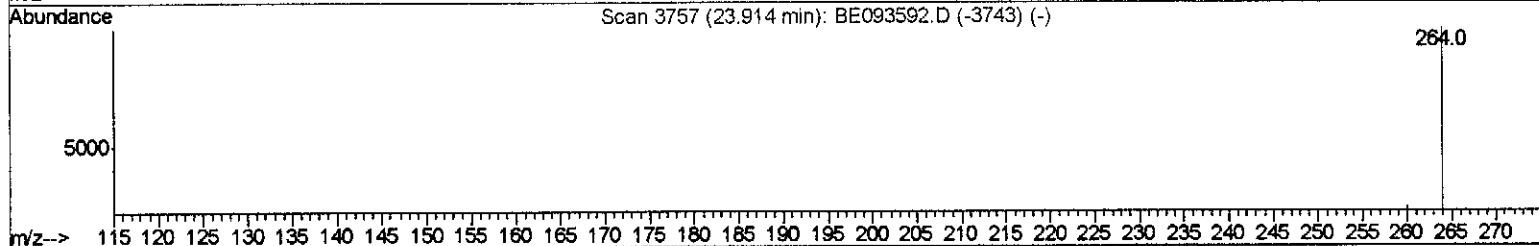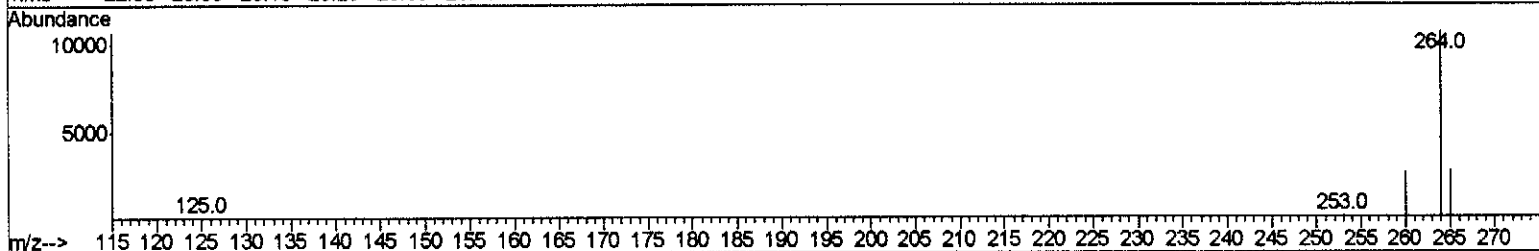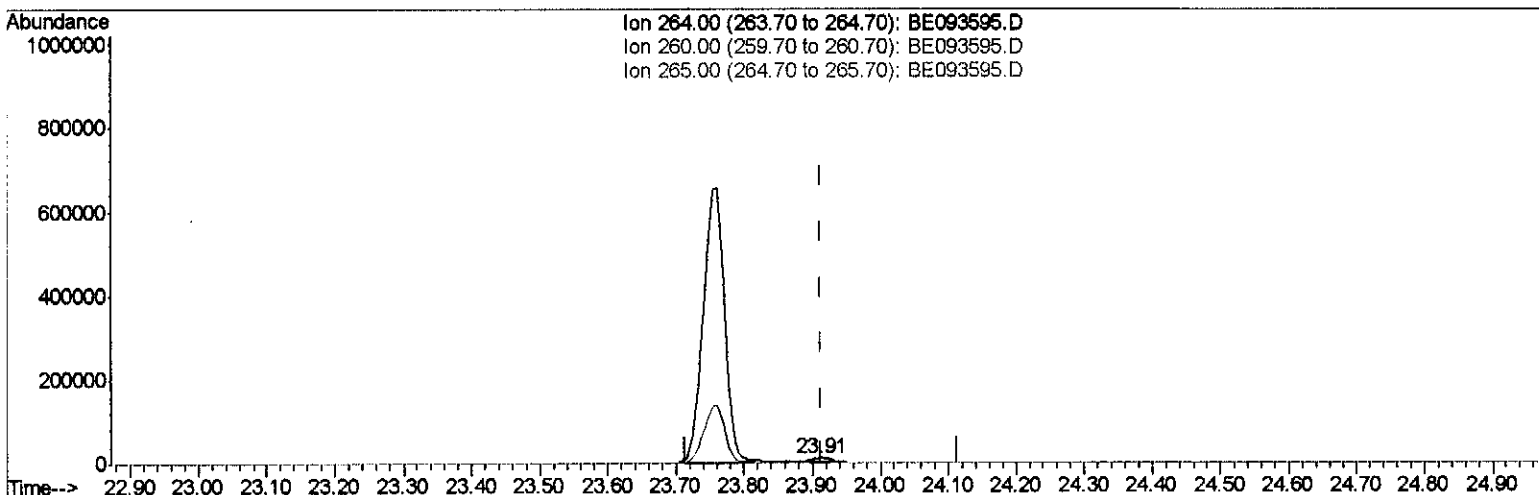

TIC: BE093595.D

(20) Perylene-d12 (I)

23.910min (-0.004) 0.40ng/ul m

SJ 8/8/17

response 19945

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.14
265.00	103.50	25.43#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE072517\
Data File : BE093595.D
Acq On : 26 Jul 2017 2:13
Operator : SJ/JU
Sample : I4373-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
7/26/2017 5:56:17 PM

Quant Time: Jul 26 06:04:42 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 05:32:22 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2620	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	13797	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	9051	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	20585m	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	21934	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	19945m	0.40	ng/ul	0.00

51 8/8/17

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.29	152	5720	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	18372	0.28	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed