


Data Path : Z:\HPCHEM1\BNA_E\Data\BE072617\
Data File : BE093599.D
Acq On : 26 Jul 2017 11:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 21 16:13:20 2017

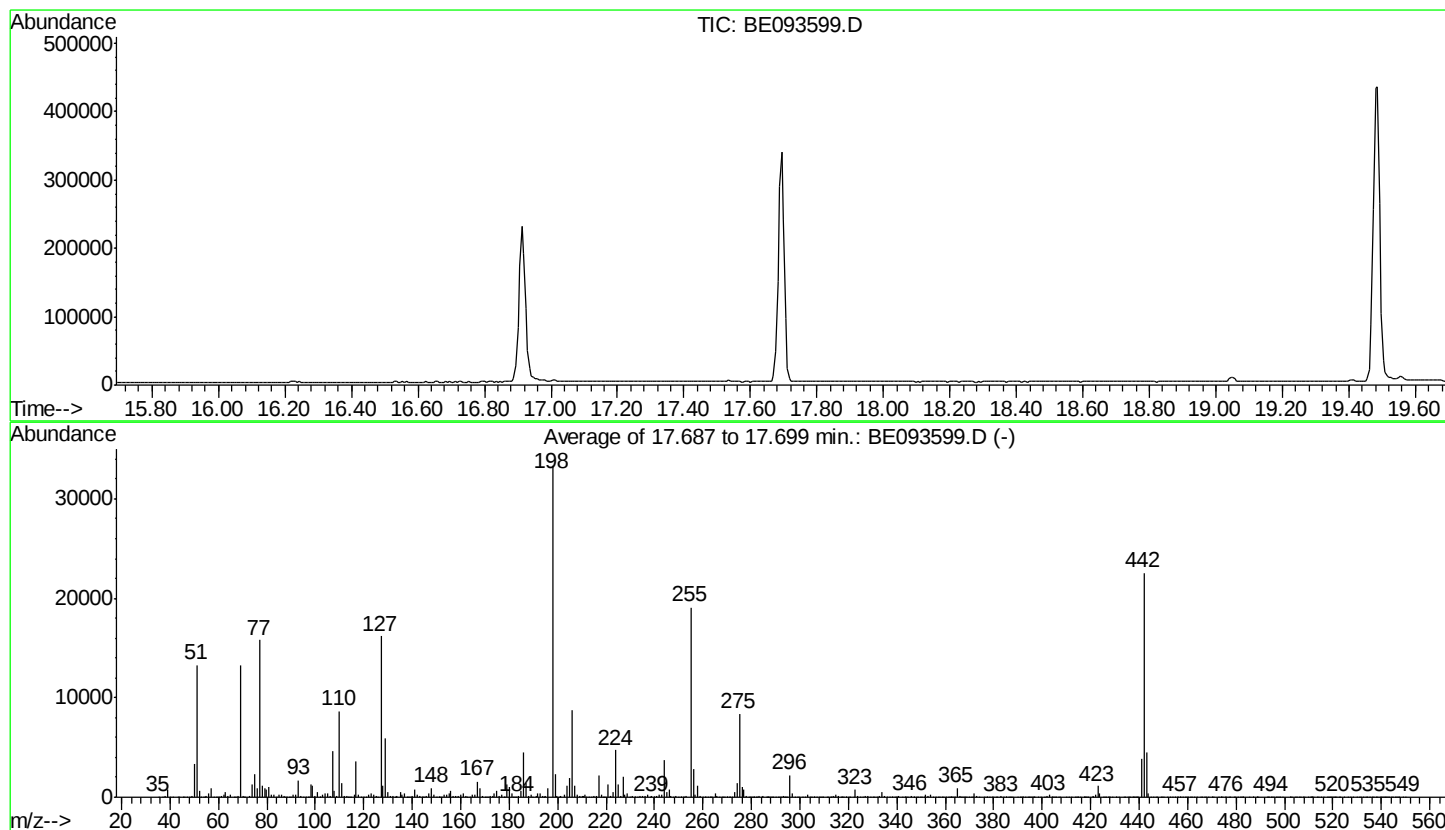

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	13270	PASS
68	69	0.00	2	1.0	134	PASS
69	198	0.00	100	39.7	13229	PASS
70	69	0.00	2	0.7	96	PASS
127	198	10	80	48.5	16170	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33337	PASS
199	198	5	9	6.9	2285	PASS
275	198	10	60	25.2	8407	PASS
365	198	1	100	2.8	920	PASS
441	442	0.01	24	17.2	3881	PASS
442	198	50	100	67.7	22556	PASS
443	442	15	24	20.0	4521	PASS