


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072716\
Data File : BE092047.D
Acq On : 27 Jul 2016 8:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 27 17:13:26 2016

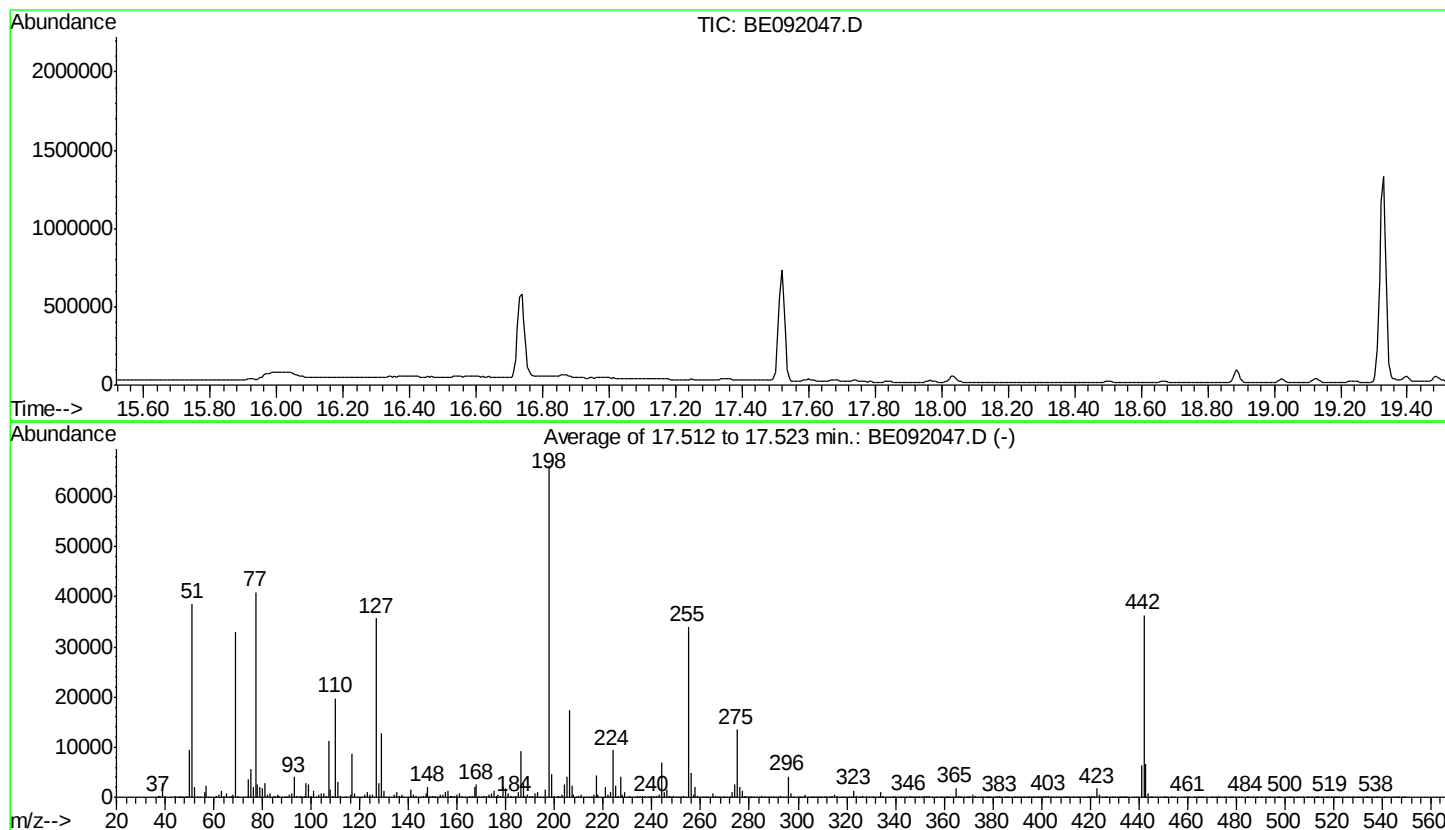

AutoFind: Scans 2540, 2541, 2542; Background Corrected with Scan 2534

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.4	38649	PASS
68	69	0.00	2	1.7	553	PASS
69	198	0.00	100	49.9	33013	PASS
70	69	0.00	2	0.4	139	PASS
127	198	10	80	54.0	35743	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66176	PASS
199	198	5	9	6.8	4523	PASS
275	198	10	60	20.4	13512	PASS
365	198	1	100	2.7	1805	PASS
441	442	0.01	24	17.5	6357	PASS
442	198	50	100	54.8	36282	PASS
443	442	15	24	18.5	6703	PASS