


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072716\
 Data File : BE092063.D
 Acq On : 28 Jul 2016 1:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 27 17:13:26 2016

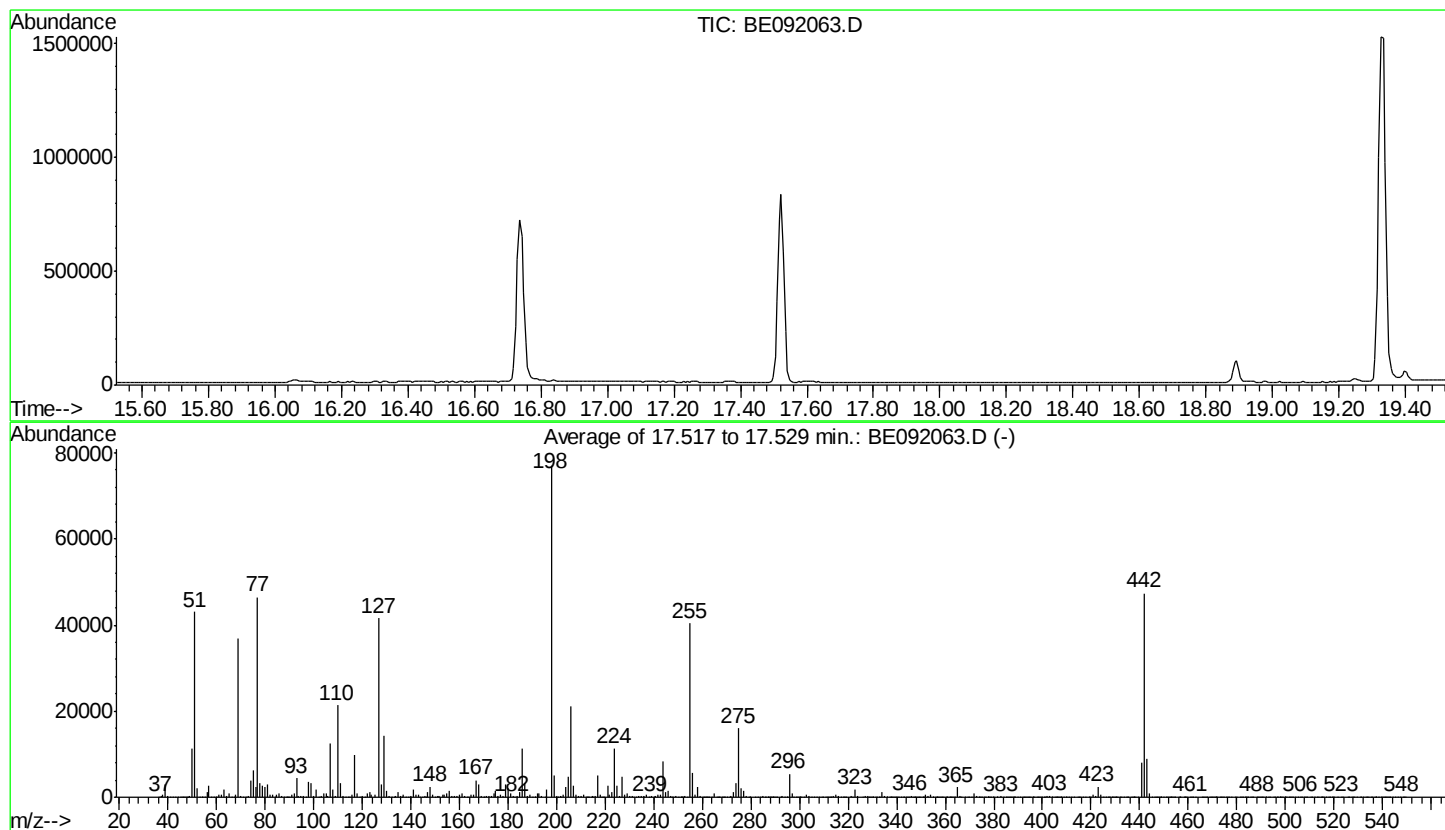

AutoFind: Scans 2541, 2542, 2543; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	43051	PASS
68	69	0.00	2	1.3	470	PASS
69	198	0.00	100	48.0	36989	PASS
70	69	0.00	2	0.5	180	PASS
127	198	10	80	53.9	41556	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77040	PASS
199	198	5	9	6.5	5045	PASS
275	198	10	60	20.8	16038	PASS
365	198	1	100	3.0	2296	PASS
441	442	0.01	24	17.3	8181	PASS
442	198	50	100	61.5	47406	PASS
443	442	15	24	19.0	9021	PASS