
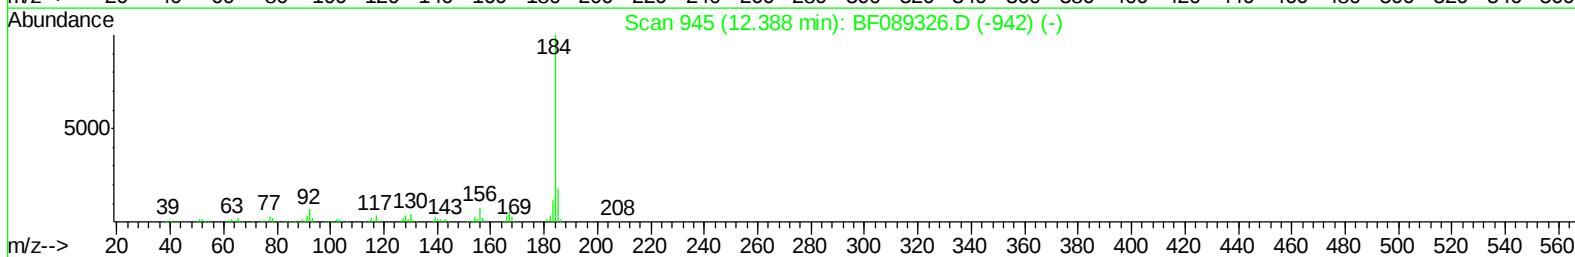
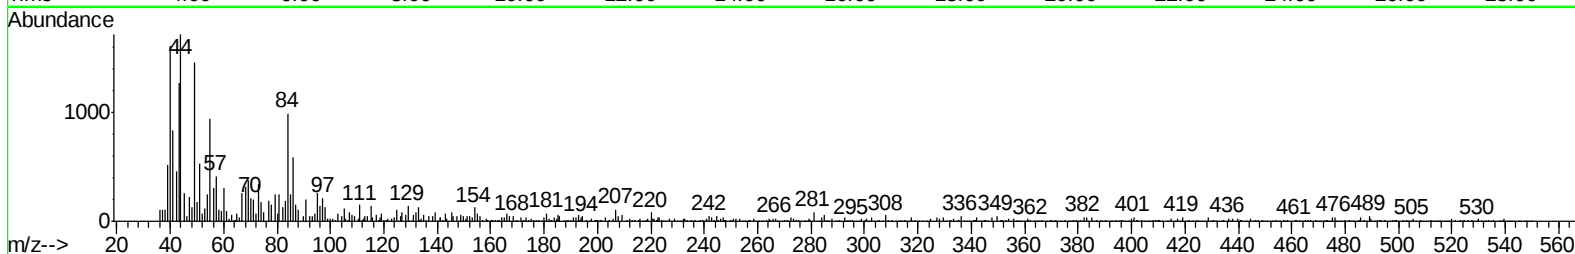


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080116\
Data File : BE092087.D
Acq On : 1 Aug 2016 11:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 05:22:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

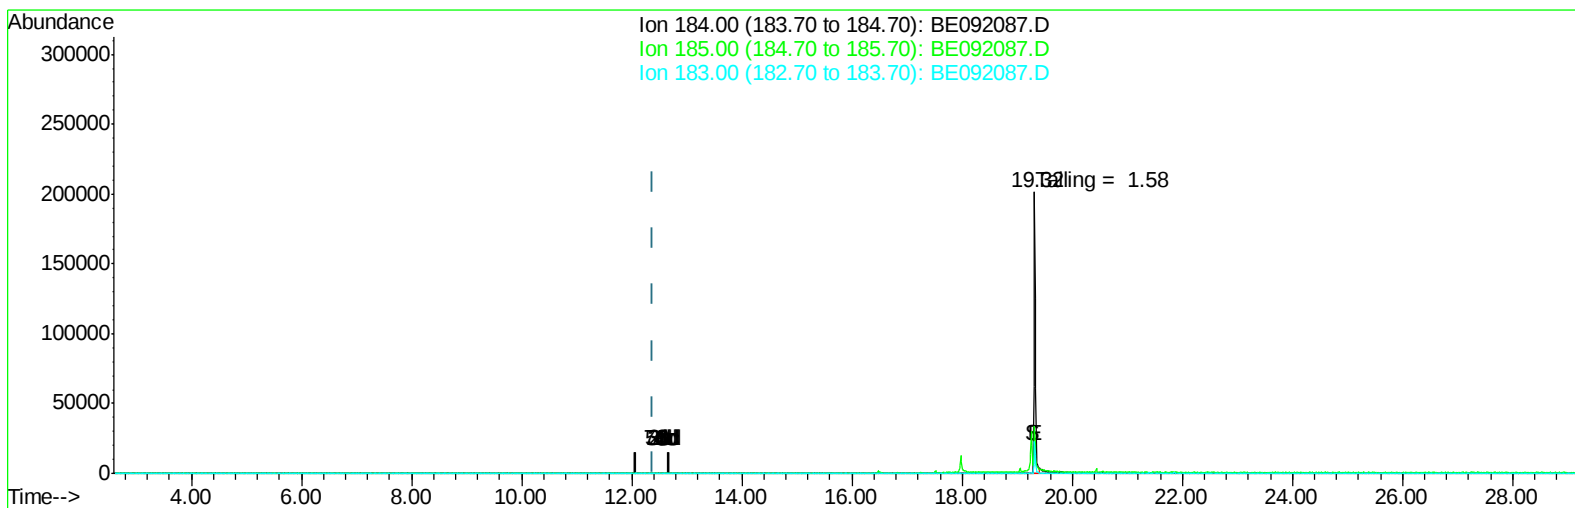

TIC: BE092087.D

(76) Benzidine




12.552min (+0.165) 234.55ng

response 52

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	110.91#
183.00	12.20	27.27#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080116\
Data File : BE092087.D
Acq On : 1 Aug 2016 11:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 05:22:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

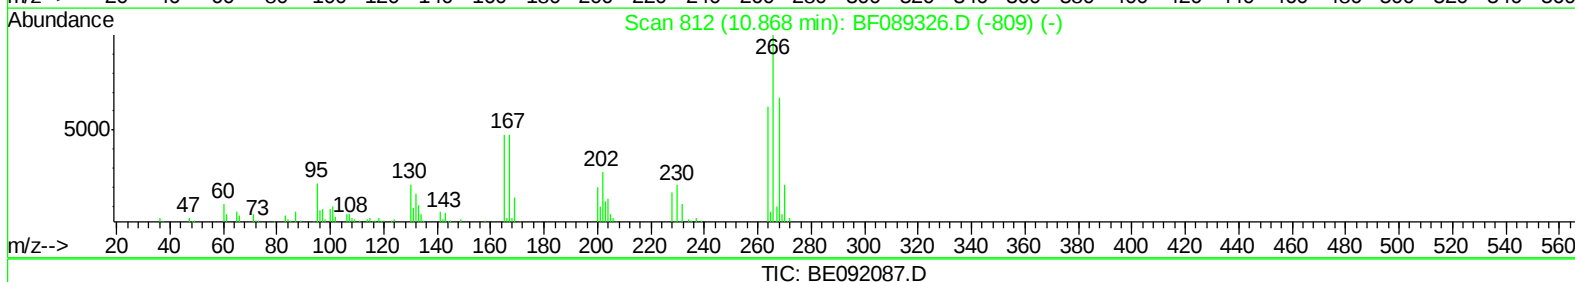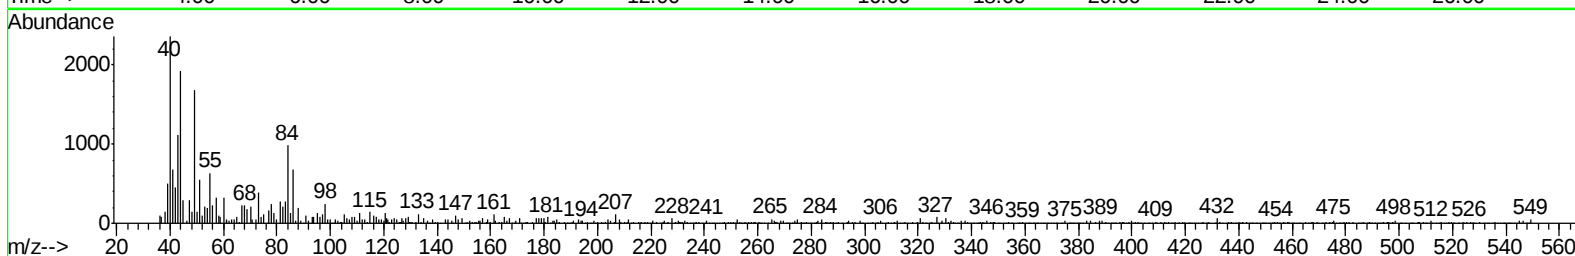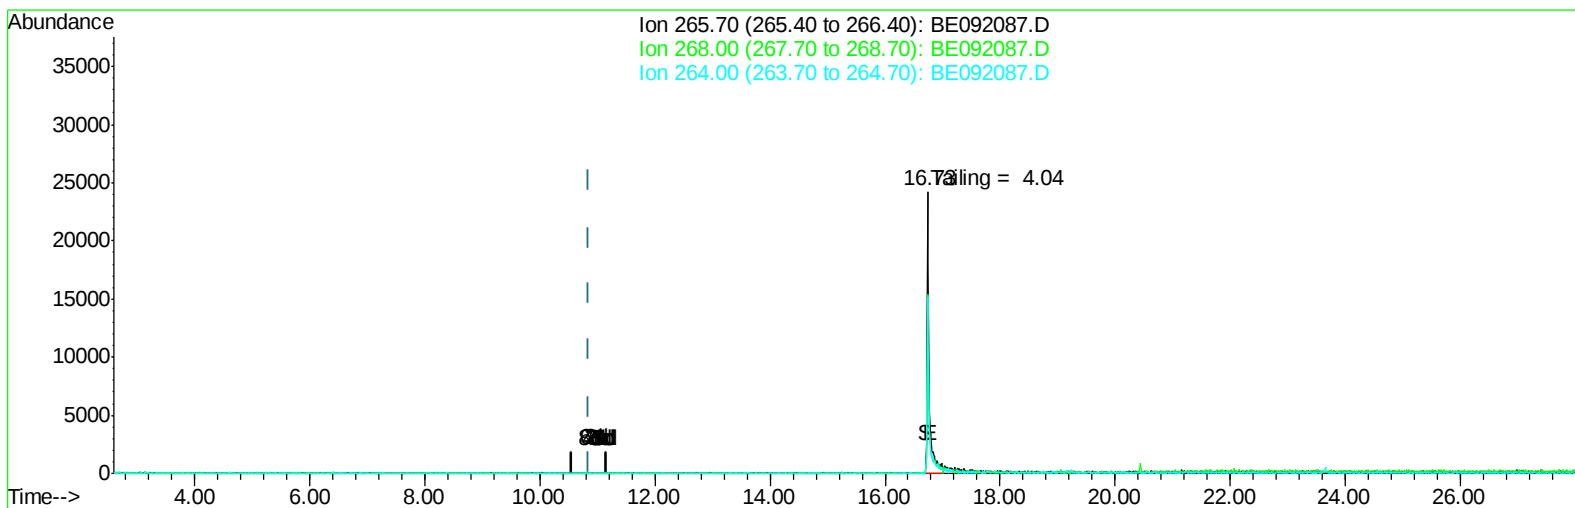

TIC: BE092087.D

(69) Pentachlorophenol (C)

11.018min (+0.151) 92.08ng

response 15

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	0.00#
264.00	62.70	13.79#
0.00	0.00	0.00