



1,4-Dioxane

Response Ratio

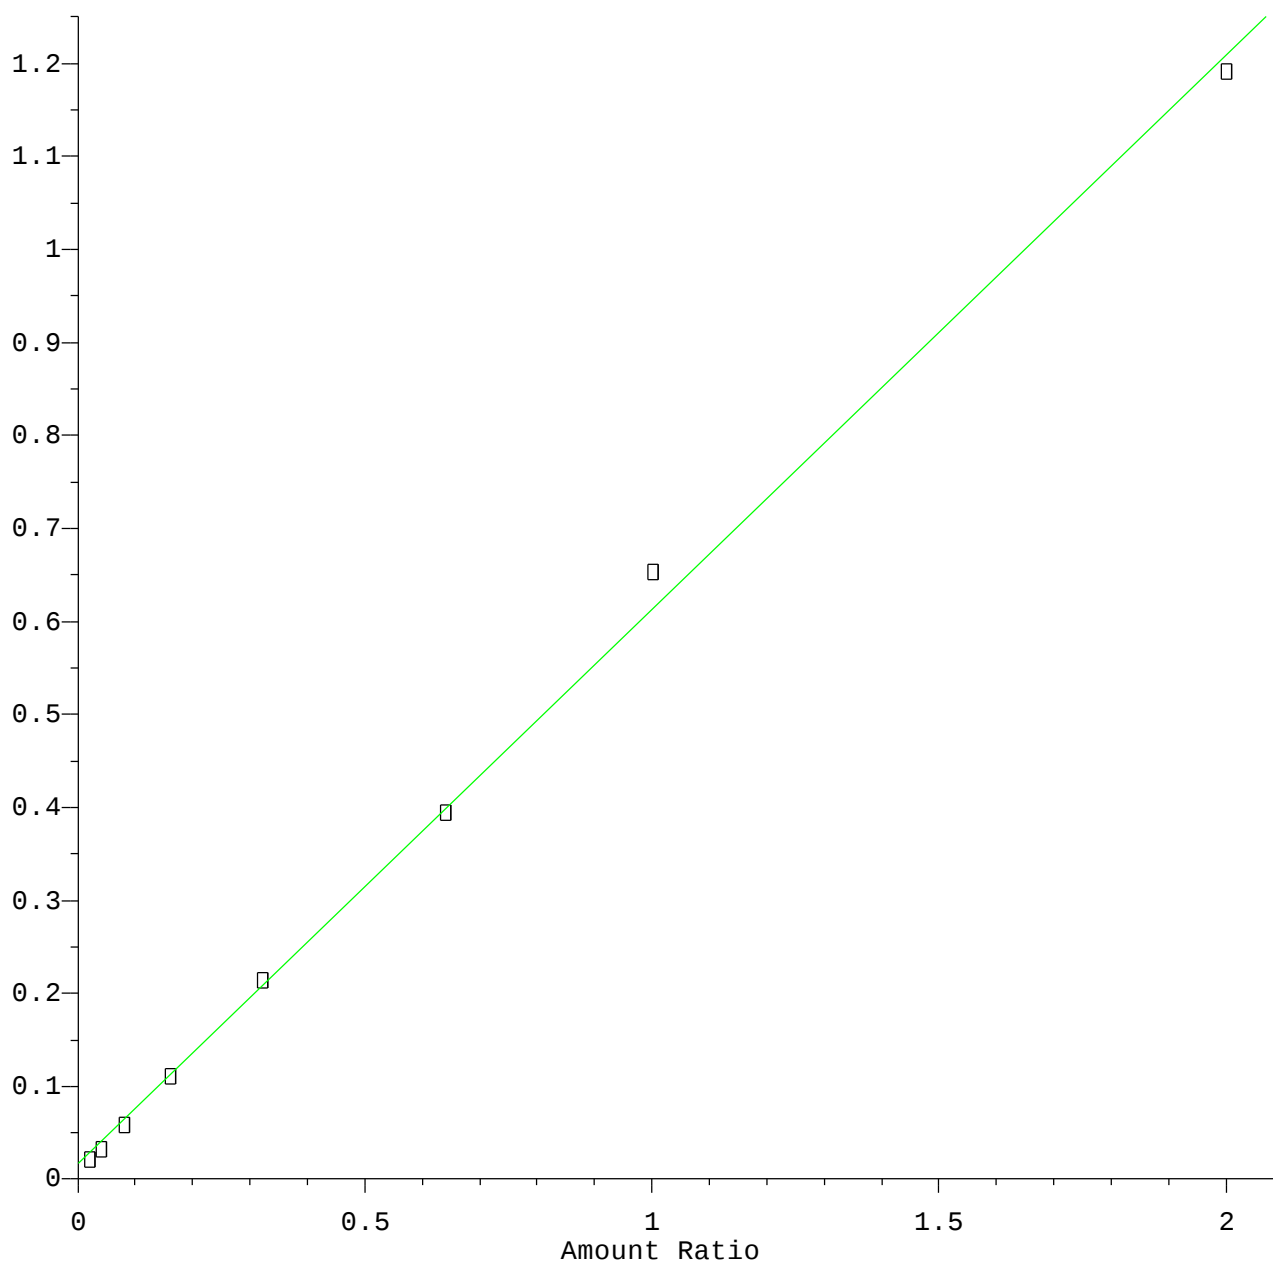


Resp Ratio = $5.97 \times 10^{-1} \times \text{Amt} + 1.60 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

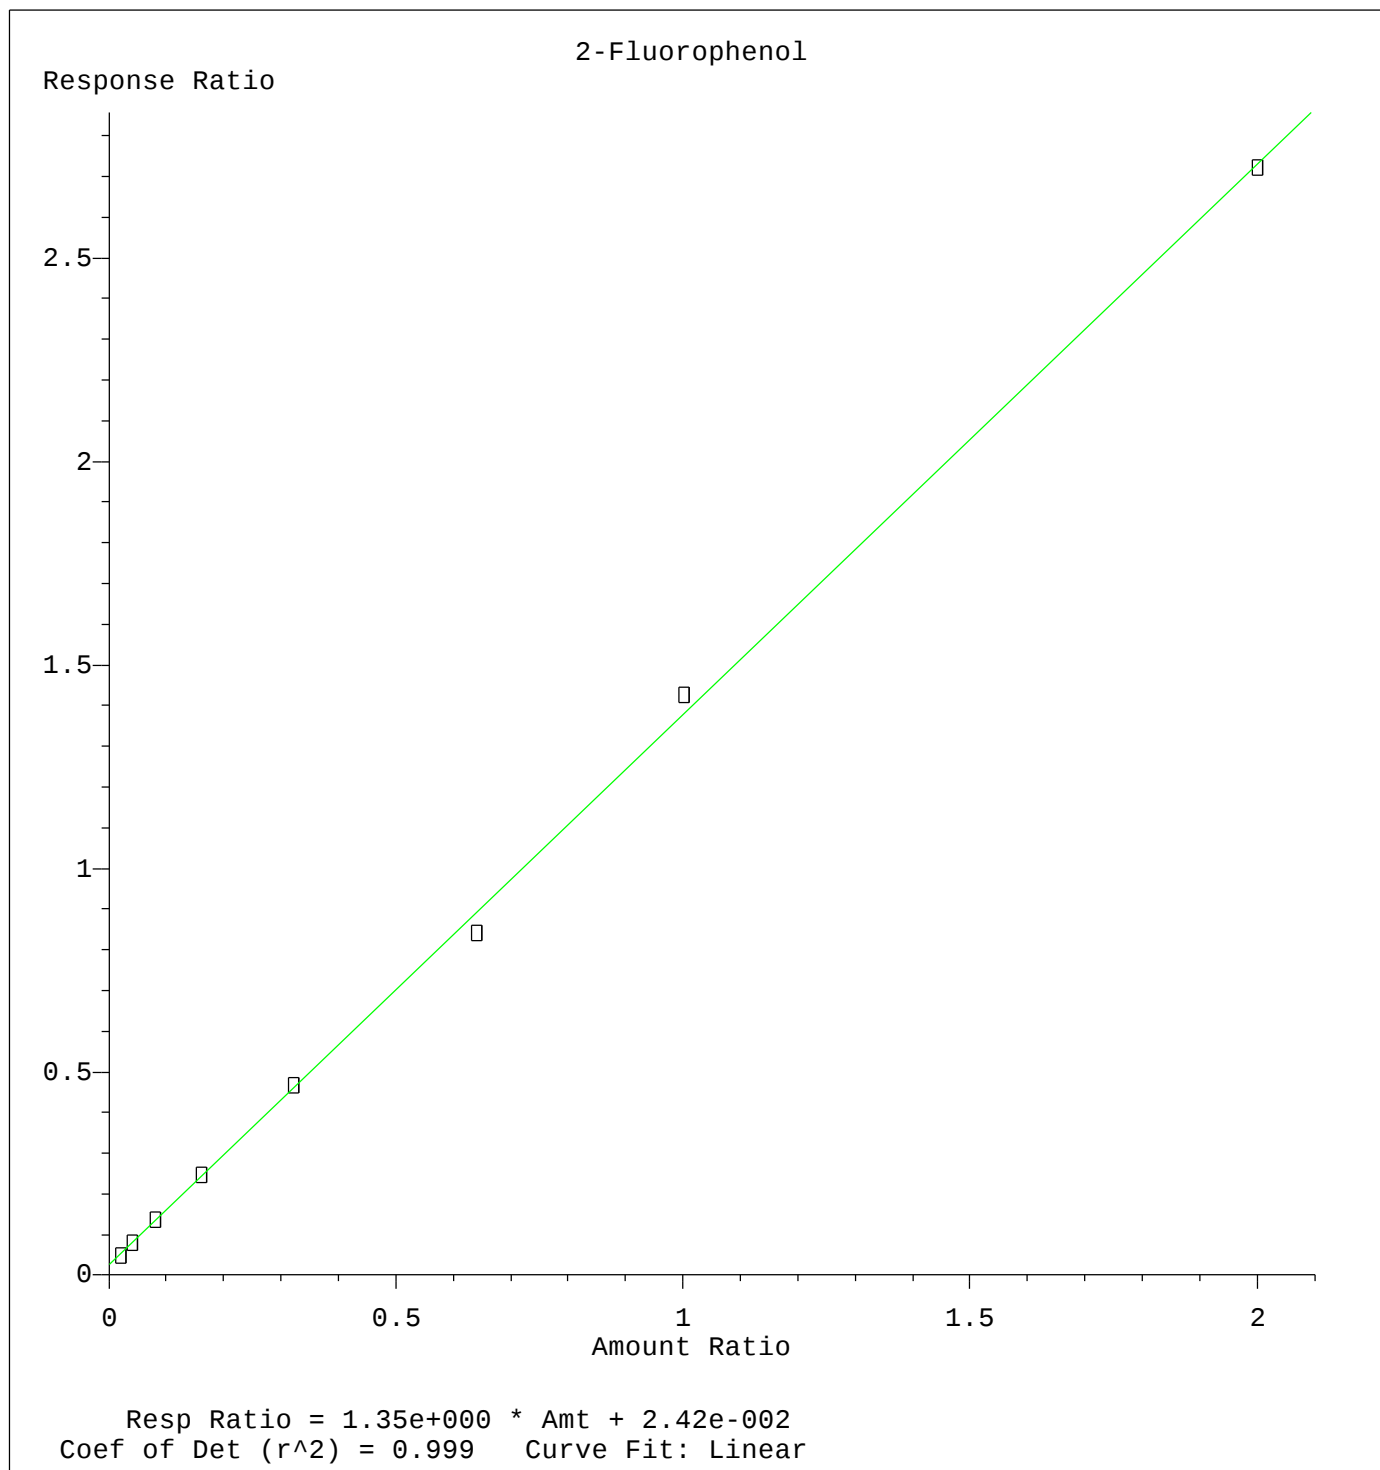

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

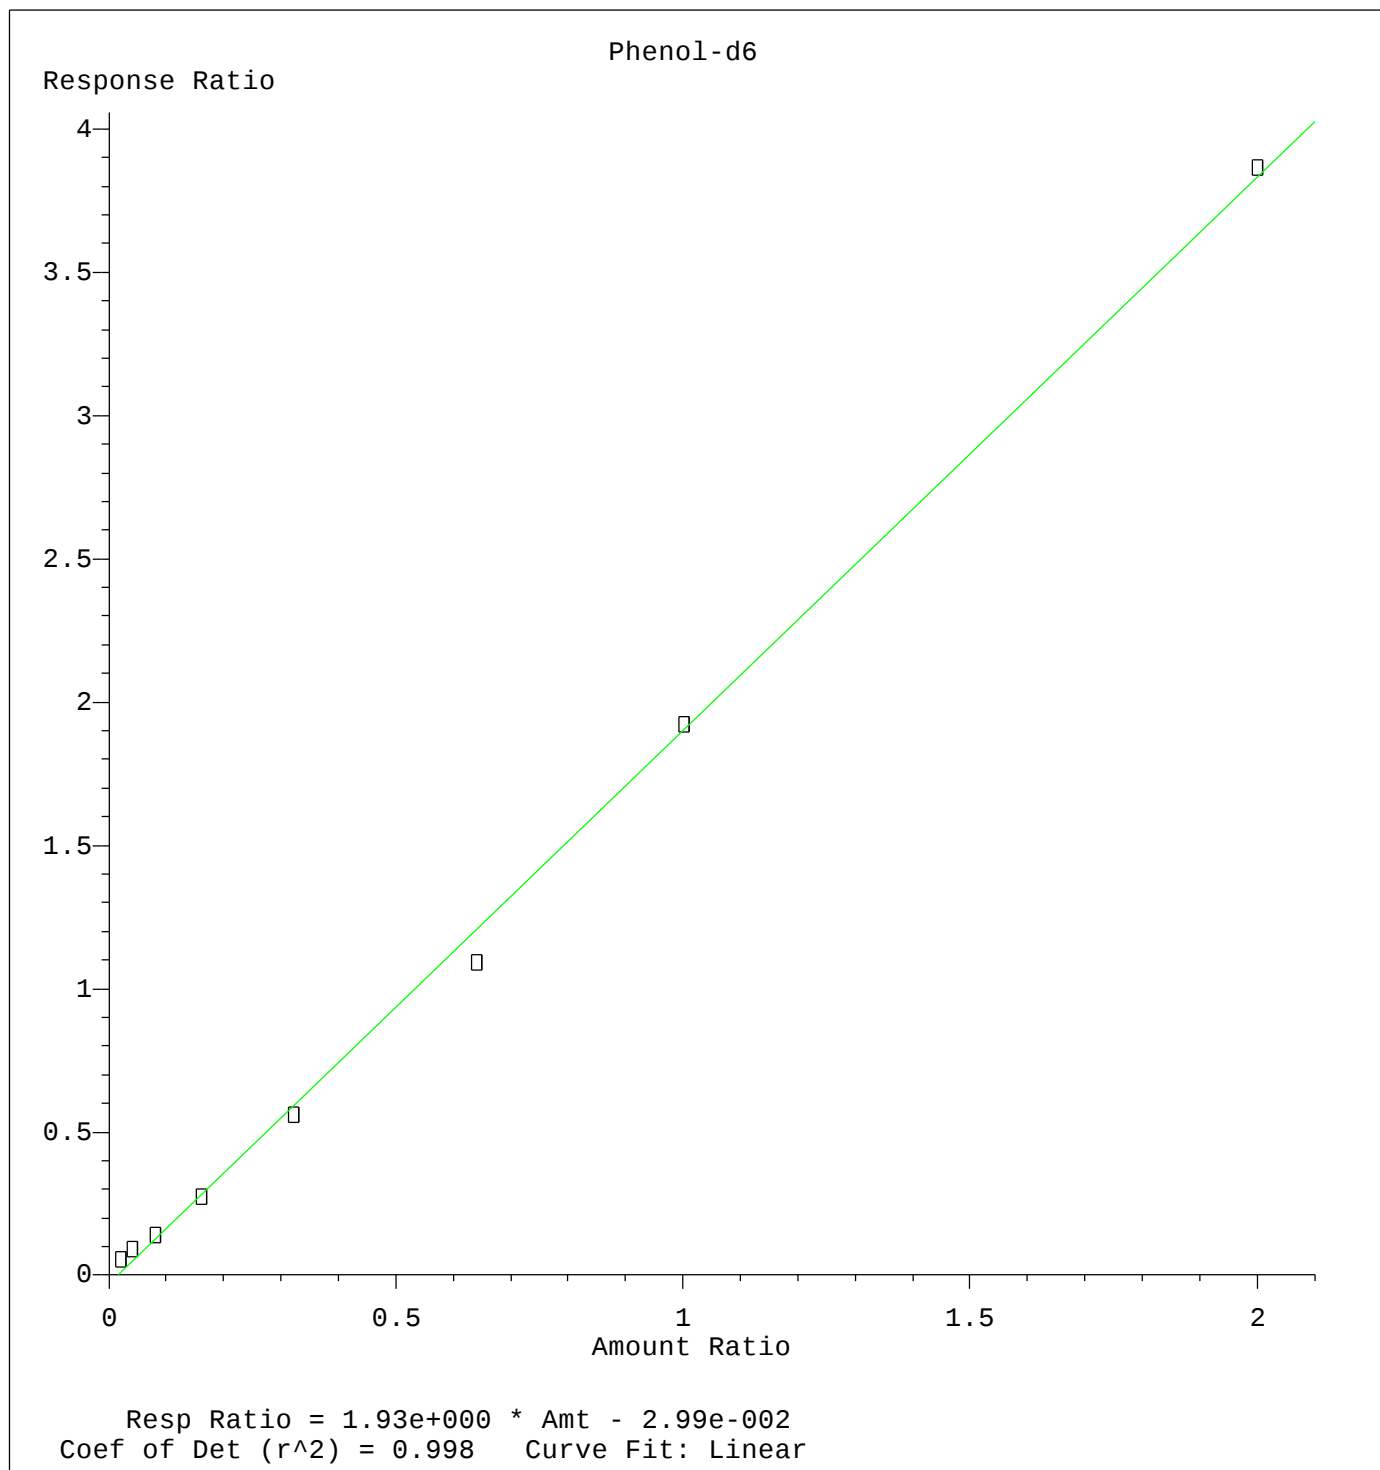


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

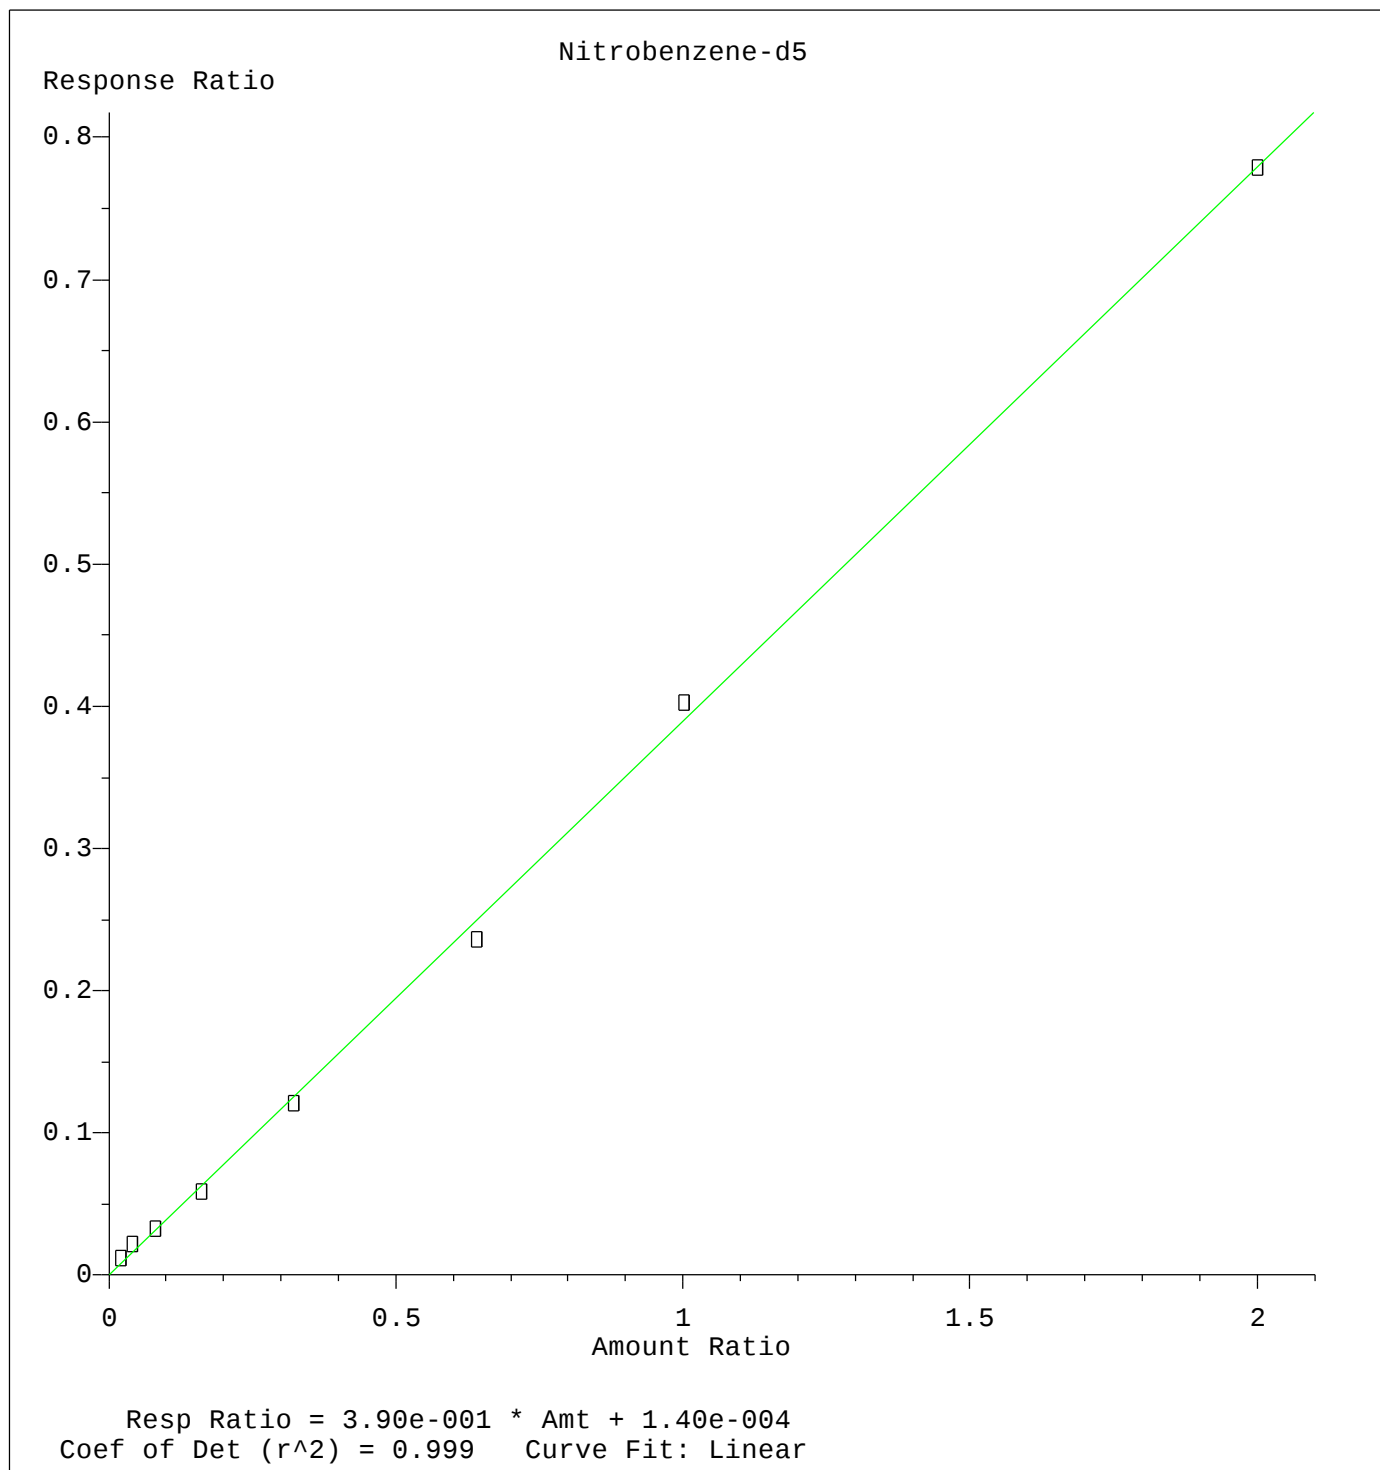

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

bis(2-Chloroethoxy)methane

Response Ratio

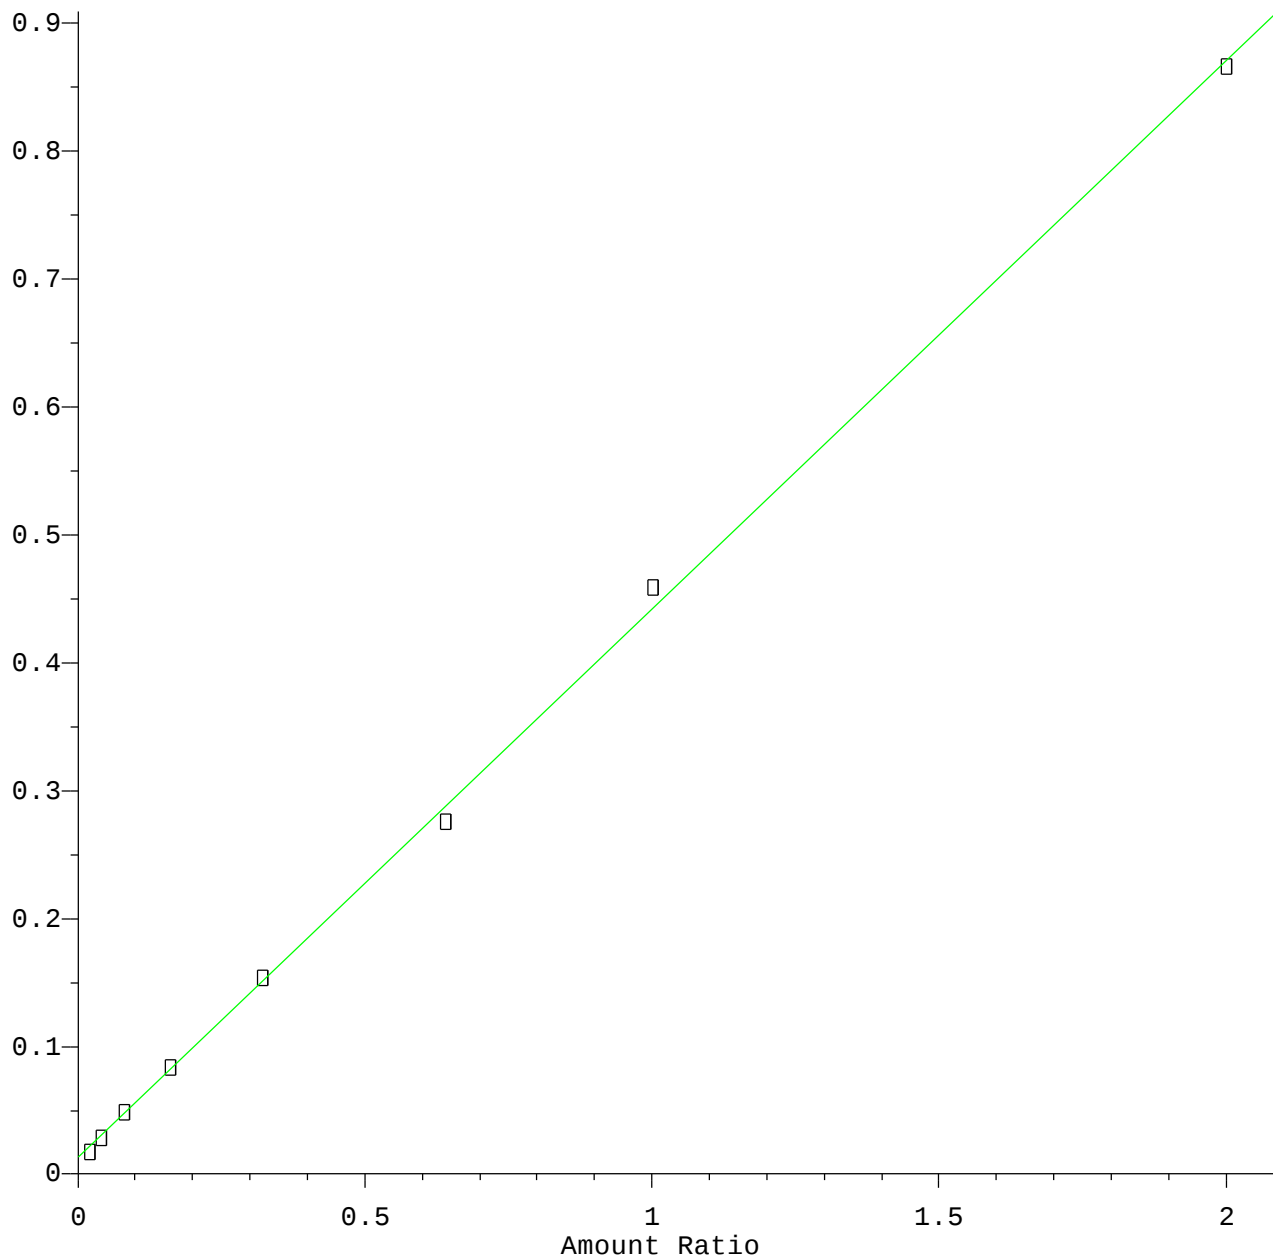


Resp Ratio = $4.29 \times 10^{-1} \times \text{Amt} + 1.26 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016


2,4,6-Tribromophenol

Response Ratio

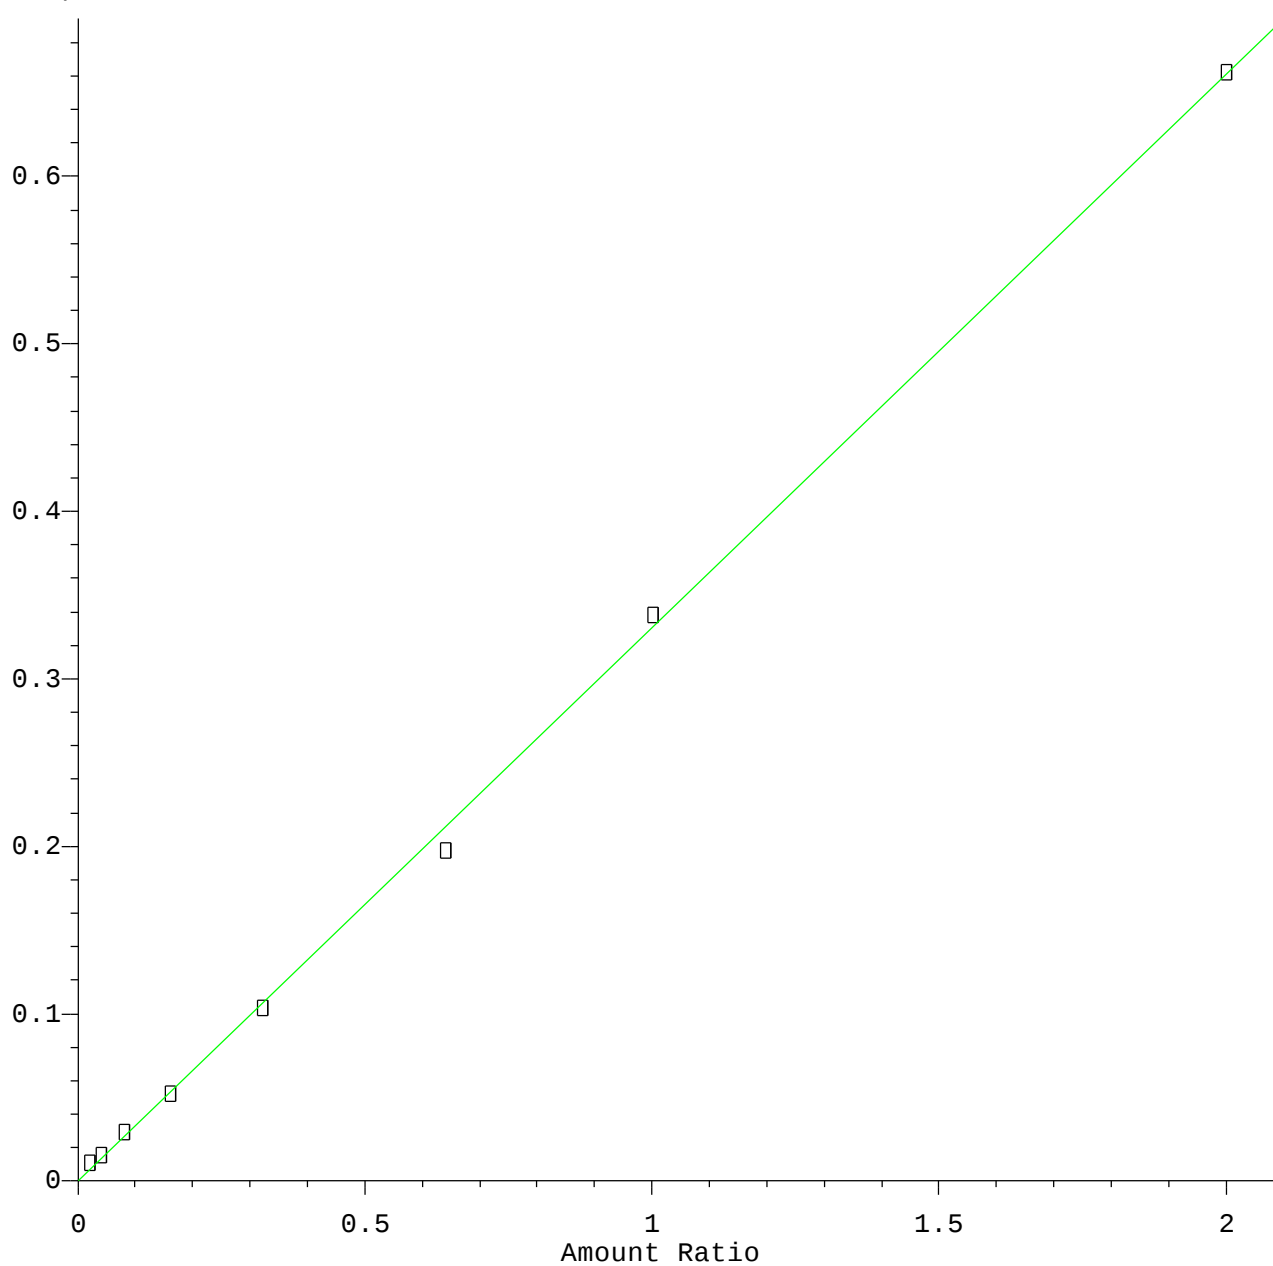


Resp Ratio = $3.30 \times 10^{-1} \times \text{Amt} - 5.91 \times 10^{-5}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

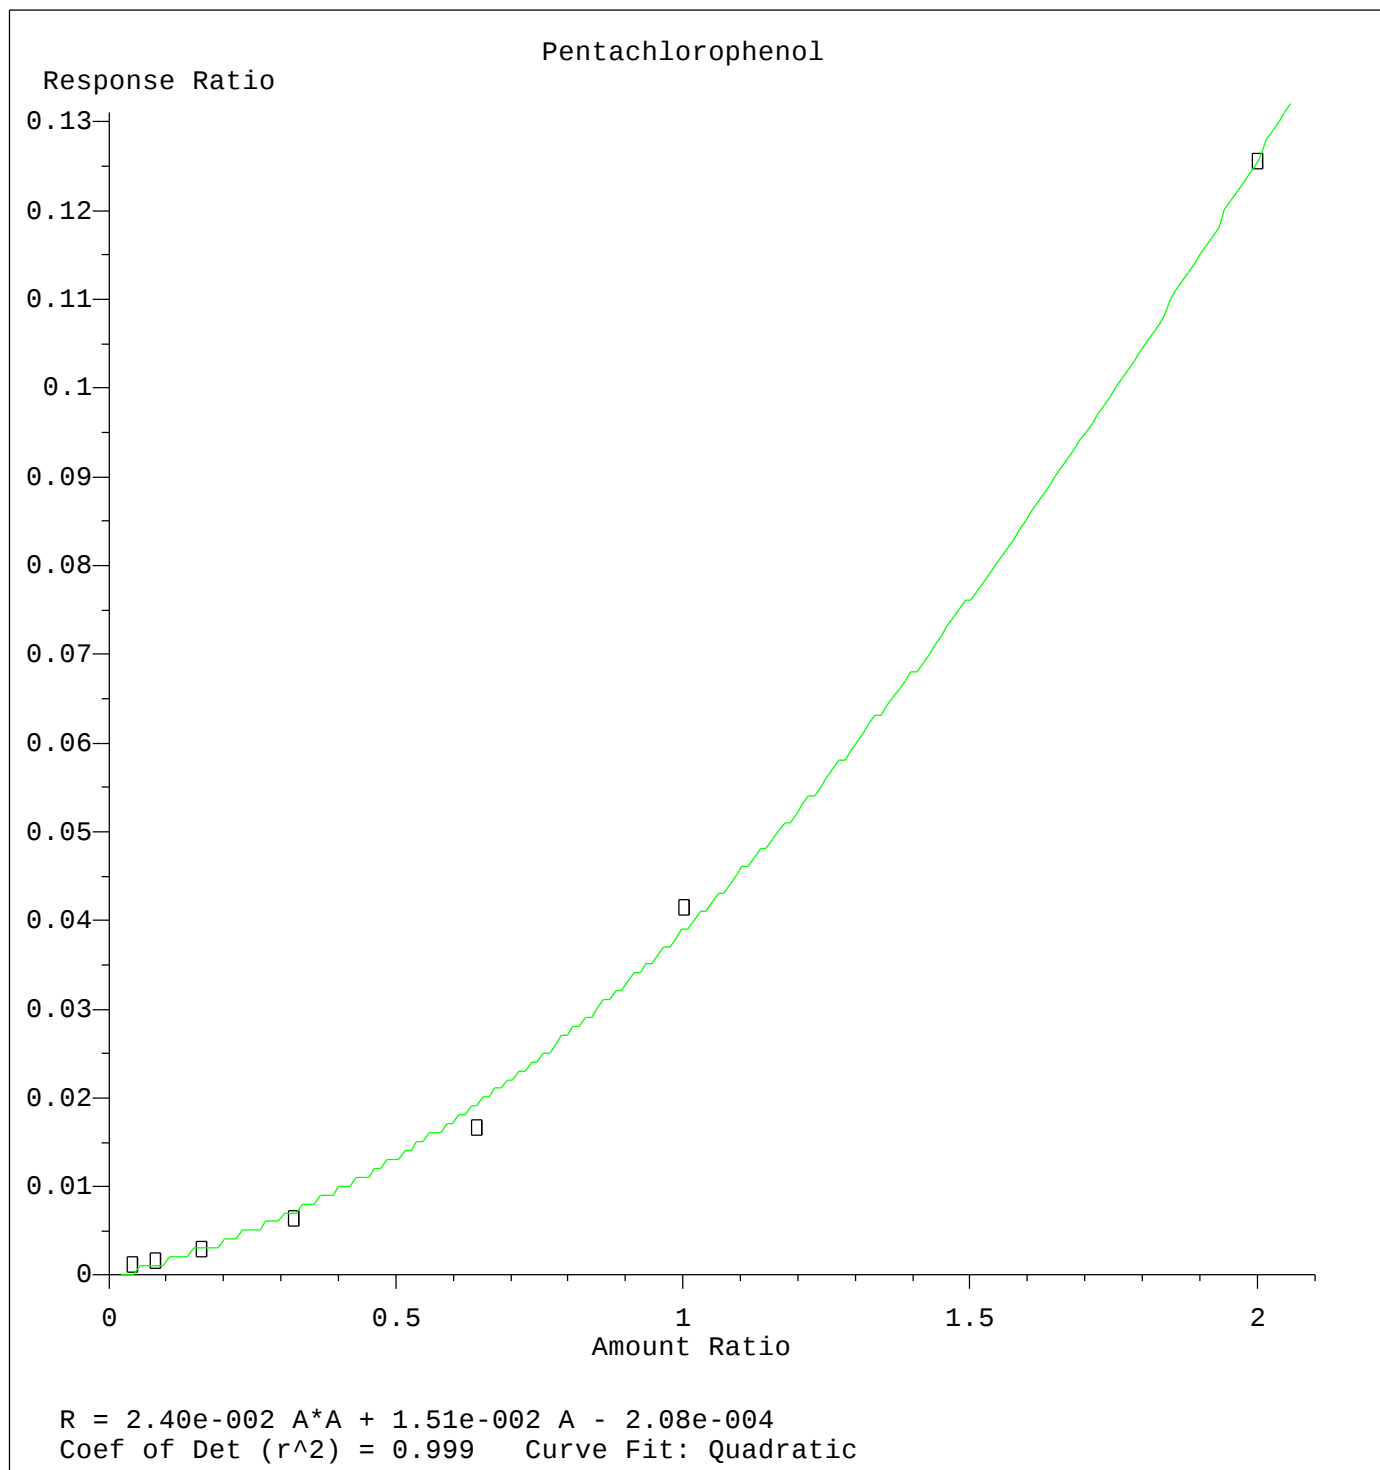


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

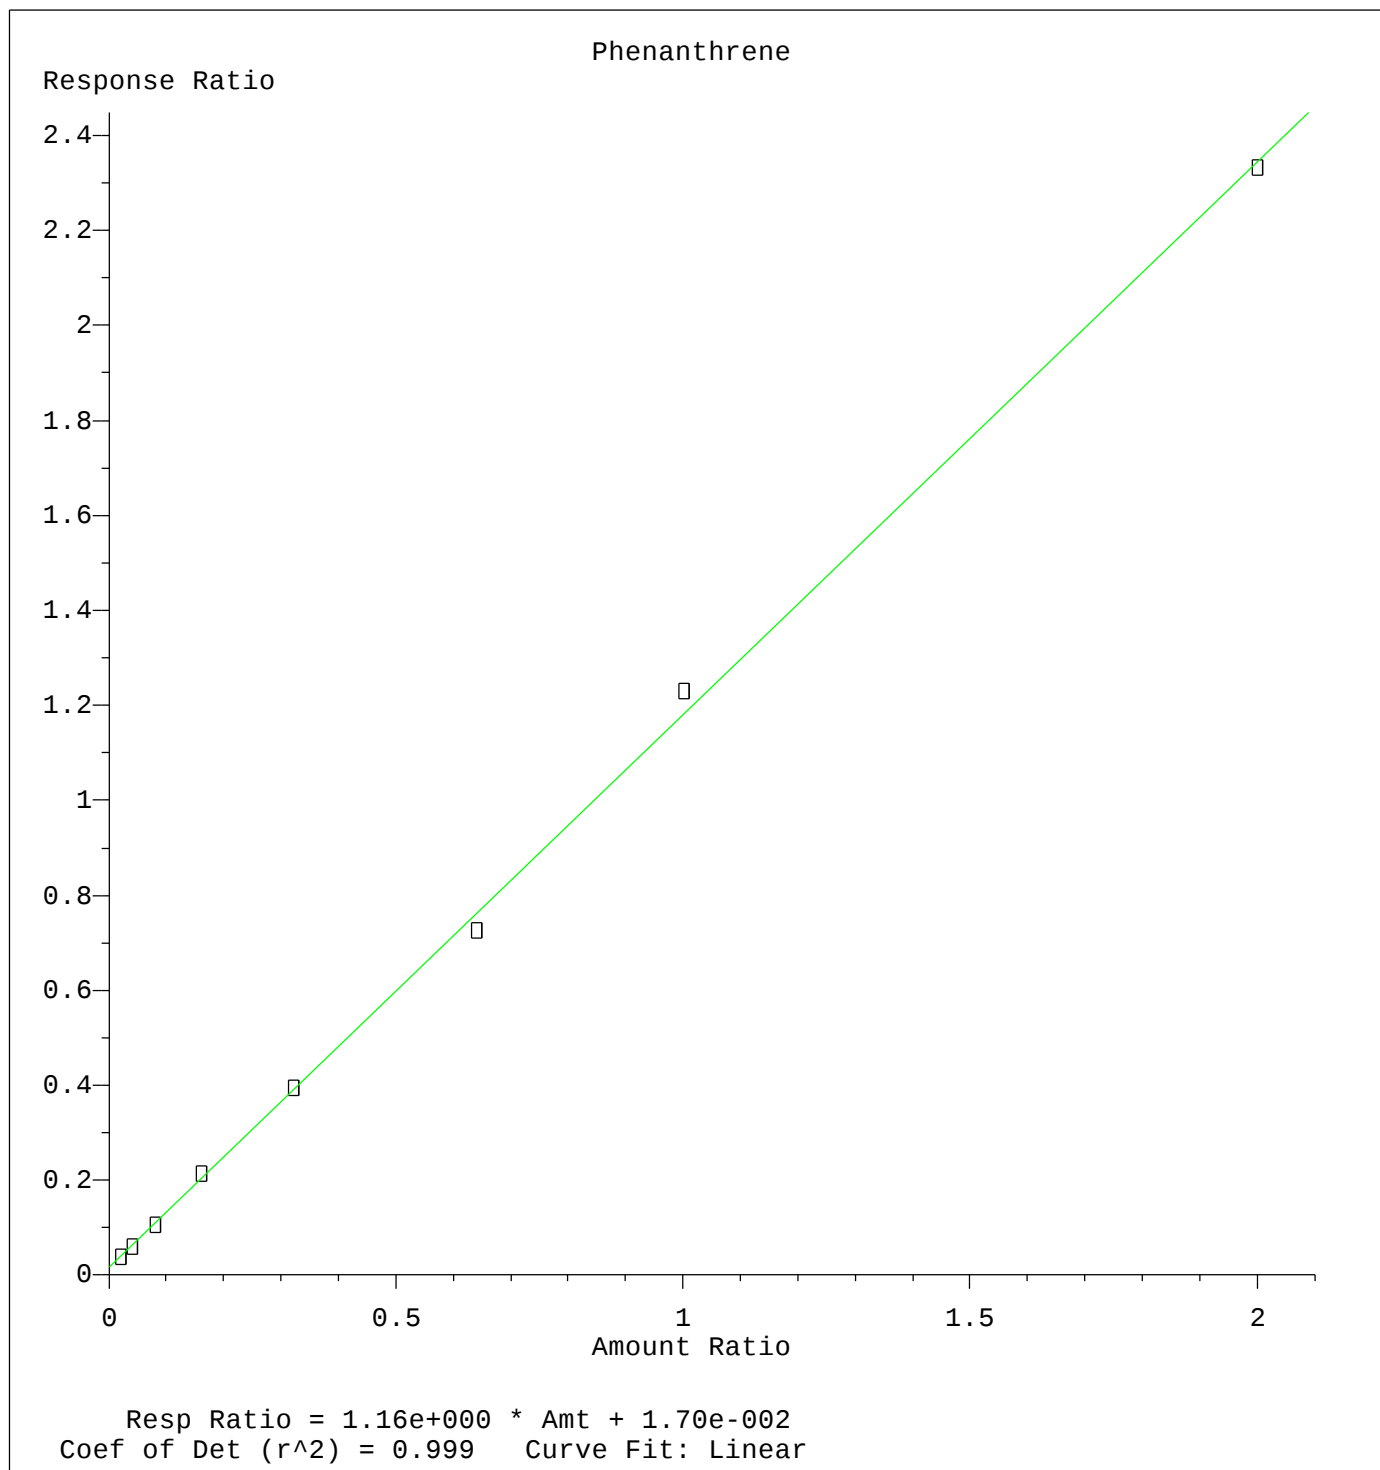

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016


Fluoranthene

Response Ratio

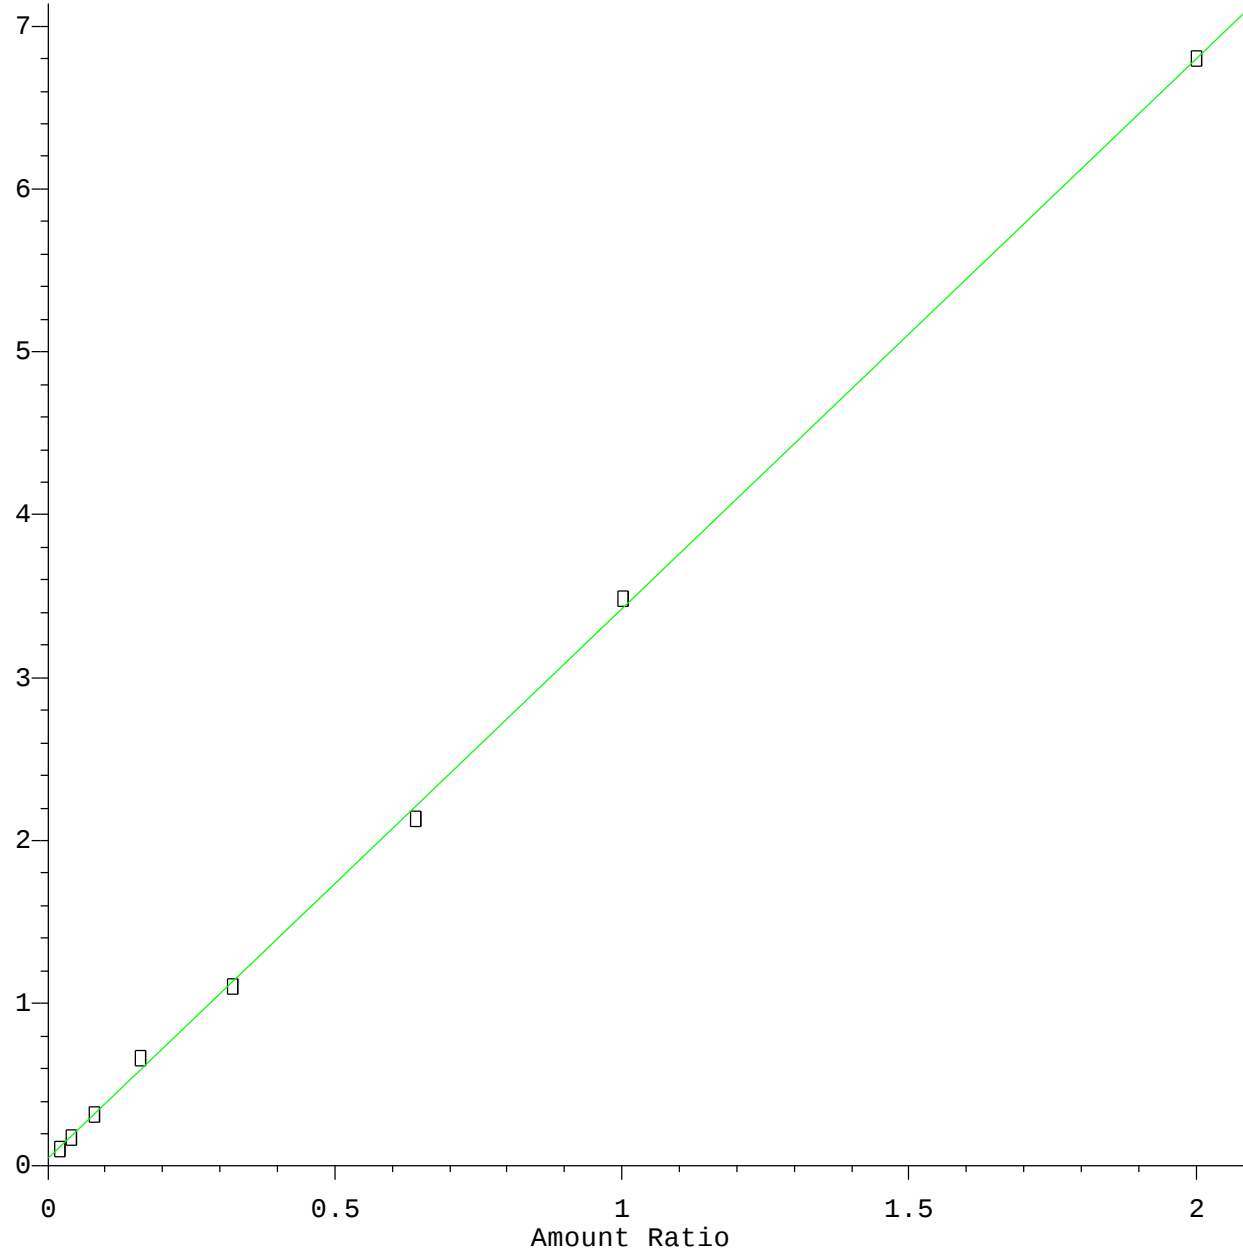


Resp Ratio = $3.38 \times 10^0 \times \text{Amt} + 4.73 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

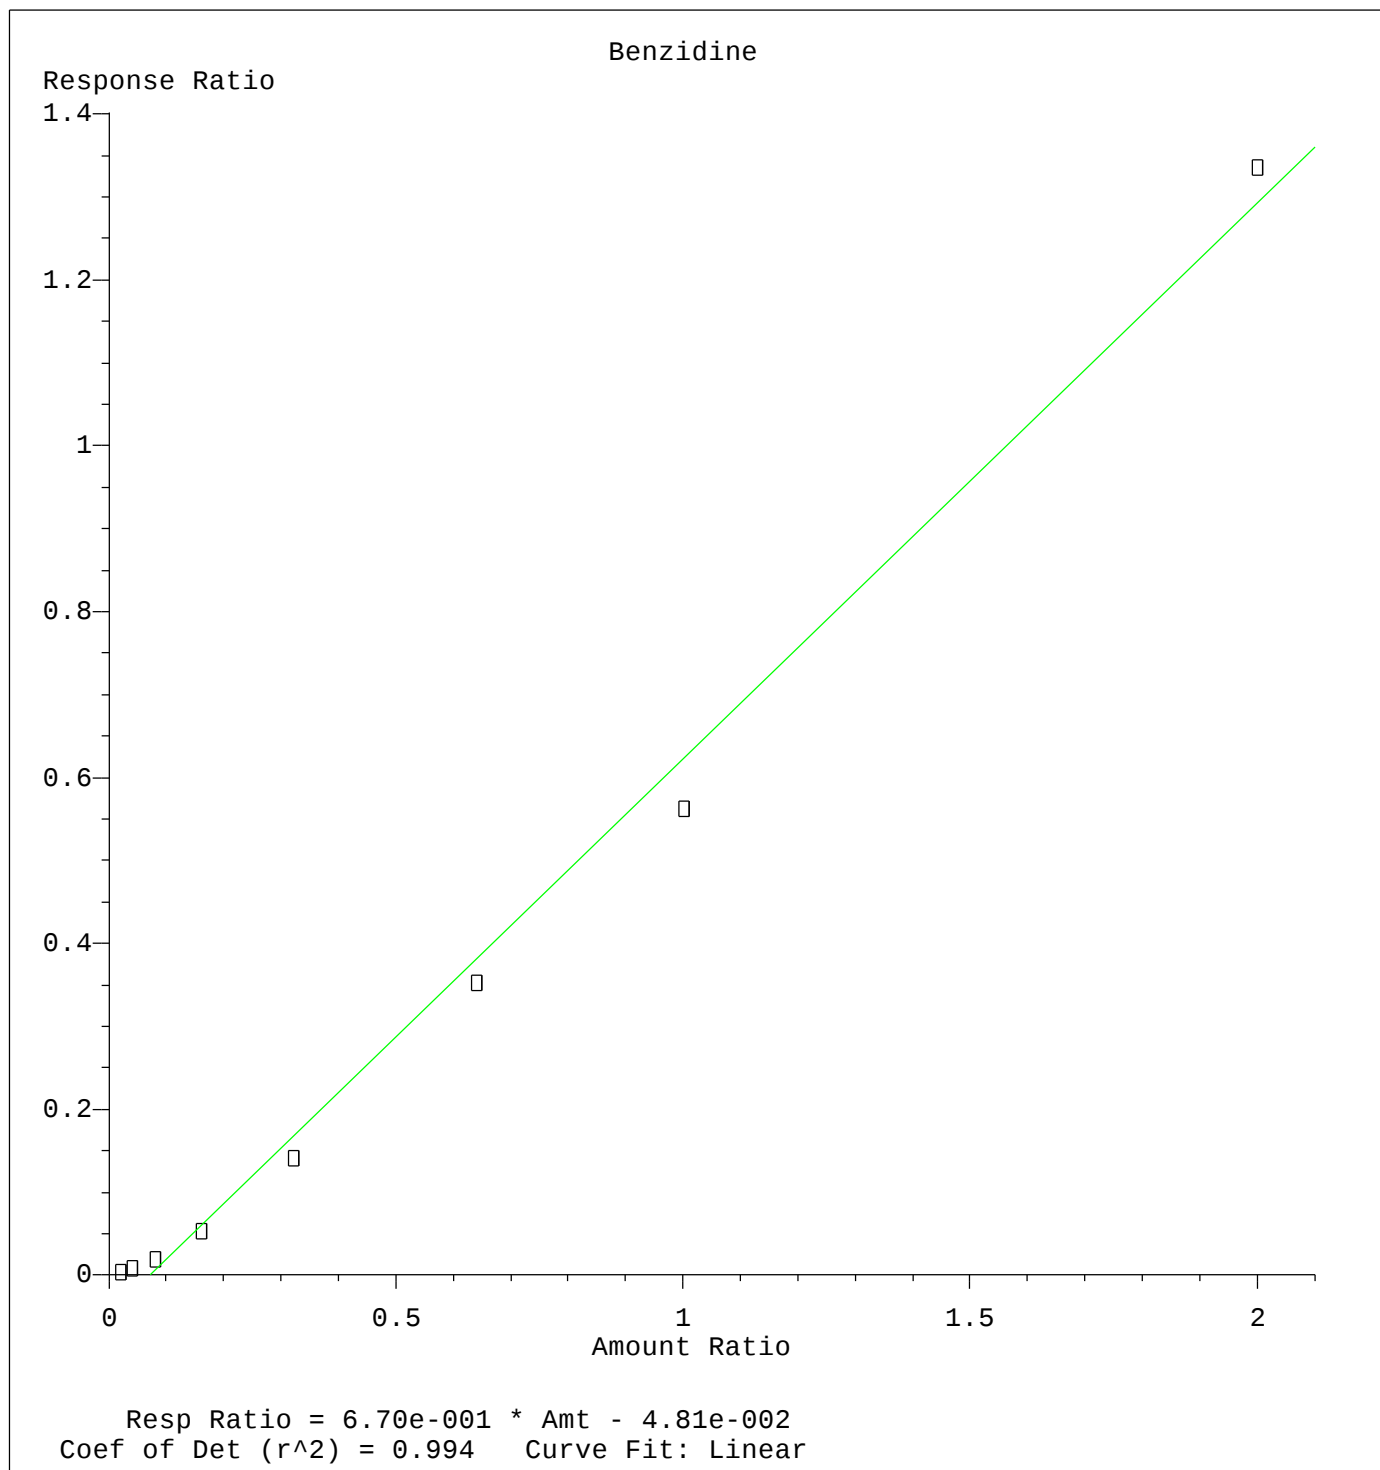


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

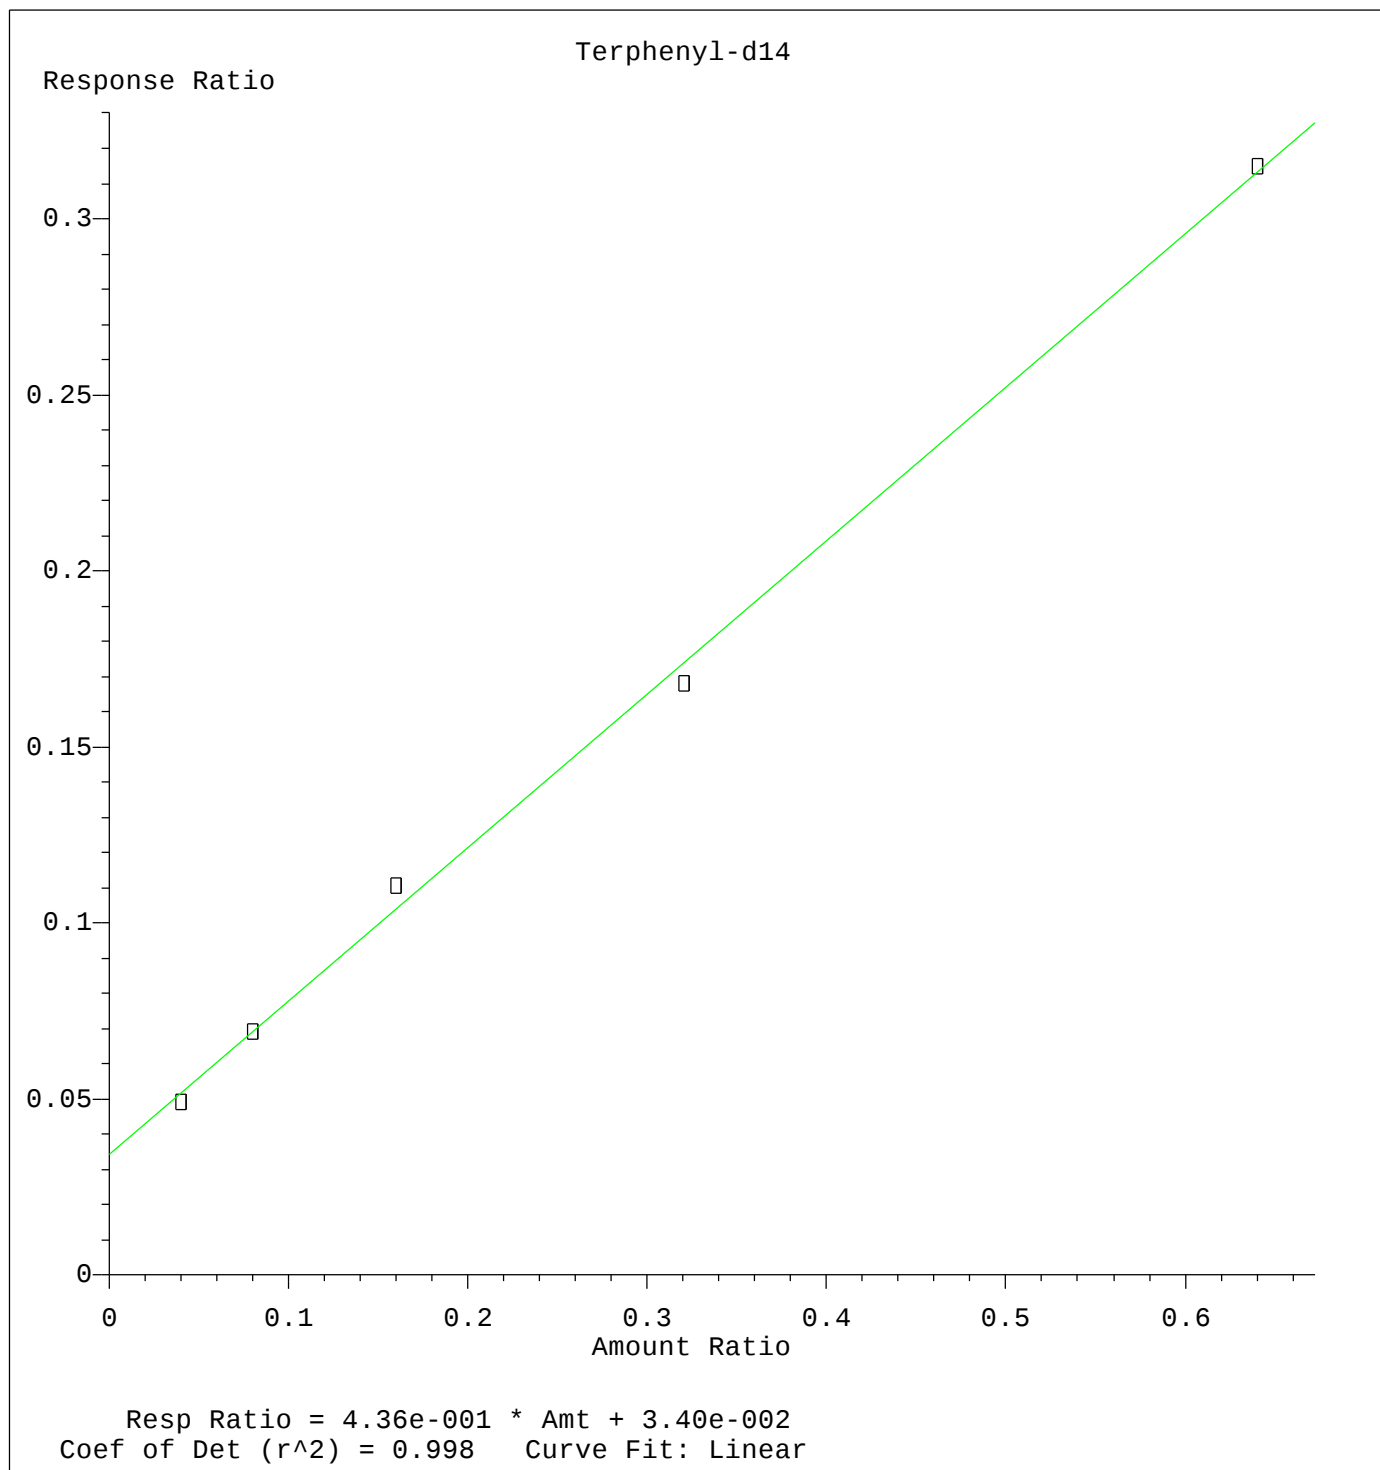

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

Benzo(a)anthracene

Response Ratio

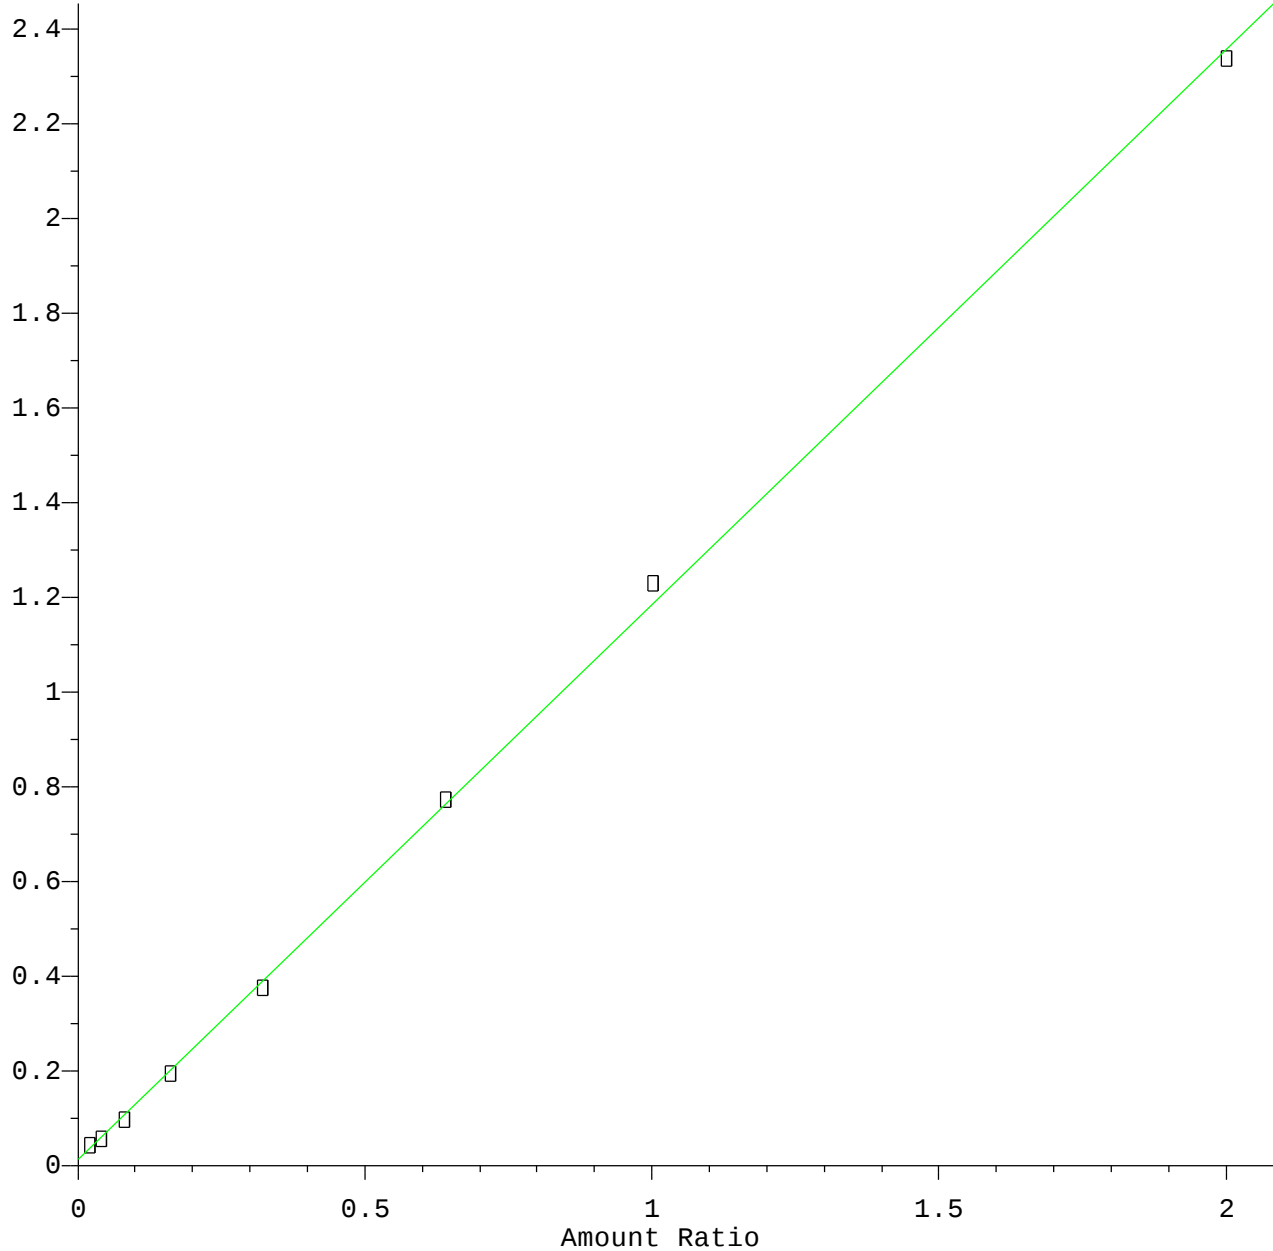


Resp Ratio = $1.17 \times 10^0 \times \text{Amt} + 1.45 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016


Bis(2-ethylhexyl)phthalate

Response Ratio

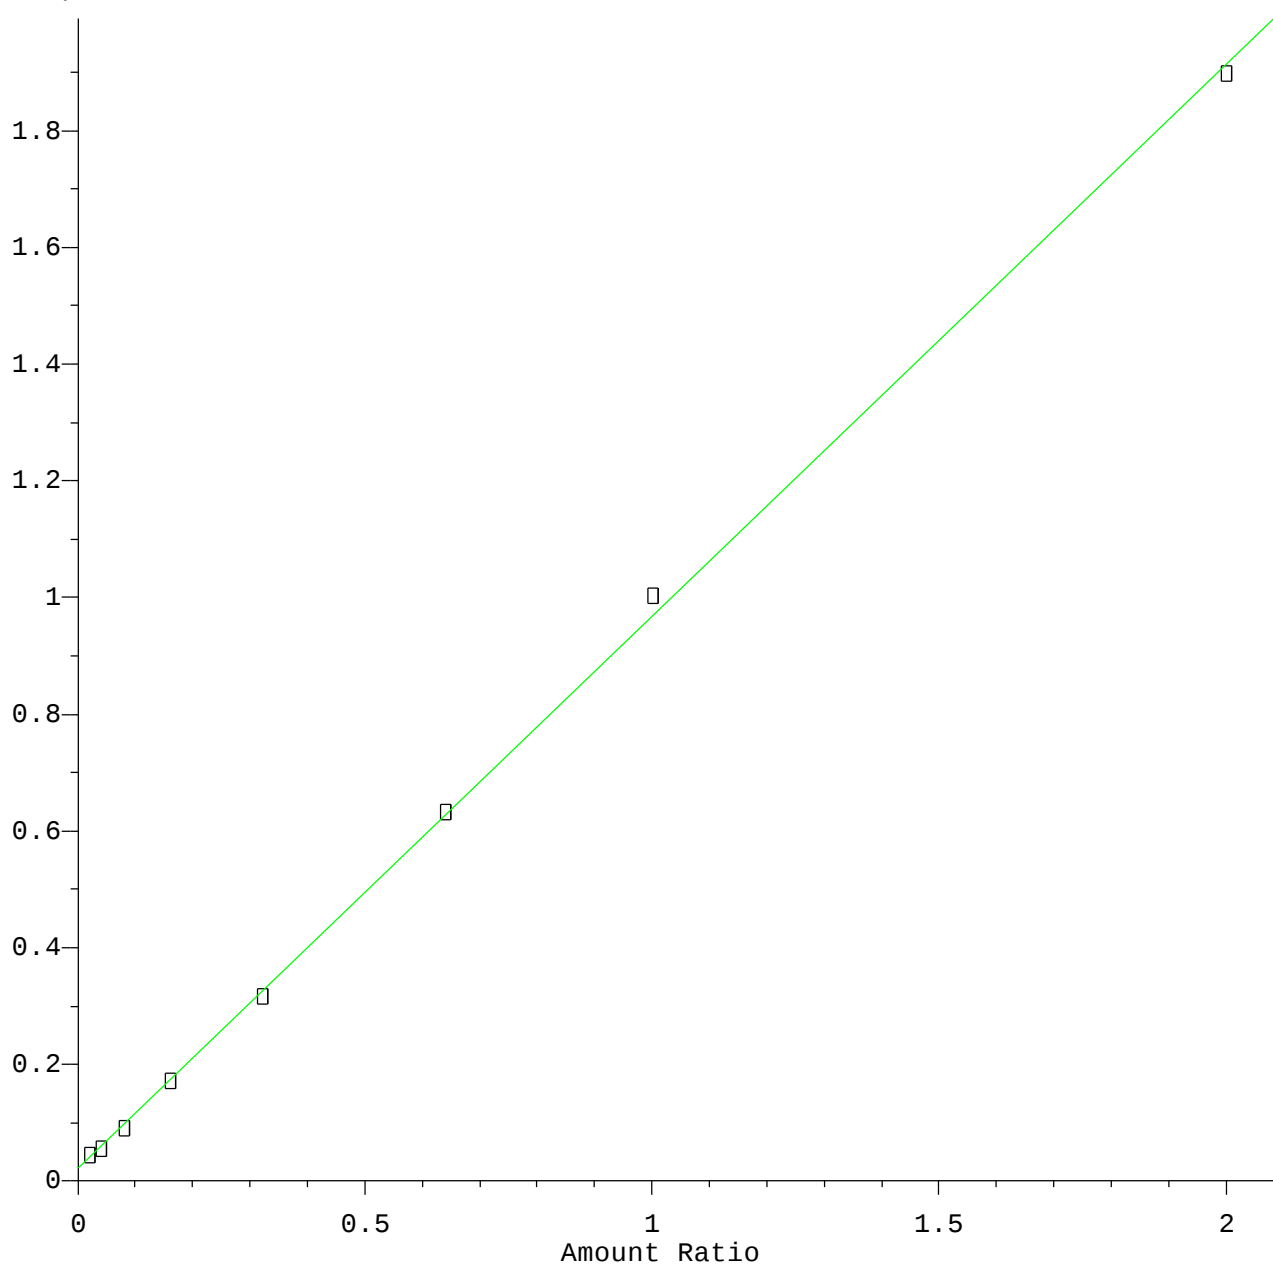

Resp Ratio = $9.45 \times 10^{-1} \times \text{Amt} + 2.21 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016

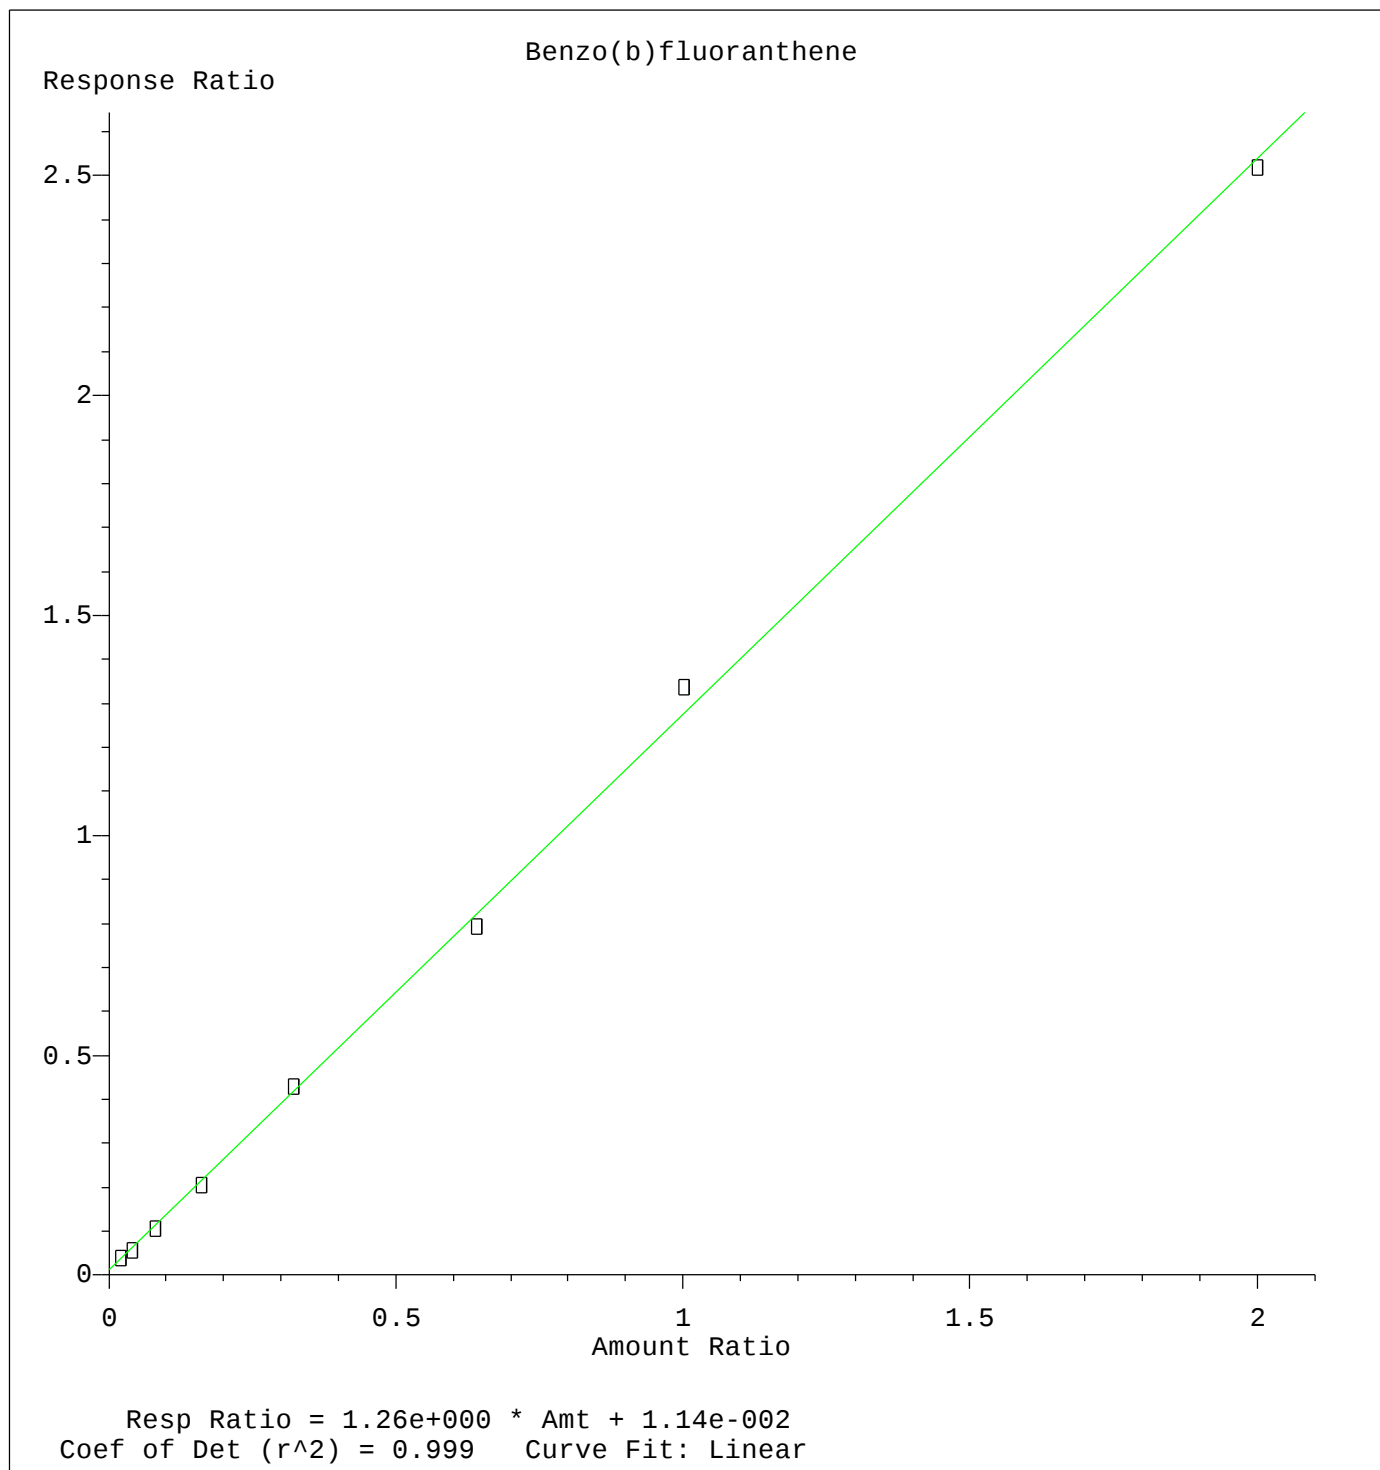

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Calibration Table Last Updated: Mon Aug 01 17:22:55 2016