


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080116\
Data File : BE092087.D
Acq On : 1 Aug 2016 11:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 01 17:22:55 2016

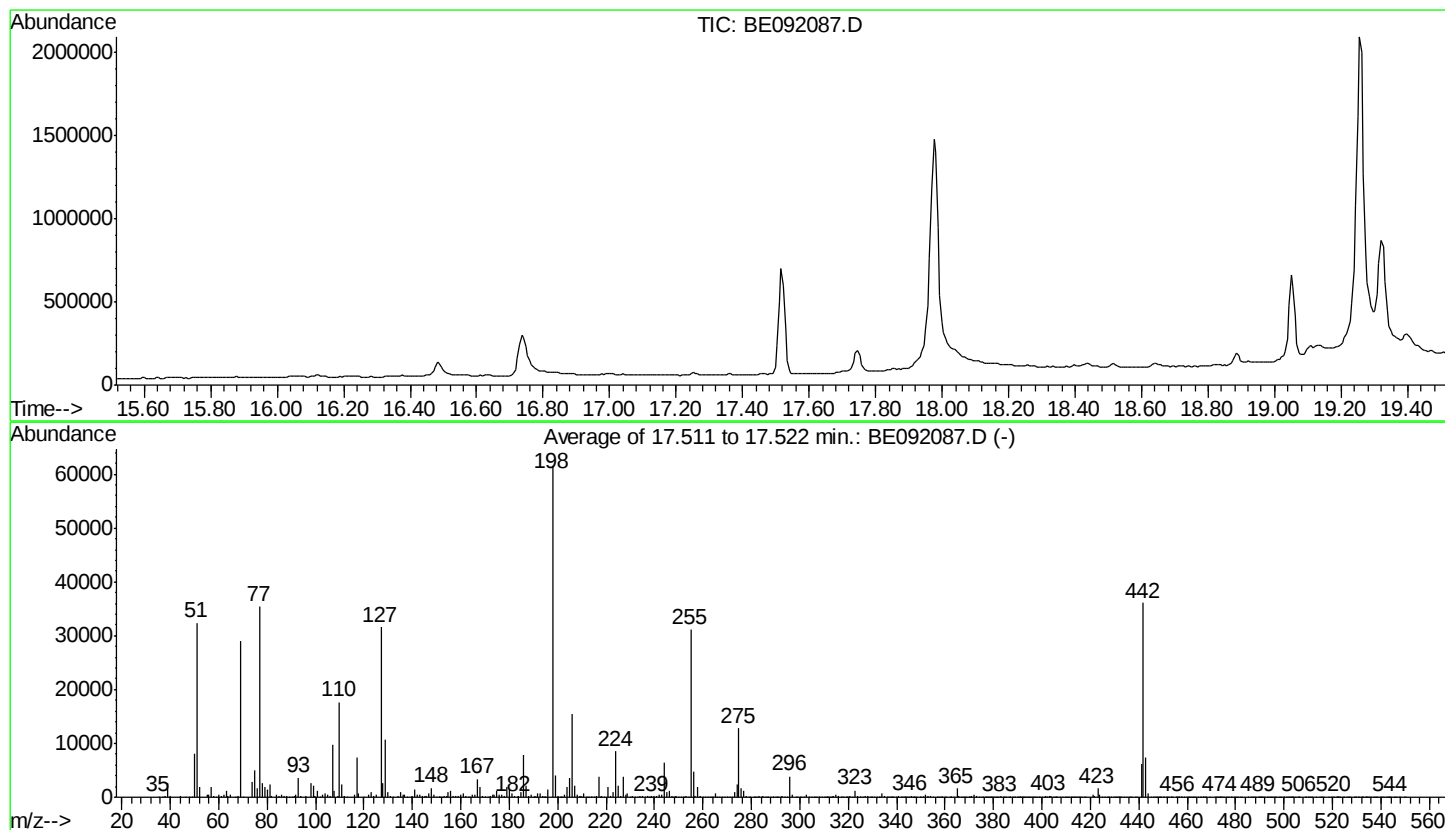

AutoFind: Scans 2540, 2541, 2542; Background Corrected with Scan 2533

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	32394	PASS
68	69	0.00	2	1.0	278	PASS
69	198	0.00	100	46.9	28911	PASS
70	69	0.00	2	0.2	55	PASS
127	198	10	80	51.2	31539	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61591	PASS
199	198	5	9	6.8	4169	PASS
275	198	10	60	20.8	12823	PASS
365	198	1	100	2.6	1629	PASS
441	442	0.01	24	17.4	6284	PASS
442	198	50	100	58.5	36061	PASS
443	442	15	24	20.6	7424	PASS