


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080117\
 Data File : BE093611.D
 Acq On : 1 Aug 2017 11:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 01 16:48:54 2017

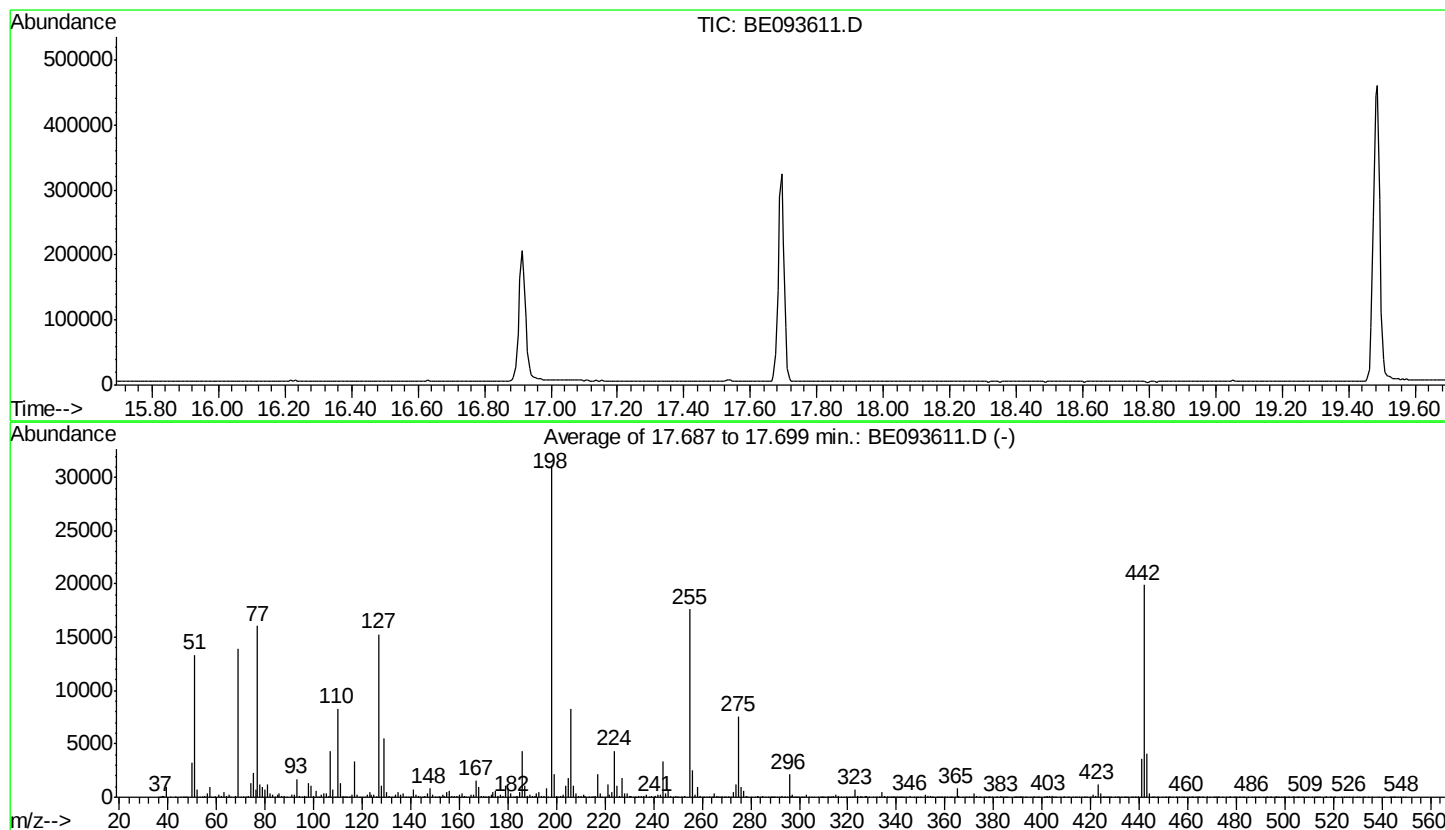

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	13384	PASS
68	69	0.00	2	1.1	151	PASS
69	198	0.00	100	44.6	13880	PASS
70	69	0.00	2	0.2	33	PASS
127	198	10	80	49.1	15271	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31105	PASS
199	198	5	9	6.8	2118	PASS
275	198	10	60	24.3	7561	PASS
365	198	1	100	2.6	823	PASS
441	442	0.01	24	18.2	3627	PASS
442	198	50	100	64.0	19919	PASS
443	442	15	24	20.5	4080	PASS