

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080216\
 Data File : BE092142.D
 Acq On : 3 Aug 2016 11:07
 Operator : UM/SJ
 Sample : H4176-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 GW-24-9.5-15.0

Quant Time: Aug 03 12:51:56 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 16:59:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	12200	5.00	ng	0.00
6) Naphthalene-d8	10.98	136	54021	5.00	ng	-0.01
10) Acenaphthene-d10	14.83	164	29319	5.00	ng	-0.02
16) Phenanthrene-d10	17.56	188	64315	5.00	ng	-0.02
22) Chrysene-d12	21.75	240	81780	5.00	ng	0.00
28) Perylene-d12	24.14	264	80876	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.68	112	210874	67.30	ng	-0.01
5) Phenol-d6	7.34	99	205041	49.12	ng	-0.01
7) Nitrobenzene-d5	9.34	82	346766	81.35	ng	-0.01
11) 2,4,6-Tribromophenol	16.33	330	131387	138.01	ng	0.00
12) 2-Fluorobiphenyl	13.46	172	637285	68.59	ng	0.00
24) Terphenyl-d14	20.21	244	803147	68.38	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080216\
Data File : BE092142.D
Acq On : 3 Aug 2016 11:07
Operator : UM/SJ
Sample : H4176-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
GW-24-9.5-15.0

Quant Time: Aug 03 12:51:56 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 16:59:37 2016
Response via : Initial Calibration

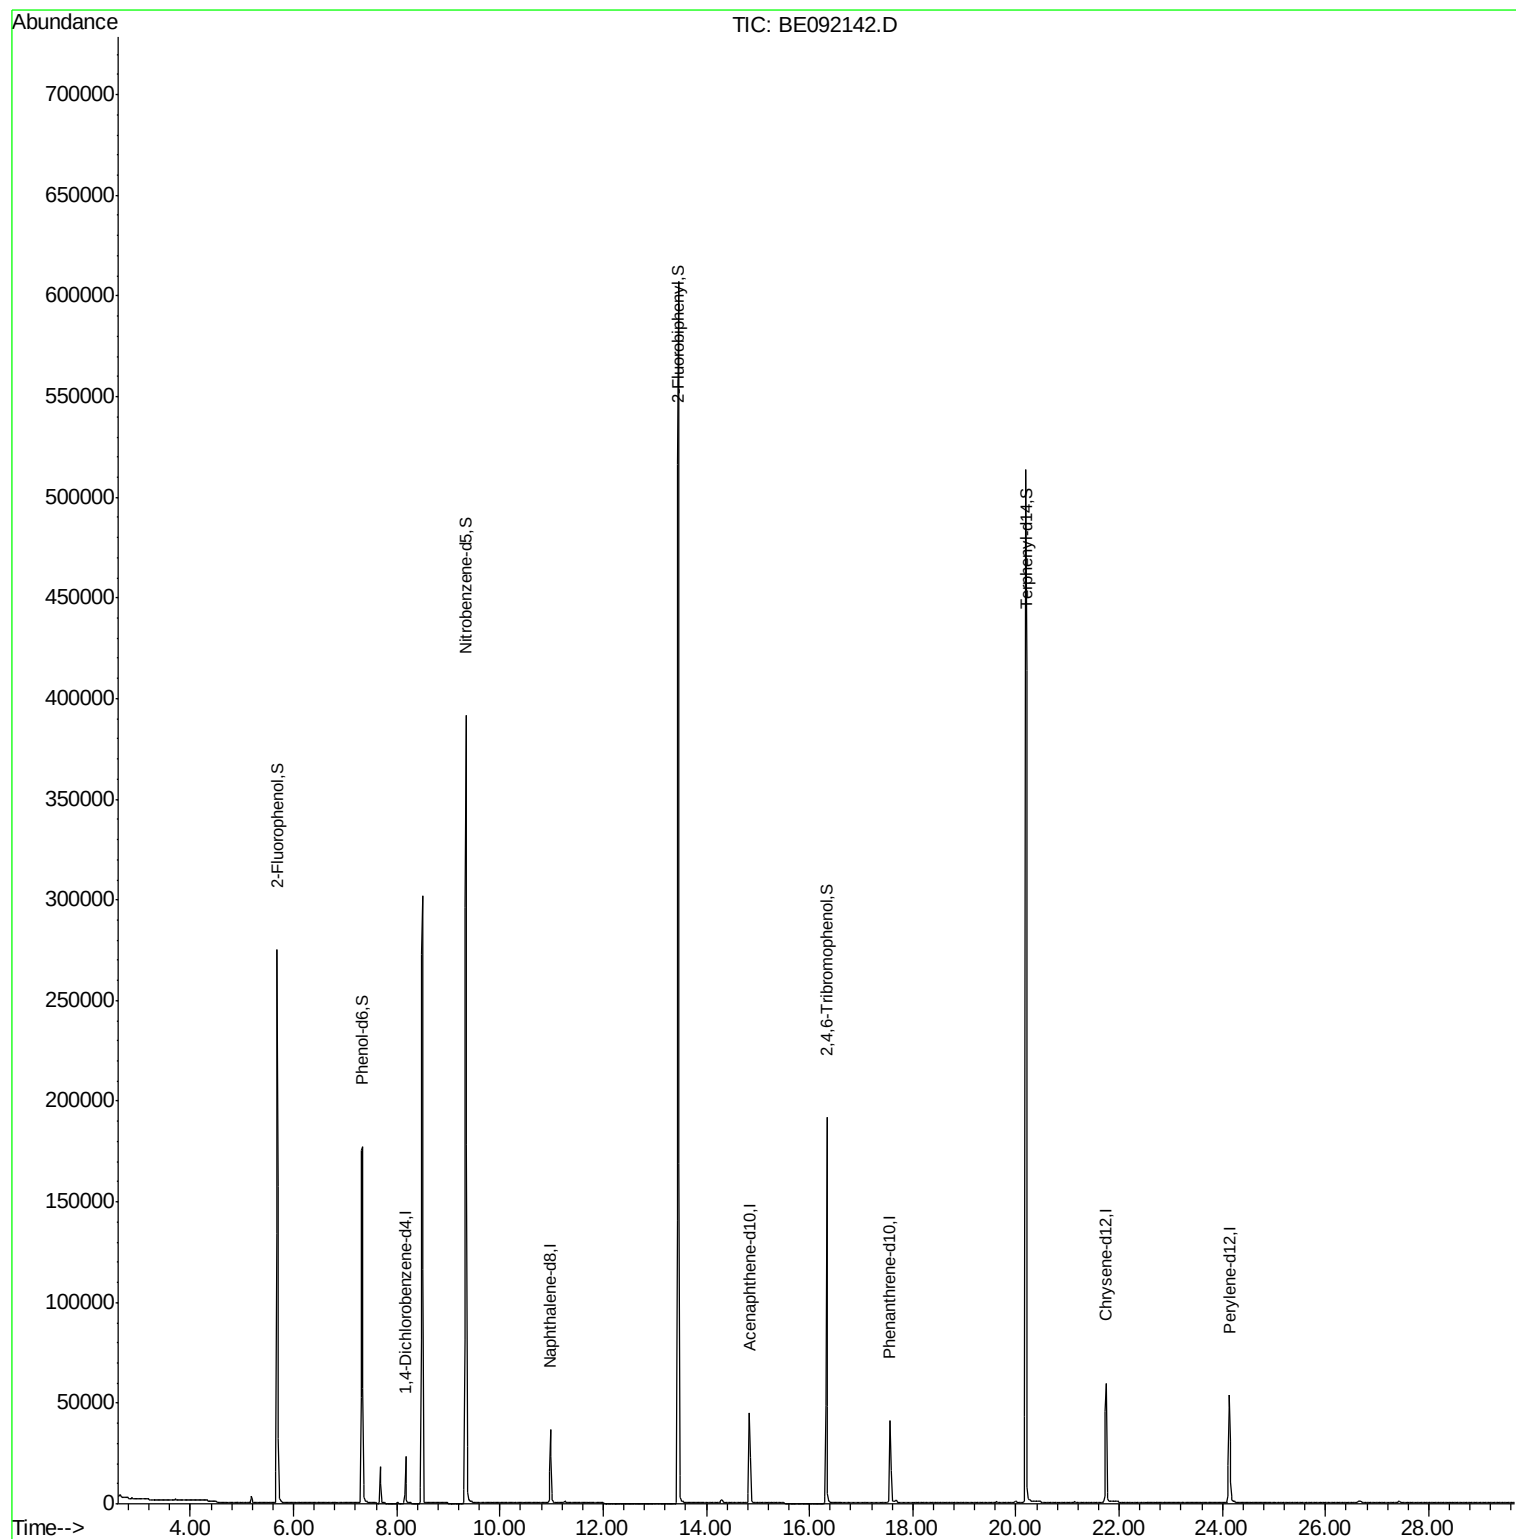

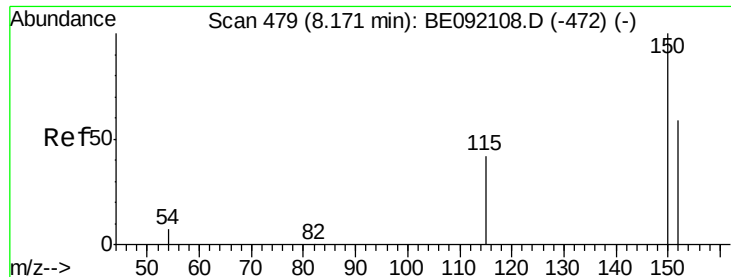


#1




1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 8.17 min Scan# 479
Delta R.T. -0.00 min
Lab File: BE092142.D
Acq: 3 Aug 2016 11:07

Instrument :
BNA_E
ClientSampleId :
GW-24-9.5-15.0

Tot Ion:152 Resp: 12200
Ion Ratio Lower Upper
152 100
150 151.9 106.0 159.0
115 53.3 36.9 55.3

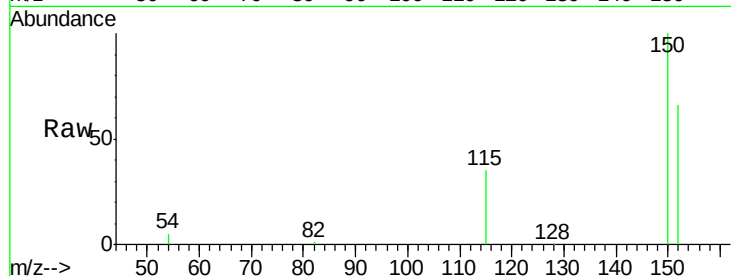


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

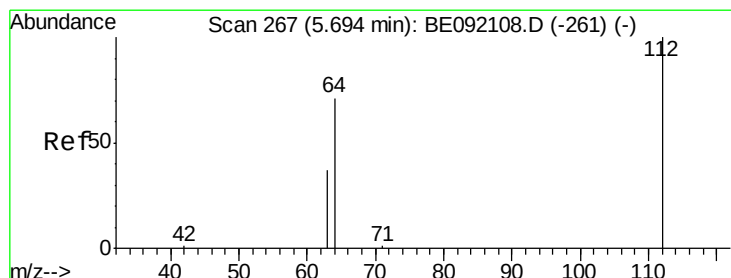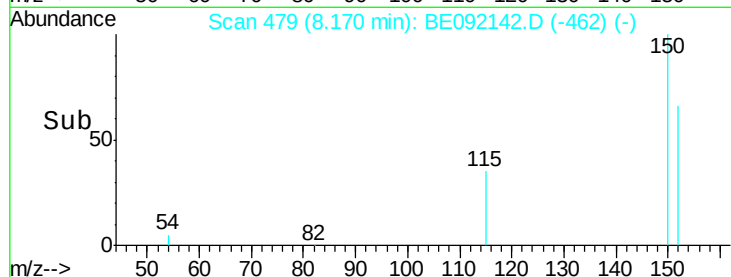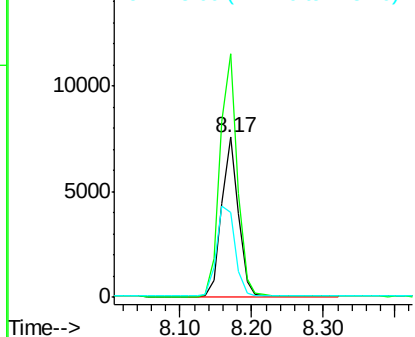



#4


2-Fluorophenol
Concen: 67.30 ng
RT: 5.68 min Scan# 266
Delta R.T. -0.01 min
Lab File: BE092142.D
Acq: 3 Aug 2016 11:07

Tgt Ion:112 Resp: 210874
Ion Ratio Lower Upper
112 100
64 68.5 55.9 83.9
63 37.1 31.1 46.7

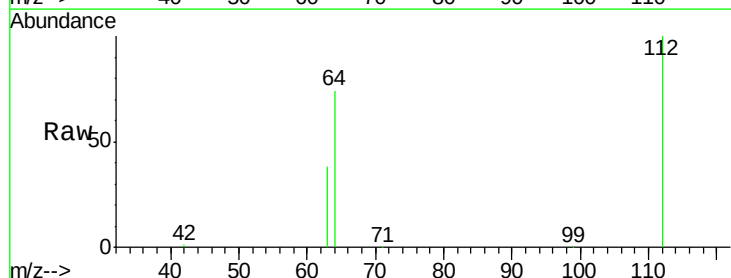

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

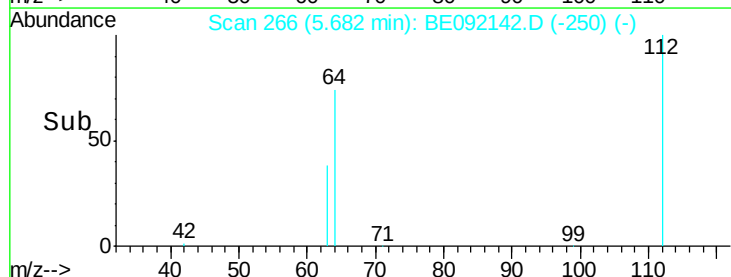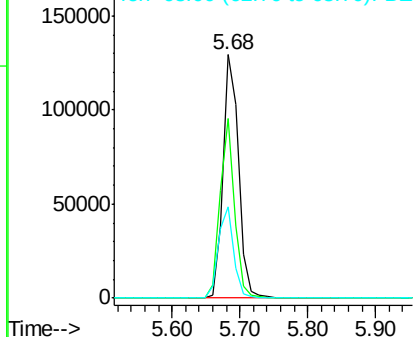

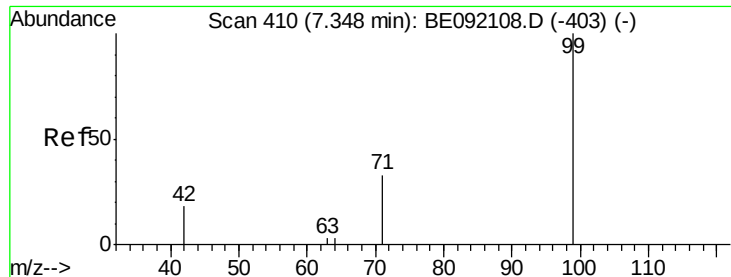

#5

Phenol-d6

Concen: 49.12 ng

RT: 7.34 min Scan# 409

Delta R.T. -0.01 min

Lab File: BE092142.D

Acq: 3 Aug 2016 11:07

Instrument :

BNA_E

ClientSampleId :

GW-24-9.5-15.0


Tot Ion: 99 Resp: 205041

Ion Ratio Lower Upper

99 100

42 25.0 22.4 33.6




71 35.8 28.9 43.3

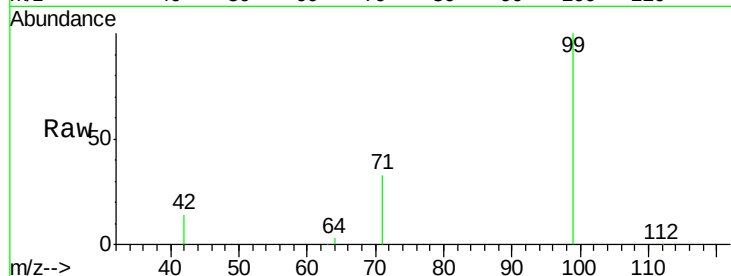

Abundance Ion 99.00 (98.70 to 99.70): BE092108.D (-403) (-)

Ion 42.00 (41.70 to 42.70): BE092108.D (-403) (-)

Ion 71.00 (70.70 to 71.70): BE092108.D (-403) (-)

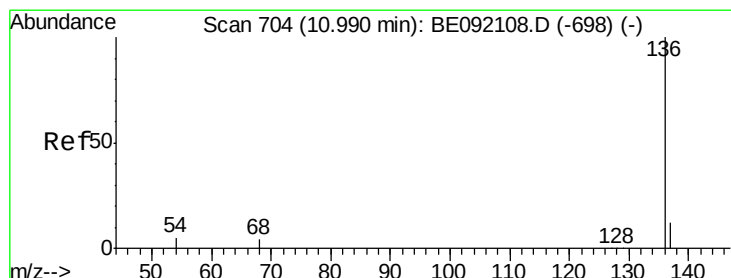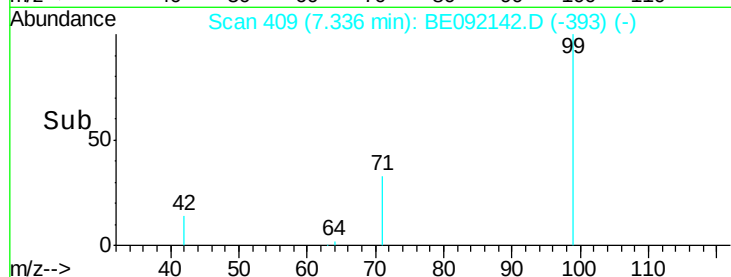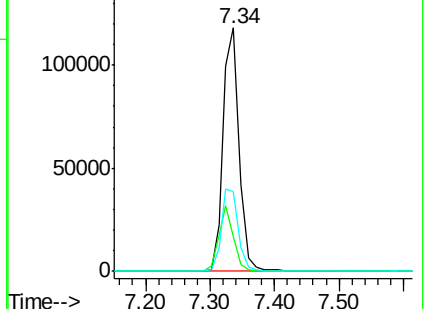

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.98 min Scan# 703

Delta R.T. -0.01 min

Lab File: BE092142.D

Acq: 3 Aug 2016 11:07

Tgt Ion: 136 Resp: 54021


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 8.7 2.7 4.1#

68 6.4 2.2 3.4#


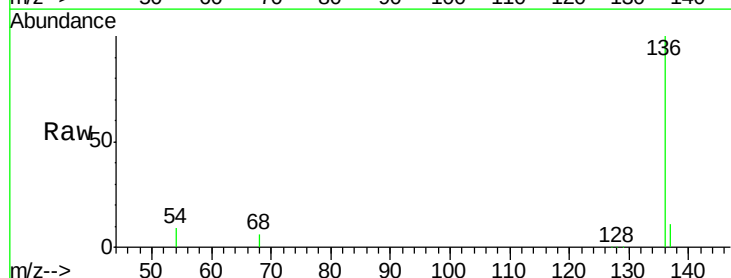



Abundance Ion 136.00 (135.70 to 136.70): BE092108.D (-698) (-)

Ion 137.00 (136.70 to 137.70): BE092108.D (-698) (-)

Ion 54.00 (53.70 to 54.70): BE092108.D (-698) (-)

Ion 68.00 (67.70 to 68.70): BE092108.D (-698) (-)

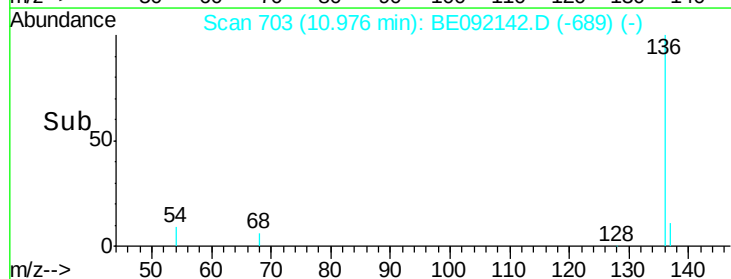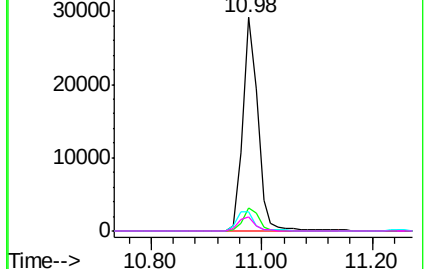

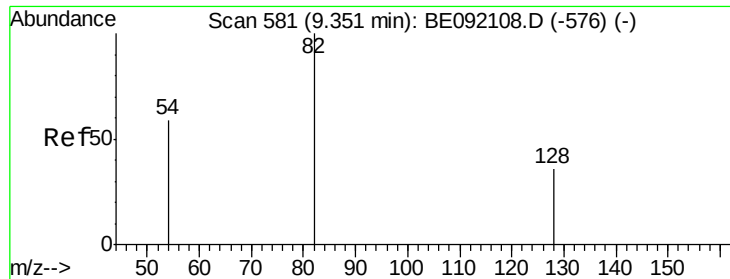

#7

Nitrobenzene-d5

Concen: 81.35 ng

RT: 9.34 min Scan# 580

Delta R.T. -0.01 min

Lab File: BE092142.D

Acq: 3 Aug 2016 11:07

Instrument :

BNA_E

ClientSampleId :

GW-24-9.5-15.0


Tot Ion: 82 Resp: 346766

Ion Ratio Lower Upper

82 100

128 39.7 33.0 49.4




54 58.4 42.6 63.8

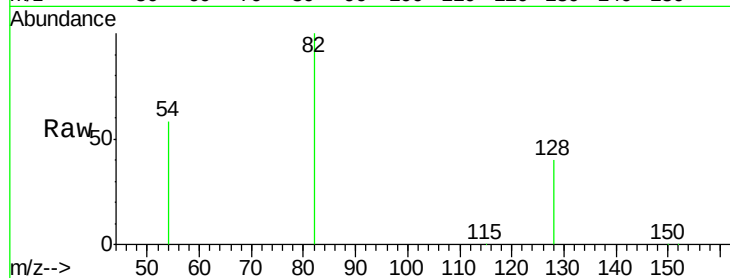

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

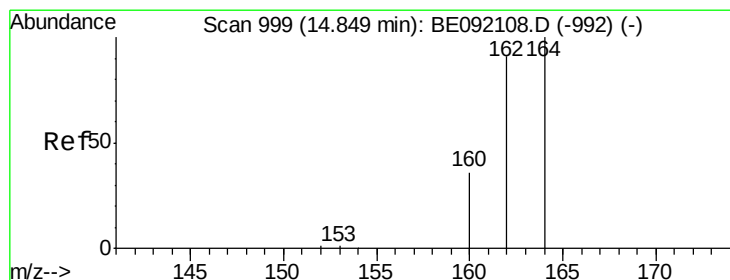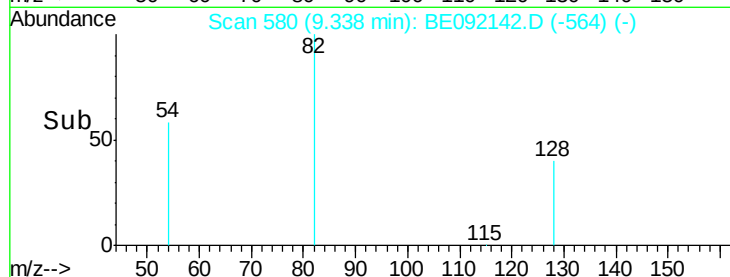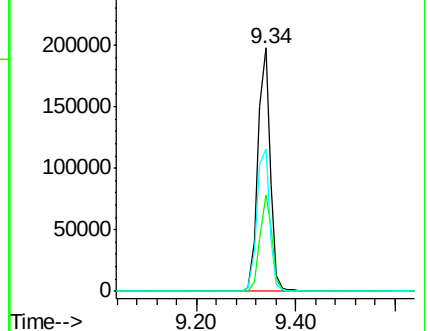

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.83 min Scan# 998

Delta R.T. -0.02 min

Lab File: BE092142.D

Acq: 3 Aug 2016 11:07


Tgt Ion: 164 Resp: 29319

Ion Ratio Lower Upper

164 100

162 111.6 69.5 104.3#



160 53.5 27.6 41.4#

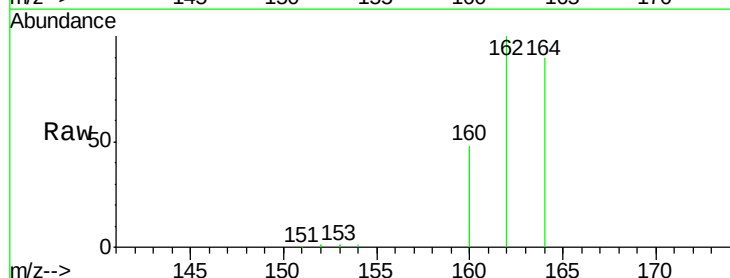


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



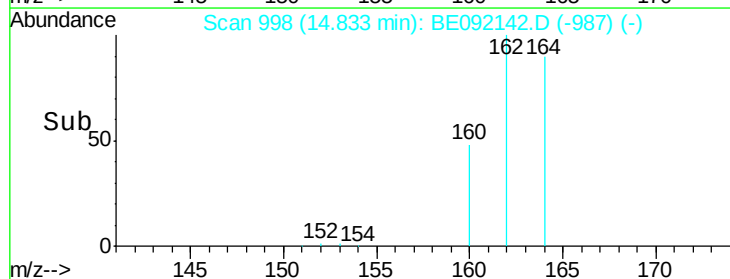
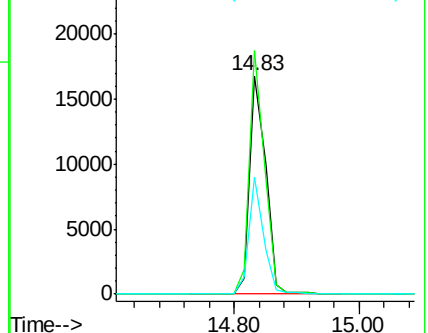


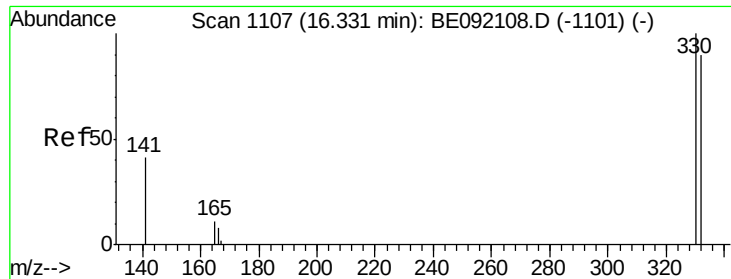

#11
 2,4,6-Tribromophenol
 Concen: 138.01 ng
 RT: 16.33 min Scan# 1107
 Delta R.T. -0.00 min
 Lab File: BE092142.D
 Acq: 3 Aug 2016 11:07




Instrument :
 BNA_E
 ClientSampleId :
 GW-24-9.5-15.0


Tot Ion:330 Resp: 131387
 Ion Ratio Lower Upper
 330 100
 332 96.9 74.2 111.4
 141 43.4 139.8 209.8#

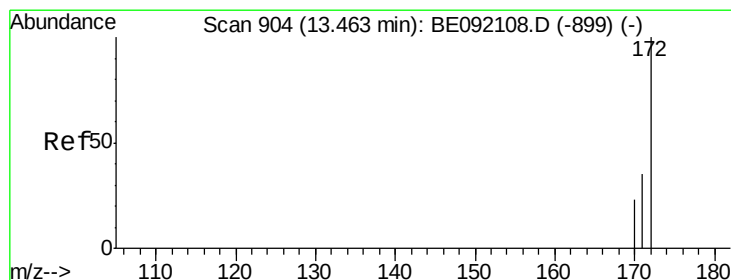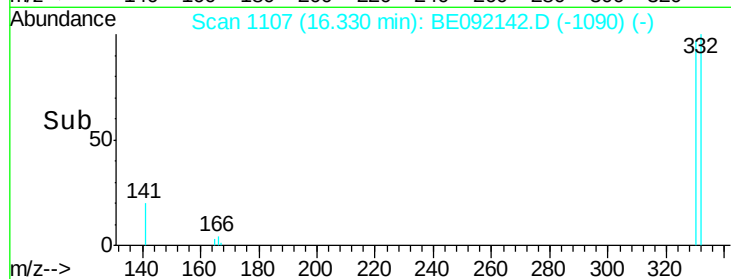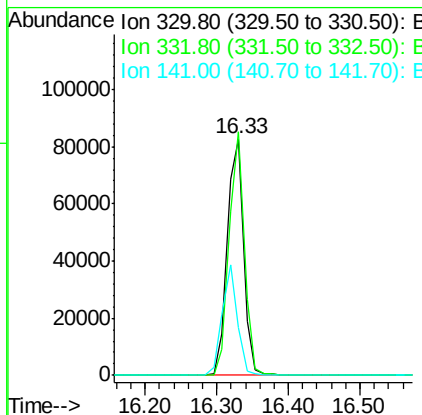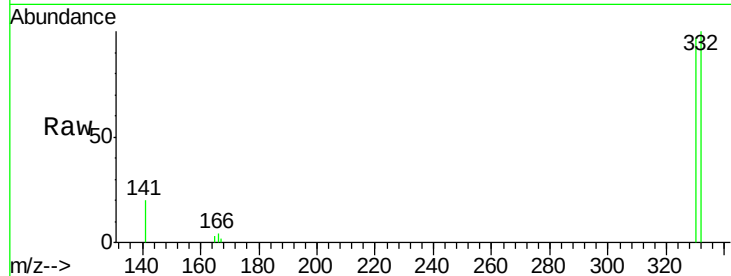

#12
 2-Fluorobiphenyl
 Concen: 68.59 ng
 RT: 13.46 min Scan# 904
 Delta R.T. -0.00 min
 Lab File: BE092142.D
 Acq: 3 Aug 2016 11:07

Tgt Ion:172 Resp: 637285
 Ion Ratio Lower Upper
 172 100
 171 32.2 30.3 45.5
 170 19.6 21.6 32.4#

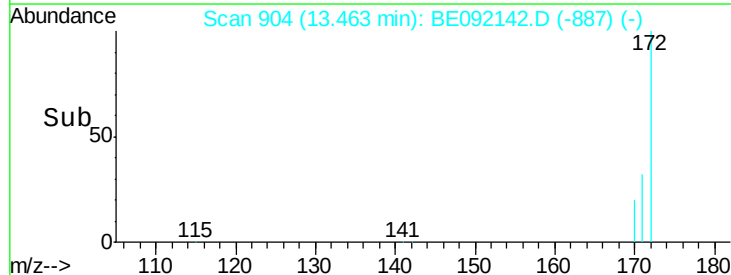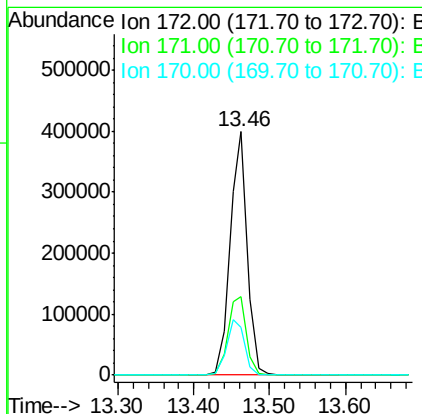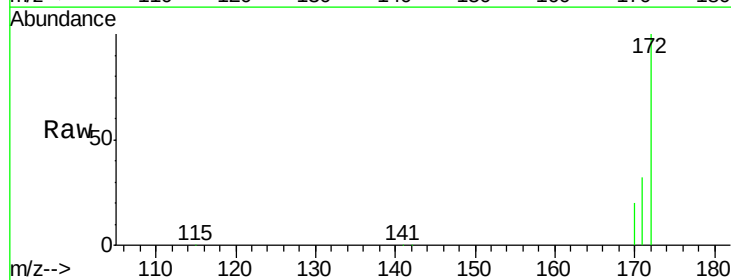

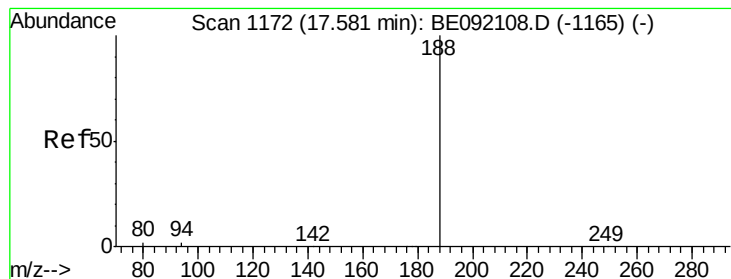

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1171

Delta R.T. -0.02 min

Lab File: BE092142.D

Acq: 3 Aug 2016 11:07

Instrument :

BNA_E

ClientSampleId :

GW-24-9.5-15.0


Tot Ion:188 Resp: 64315

Ion Ratio Lower Upper

188 100

94 16.1 3.9 5.9#




80 16.9 3.4 5.0#

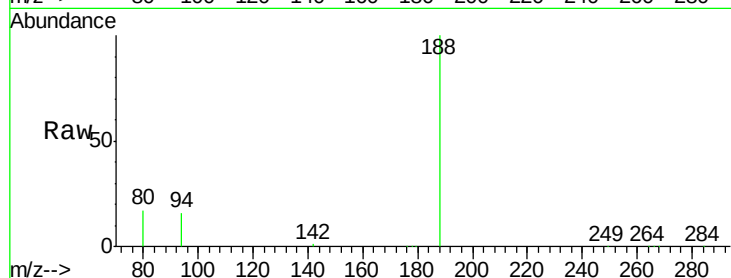

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

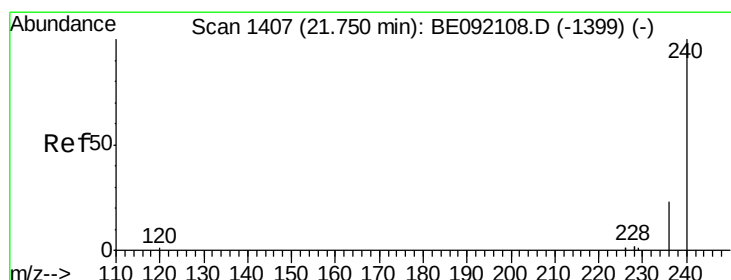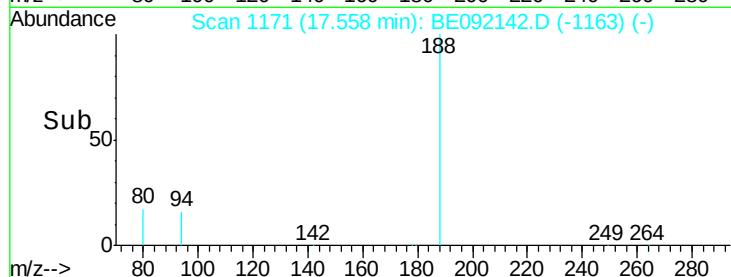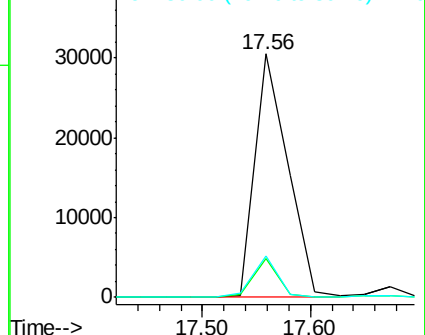

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1407

Delta R.T. -0.00 min

Lab File: BE092142.D

Acq: 3 Aug 2016 11:07


Tgt Ion:240 Resp: 81780

Ion Ratio Lower Upper

240 100

120 1.4 0.6 1.0#



236 22.7 18.2 27.4

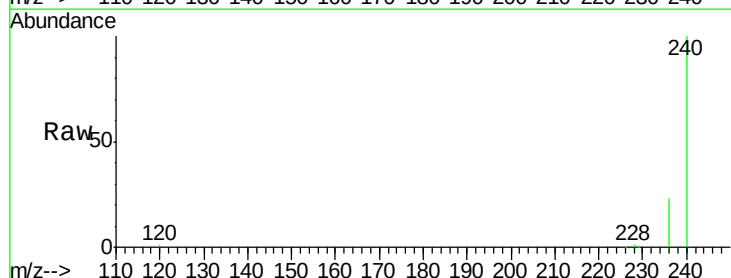


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



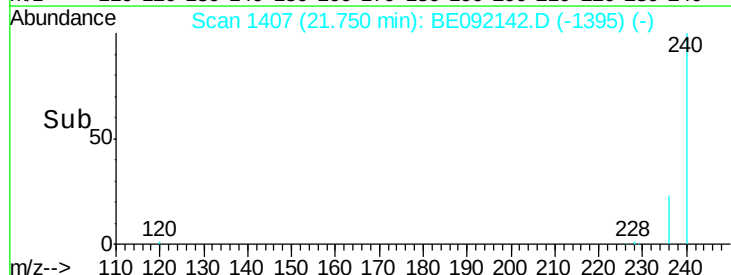
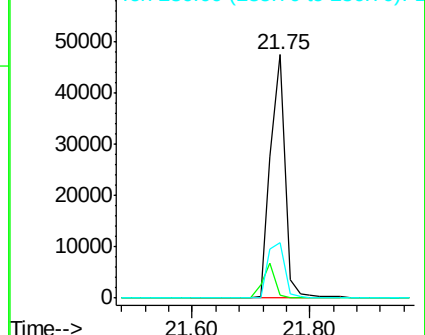


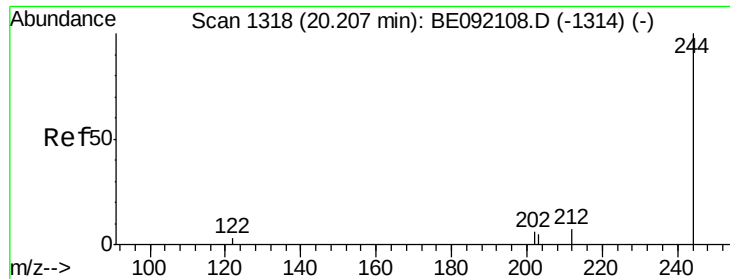

#24
 Terphenyl-d14
 Concen: 68.38 ng
 RT: 20.21 min Scan# 1318
 Delta R.T. -0.00 min
 Lab File: BE092142.D
 Acq: 3 Aug 2016 11:07

Instrument :
 BNA_E
 ClientSampleId :
 GW-24-9.5-15.0

Tot Ion:244 Resp: 803147
 Ion Ratio Lower Upper
 244 100
 212 6.7 9.1 13.7#
 122 0.6 11.0 16.4#

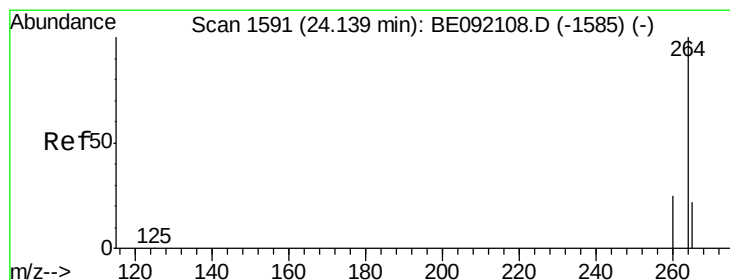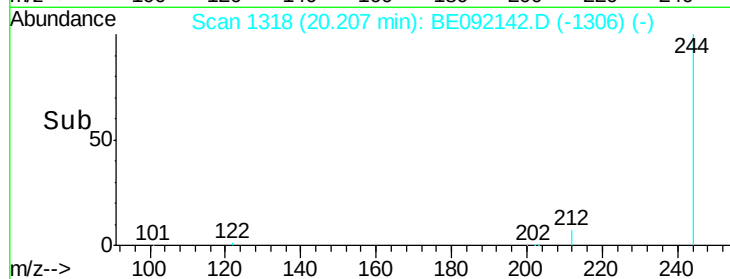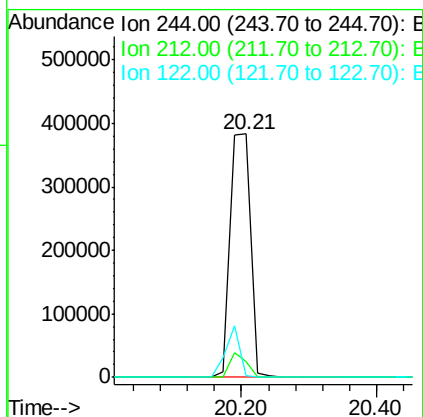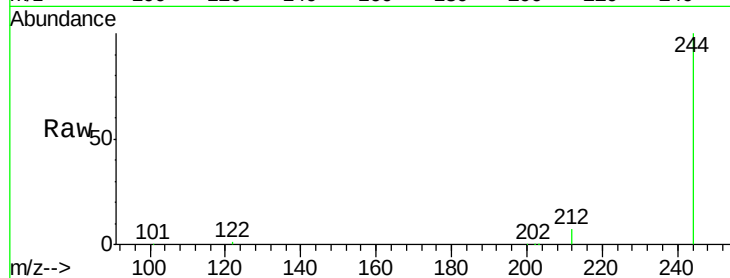

#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 24.14 min Scan# 1591
 Delta R.T. 0.00 min
 Lab File: BE092142.D
 Acq: 3 Aug 2016 11:07

Tgt Ion:264 Resp: 80876
 Ion Ratio Lower Upper
 264 100
 260 23.8 20.8 31.2
 265 23.0 16.6 25.0

