


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080216\
Data File : BE092105.D
Acq On : 2 Aug 2016 10:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 02 16:59:37 2016

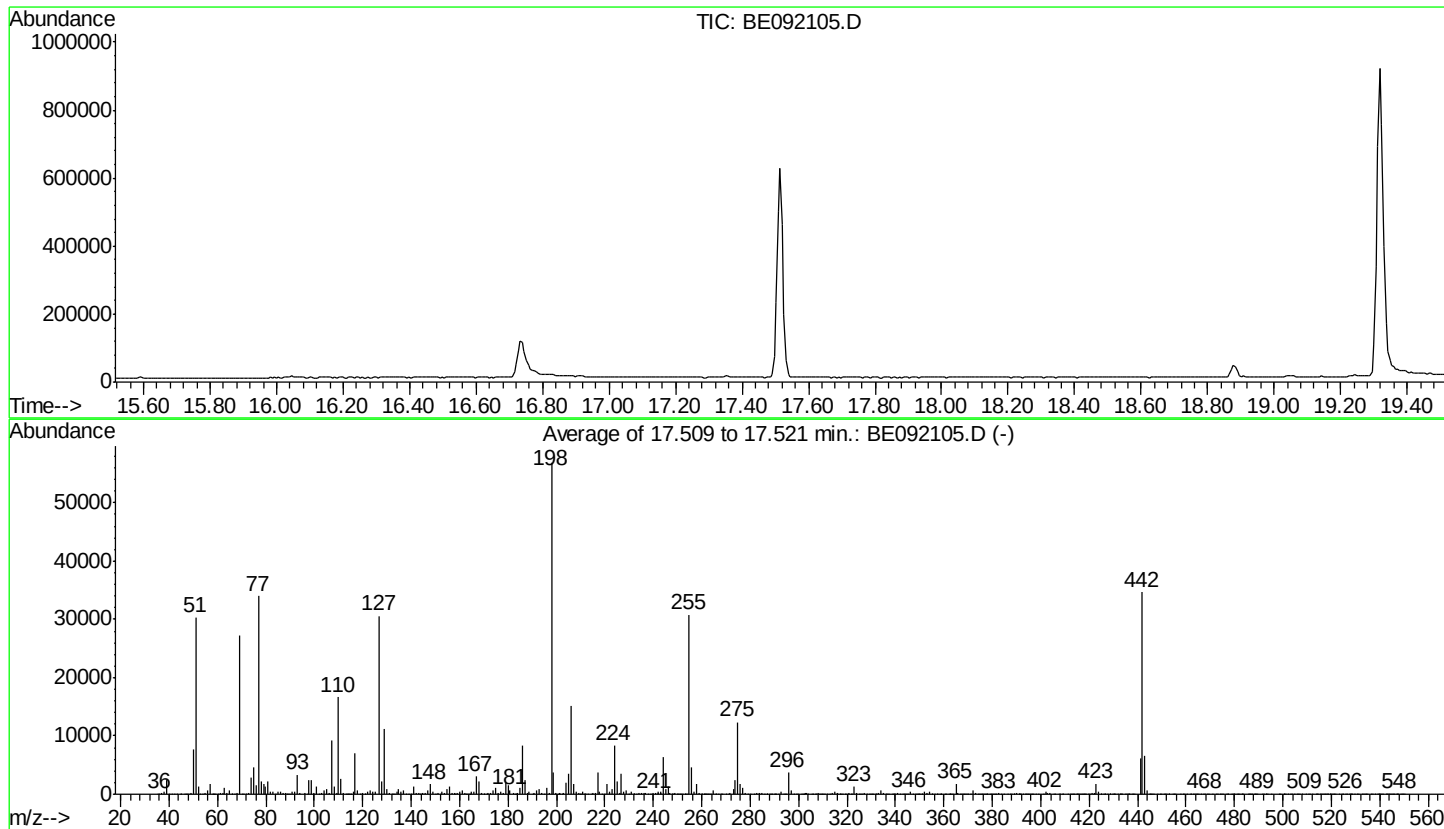

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	30219	PASS
68	69	0.00	2	0.8	216	PASS
69	198	0.00	100	47.9	27228	PASS
70	69	0.00	2	0.2	55	PASS
127	198	10	80	53.8	30623	PASS
197	198	0.00	2	0.2	123	PASS
198	198	100	100	100.0	56887	PASS
199	198	5	9	6.7	3818	PASS
275	198	10	60	21.7	12348	PASS
365	198	1	100	3.1	1772	PASS
441	442	0.01	24	17.7	6137	PASS
442	198	50	100	60.9	34626	PASS
443	442	15	24	18.8	6524	PASS