


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080216\
 Data File : BE092115.D
 Acq On : 2 Aug 2016 17:34
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 16:59:37 2016

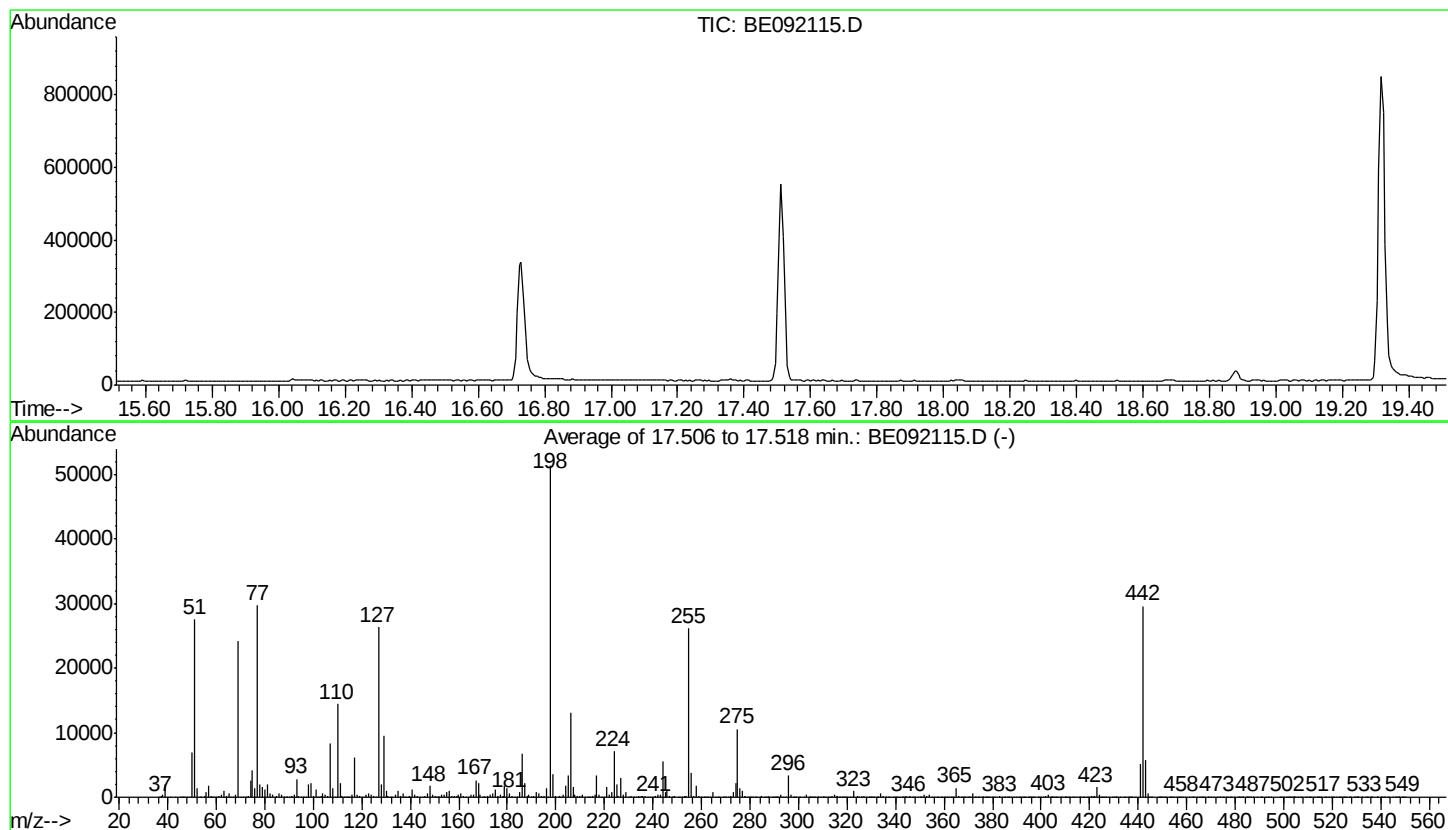

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	27525	PASS
68	69	0.00	2	1.8	427	PASS
69	198	0.00	100	47.3	24261	PASS
70	69	0.00	2	0.4	97	PASS
127	198	10	80	51.3	26338	PASS
197	198	0.00	2	0.2	97	PASS
198	198	100	100	100.0	51344	PASS
199	198	5	9	6.8	3482	PASS
275	198	10	60	20.5	10521	PASS
365	198	1	100	2.9	1470	PASS
441	442	0.01	24	17.5	5169	PASS
442	198	50	100	57.5	29533	PASS
443	442	15	24	19.6	5792	PASS