
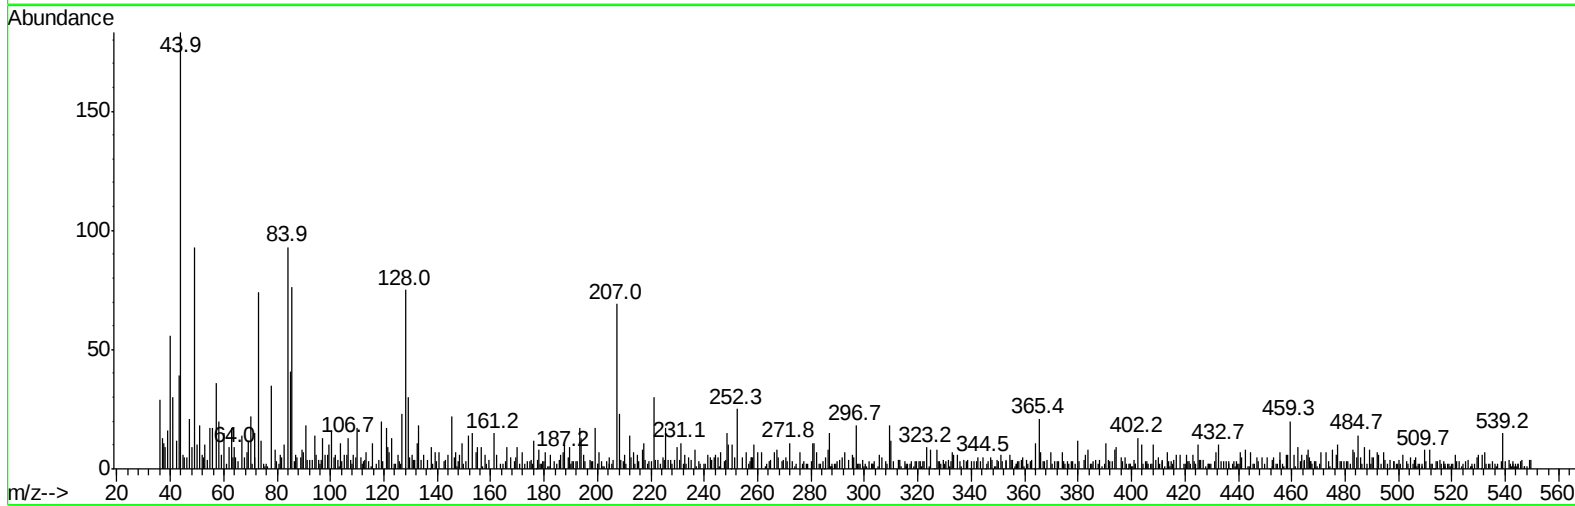


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080217\
Data File : BE093630.D
Acq On : 2 Aug 2017 17:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 04:36:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

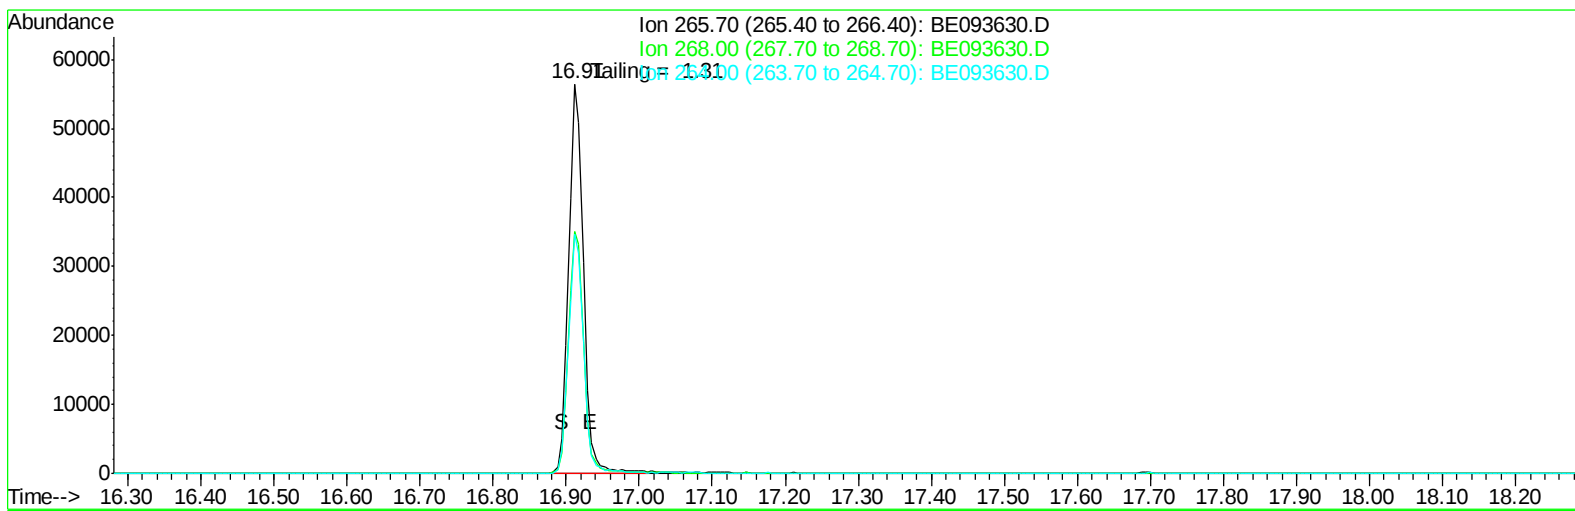

TIC: BE093630.D

(69) Pentachlorophenol (C)



10.772min (-0.049) 107.98ng

response 4

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	71.43
264.00	64.60	100.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080217\
Data File : BE093630.D
Acq On : 2 Aug 2017 17:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 04:36:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

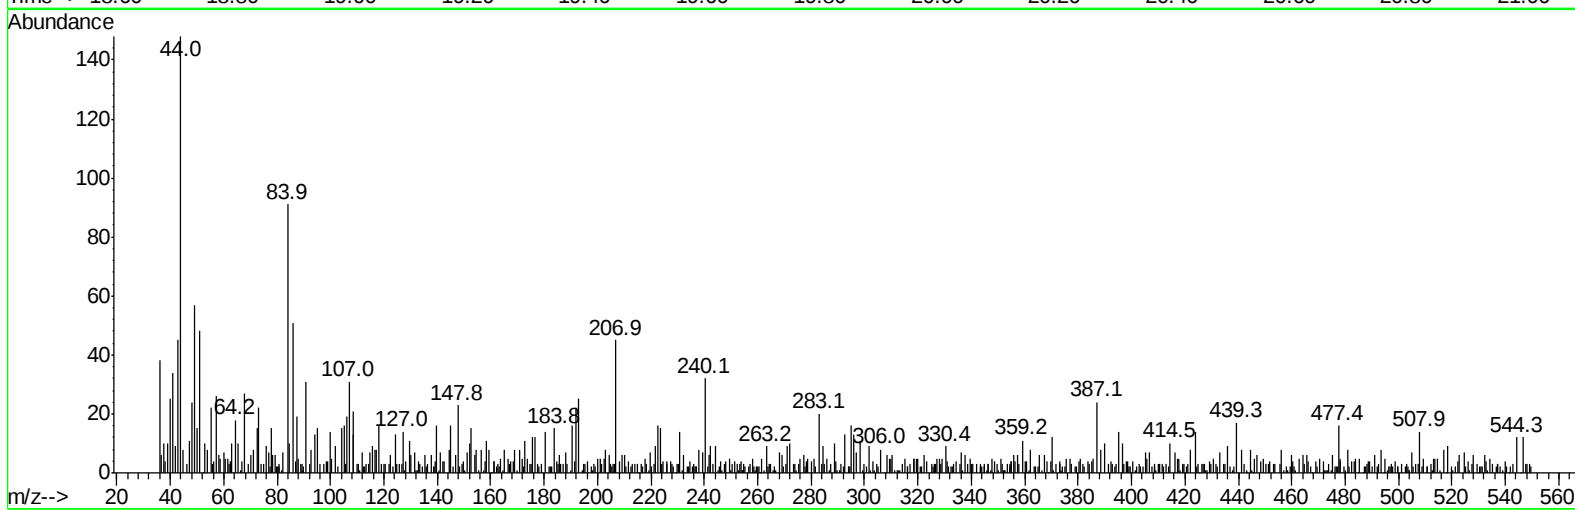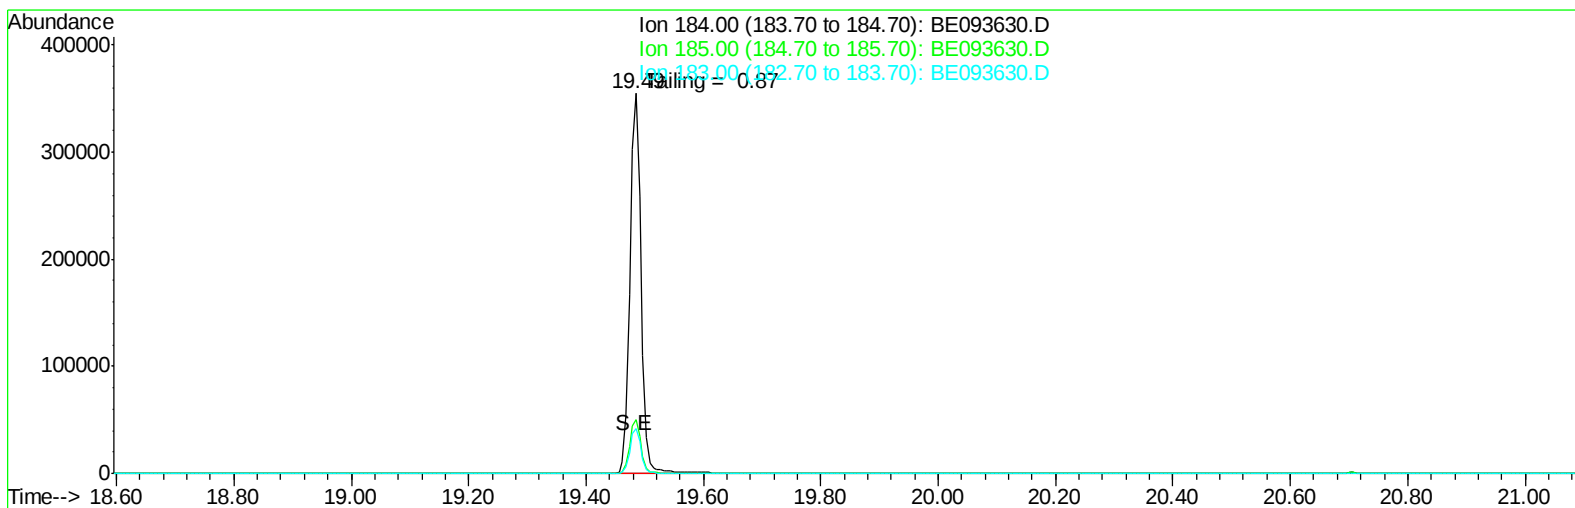

TIC: BE093630.D

(76) Benzidine

12.535min (+0.201) 25.03ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.79
183.00	12.20	10.53
0.00	0.00	0.00