
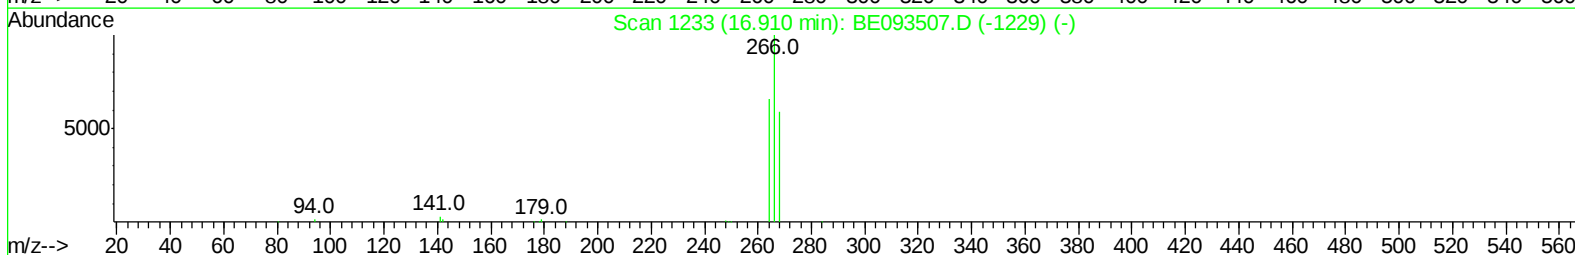
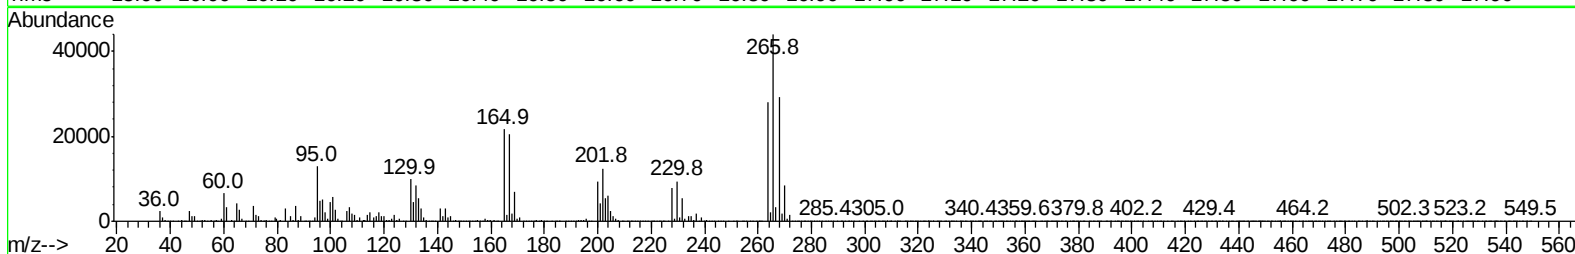


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080217\  
Data File : BE093619.D  
Acq On : 2 Aug 2017 8:11  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:19:05 2017  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE080117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 02 10:58:31 2017  
Response via : Initial Calibration

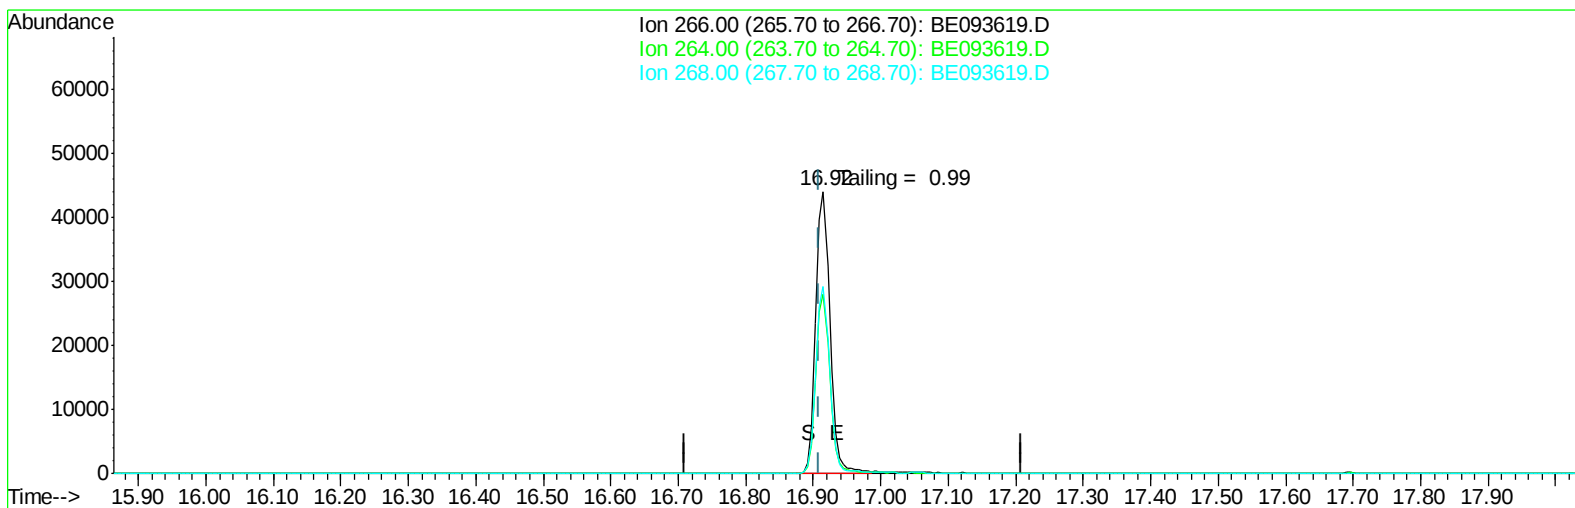

TIC: BE093619.D

(22) Pentachlorophenol

16.915min (+0.005) 4066.27ng

response 63487

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 266.00 | 100   | 100   |
| 264.00 | 70.00 | 63.65 |
| 268.00 | 65.00 | 66.43 |
| 0.00   | 0.00  | 0.00  |