


Data Path : Z:\HPCHEM1\BNA_E\Data\BE080217\
 Data File : BE093619.D
 Acq On : 2 Aug 2017 8:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 02 10:58:31 2017

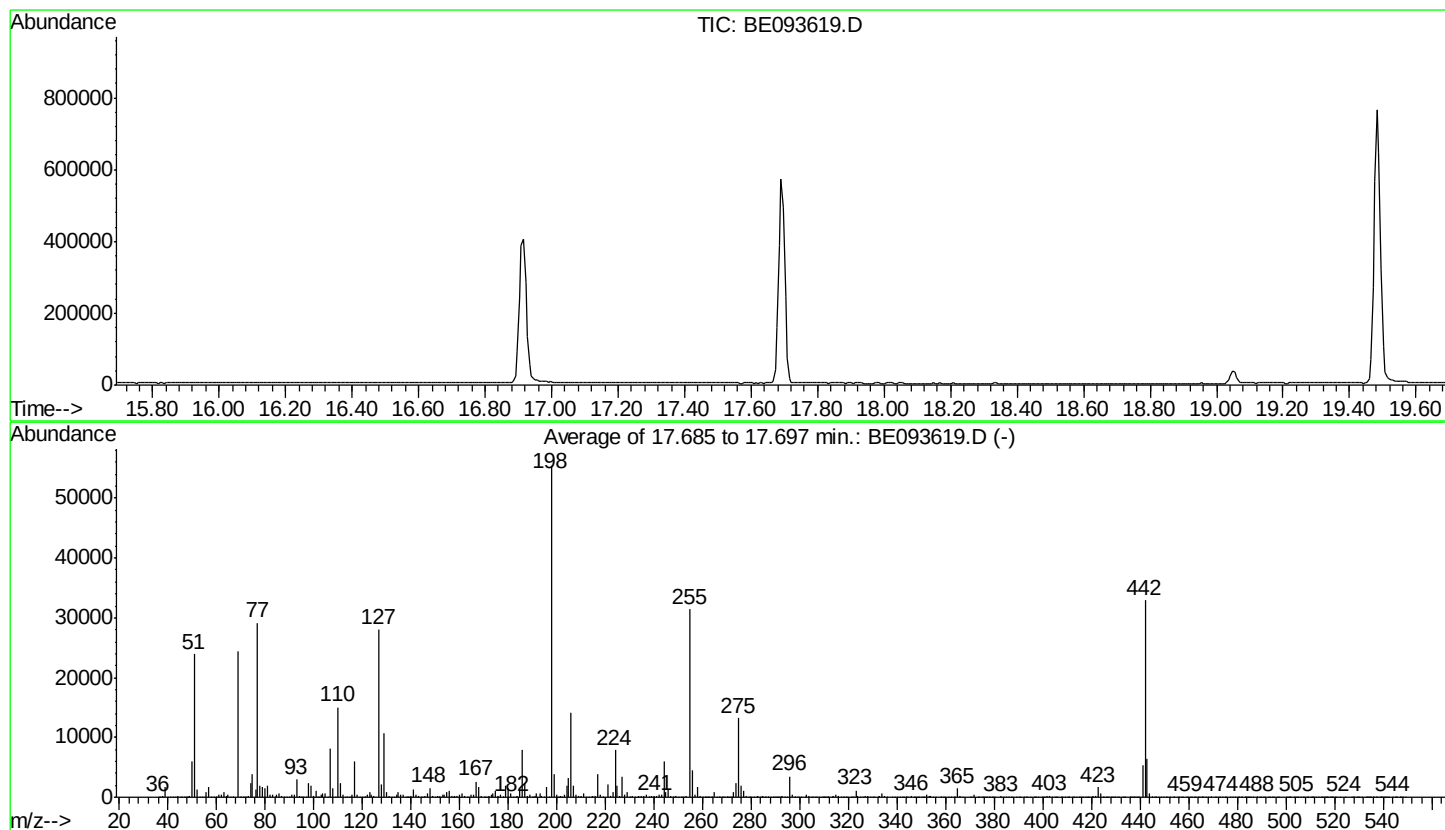

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	23949	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	24406	PASS
70	69	0.00	2	0.4	94	PASS
127	198	10	80	50.5	27971	PASS
197	198	0.00	2	0.2	111	PASS
198	198	100	100	100.0	55438	PASS
199	198	5	9	7.1	3925	PASS
275	198	10	60	23.9	13230	PASS
365	198	1	100	2.7	1473	PASS
441	442	0.01	24	16.3	5365	PASS
442	198	50	100	59.3	32901	PASS
443	442	15	24	19.4	6383	PASS