


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080315\
Data File : BE090316.D
Acq On : 3 Aug 2015 11:37
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 04 02:31:31 2015

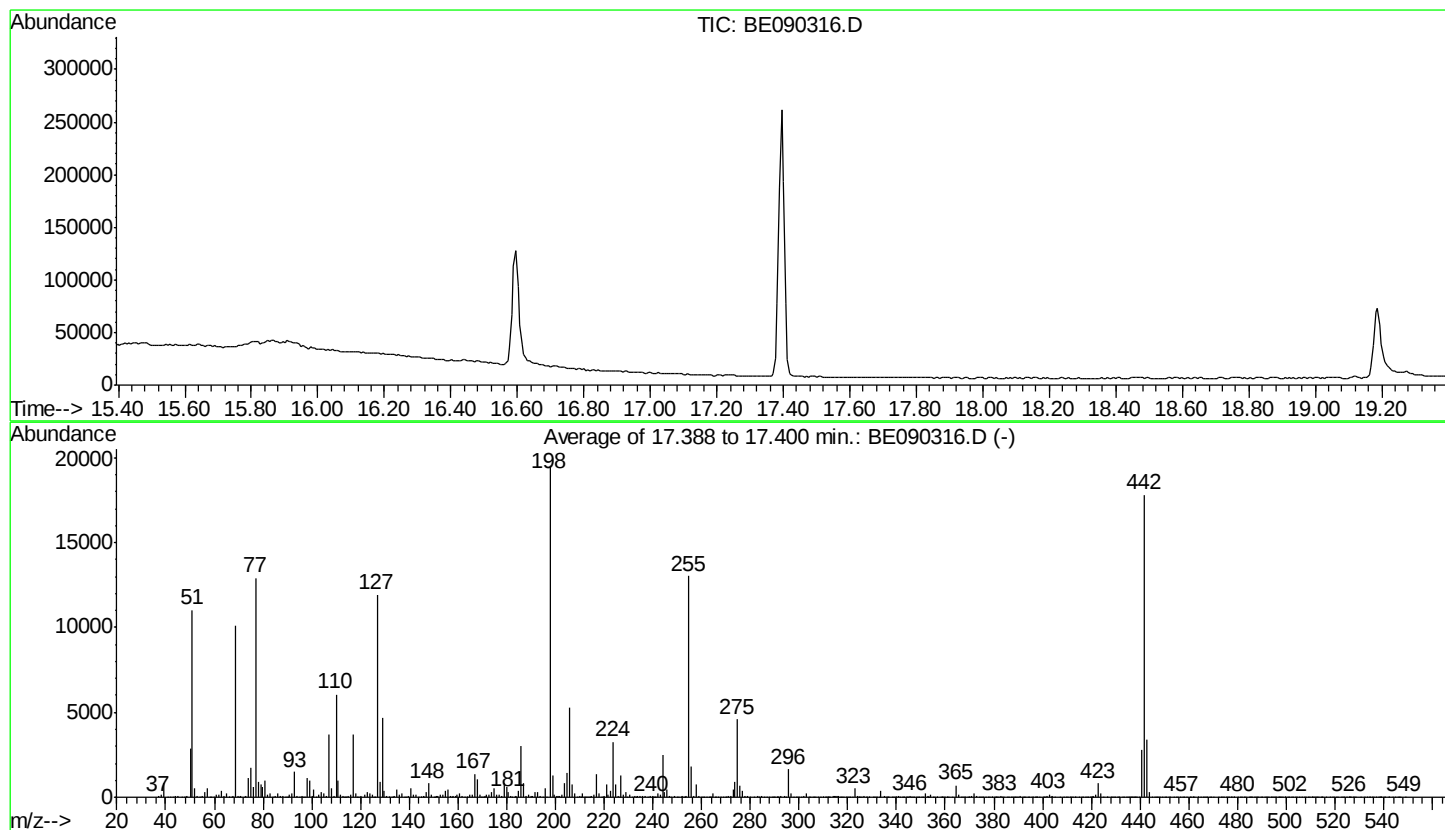

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.4	11023	PASS
68	69	0.00	2	1.0	101	PASS
69	198	0.00	100	51.8	10122	PASS
70	69	0.00	2	0.6	59	PASS
127	198	10	80	61.1	11933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19533	PASS
199	198	5	9	6.6	1280	PASS
275	198	10	60	23.5	4583	PASS
365	198	1	100	3.6	697	PASS
441	442	0.01	24	15.5	2757	PASS
442	198	50	100	91.3	17830	PASS
443	442	15	24	19.0	3396	PASS