


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080315\
 Data File : BE090334.D
 Acq On : 4 Aug 2015 7:01
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 04 02:31:31 2015

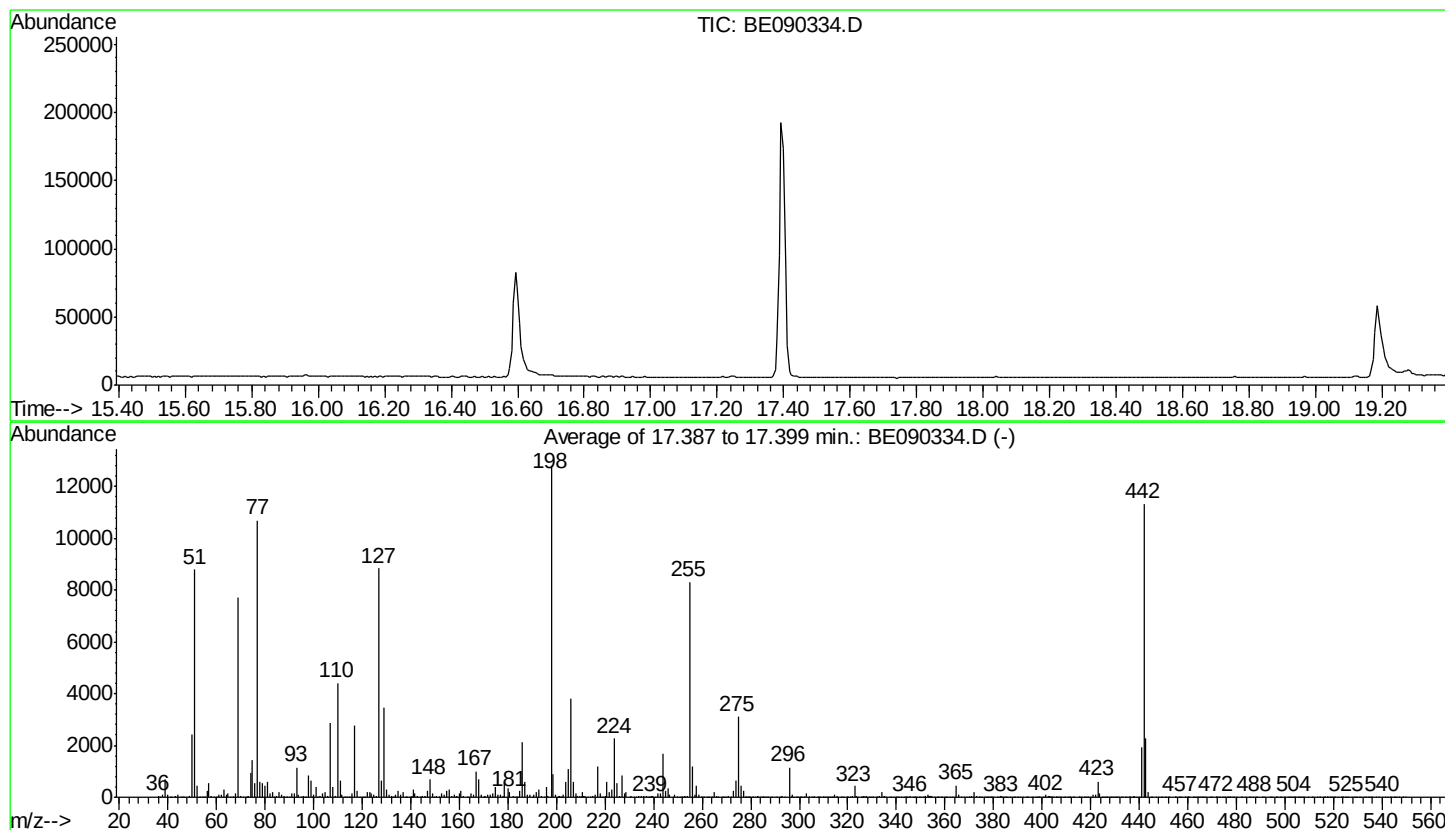

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.6	8786	PASS
68	69	0.00	2	2.0	153	PASS
69	198	0.00	100	60.2	7705	PASS
70	69	0.00	2	0.7	54	PASS
127	198	10	80	69.0	8842	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12806	PASS
199	198	5	9	6.8	870	PASS
275	198	10	60	24.2	3104	PASS
365	198	1	100	3.6	455	PASS
441	442	0.01	24	16.9	1916	PASS
442	198	50	100	88.5	11336	PASS
443	442	15	24	20.0	2270	PASS