

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080316\
 Data File : BE092161.D
 Acq On : 4 Aug 2016 1:09
 Operator : UM/SJ
 Sample : H4227-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS027-160725

Quant Time: Aug 04 03:58:36 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 16:59:37 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	12332	5.00	ng	0.00
6) Naphthalene-d8	10.98	136	59320	5.00	ng	-0.01
10) Acenaphthene-d10	14.83	164	34729	5.00	ng	-0.02
16) Phenanthrene-d10	17.56	188	76322	5.00	ng	-0.02
22) Chrysene-d12	21.75	240	92834	5.00	ng	0.00
28) Perylene-d12	24.14	264	91542	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.69	112	3625	1.14	ng	0.00
5) Phenol-d6	7.35	99	3919	0.93	ng	0.00
7) Nitrobenzene-d5	9.35	82	11023	2.35	ng	0.00
11) 2,4,6-Tribromophenol	16.33	330	5304	4.70	ng	0.00
12) 2-Fluorobiphenyl	13.46	172	28356	2.58	ng	0.00
24) Terphenyl-d14	20.19	244	53485	4.01	ng	-0.02
Target Compounds						
2) 1,4-Dioxane	3.44	88	102	0.06	ng	# 11
3) n-Nitrosodimethylamine	3.87	42	38	0.11	ng	# 19
8) Naphthalene	11.03	128	53	Below Cal		# 1
18) Pentachlorophenol	17.24	266	10	0.20	ng	# 78
19) Phenanthrene	17.60	178	217	Below Cal		# 70
30) Benzo(k)fluoranthene	23.40	252	87	Below Cal		# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080316\
Data File : BE092161.D
Acq On : 4 Aug 2016 1:09
Operator : UM/SJ
Sample : H4227-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
KY038PS027-160725

Quant Time: Aug 04 03:58:36 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 16:59:37 2016
Response via : Initial Calibration

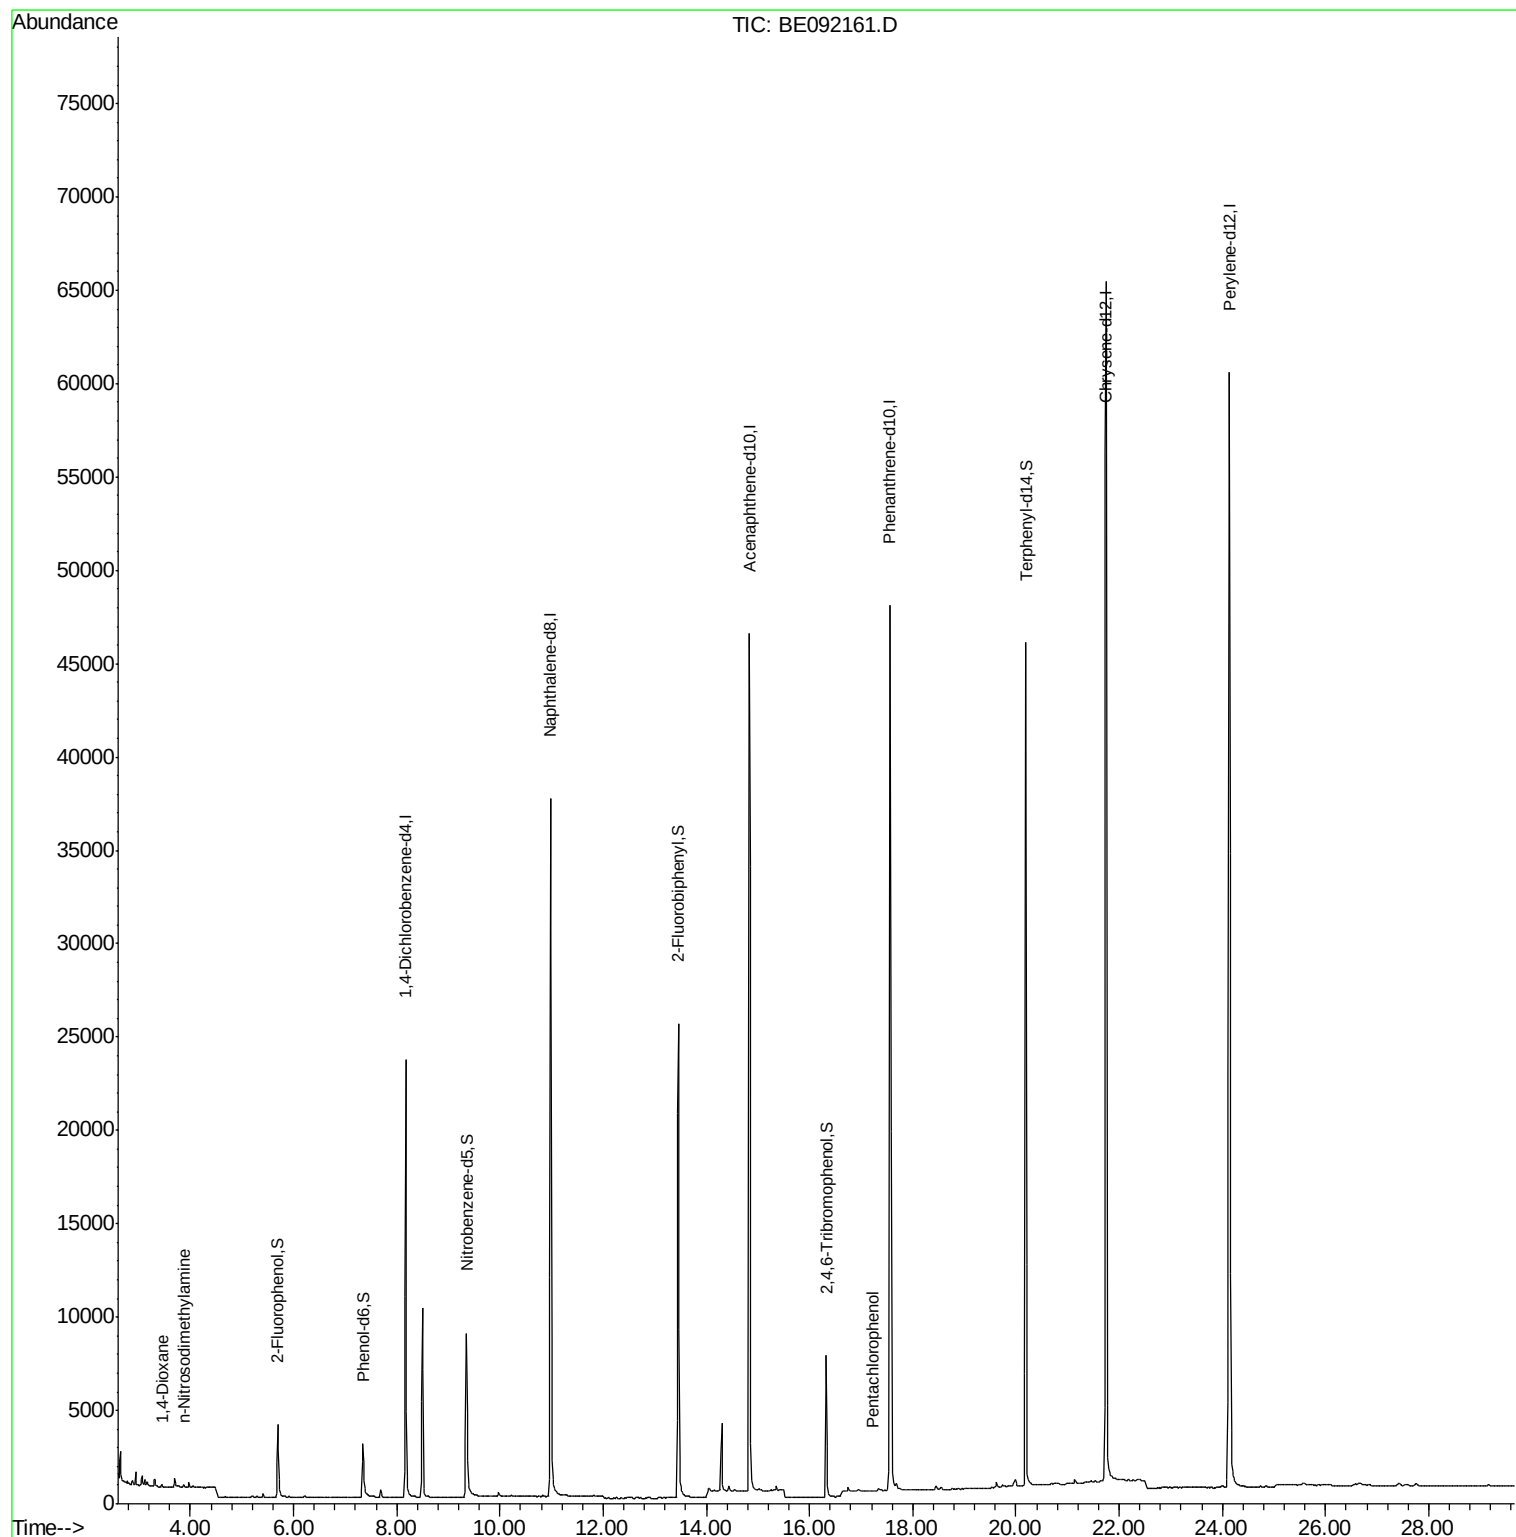

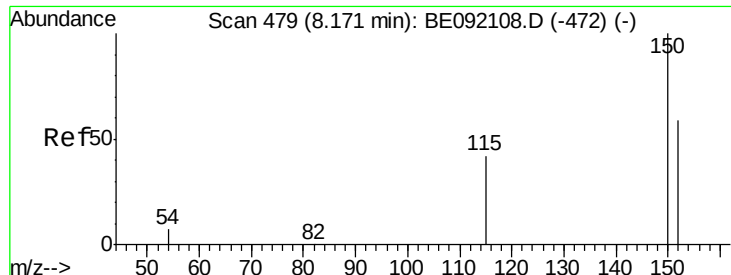

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.17 min Scan# 479

Delta R.T. -0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion:152 Resp: 12332

Ion Ratio Lower Upper

152 100

150 165.6 106.0 159.0#




115 69.0 36.9 55.3#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

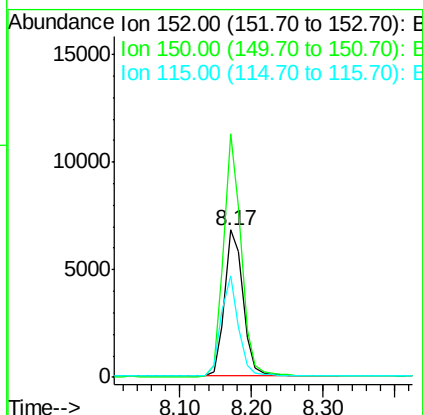

#2

1,4-Dioxane

Concen: 0.06 ng

RT: 3.44 min Scan# 74

Delta R.T. -0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09


Tgt Ion: 88 Resp: 102

Ion Ratio Lower Upper

88 100

58 0.0 62.1 93.1#



43 85.3 27.2 40.8#




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

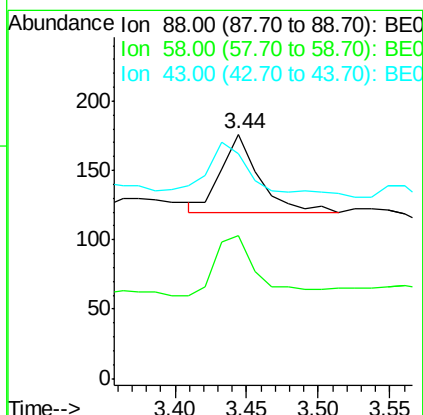

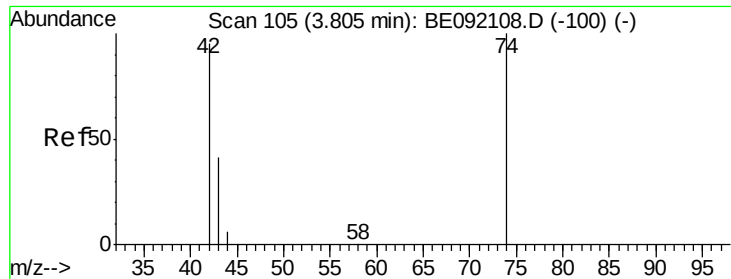

#3

n-Nitrosodimethylamine

Concen: 0.11 ng

RT: 3.87 min Scan# 111

Delta R.T. 0.07 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion: 42 Resp: 38

Ion Ratio Lower Upper

42 100

74 26.3 82.8 124.2#




44 60.5 9.0 13.4#

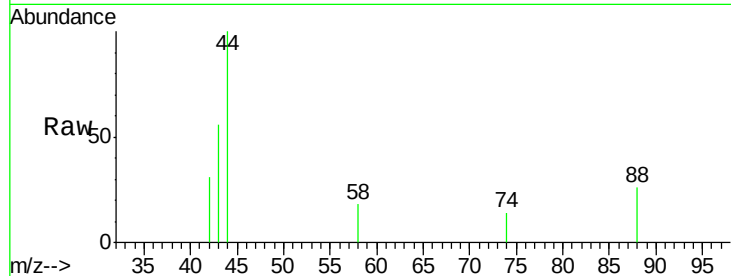

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

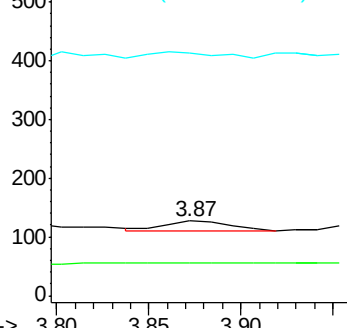

#4

2-Fluorophenol

Concen: 1.14 ng

RT: 5.69 min Scan# 267

Delta R.T. -0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09


Tgt Ion: 112 Resp: 3625

Ion Ratio Lower Upper

112 100

64 67.9 55.9 83.9



63 36.8 31.1 46.7




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

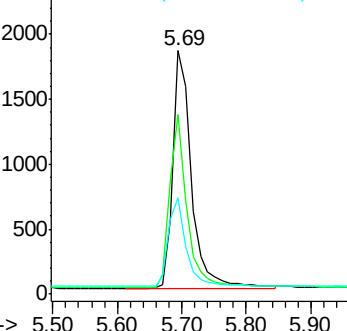

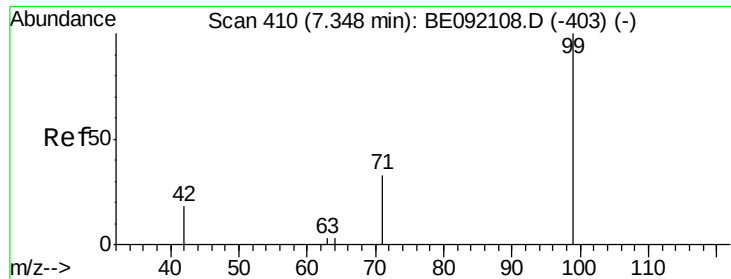

#5

Phenol-d6

Concen: 0.93 ng

RT: 7.35 min Scan# 410

Delta R.T. -0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion: 99 Resp: 3919

Ion Ratio Lower Upper

99 100

42 24.5 22.4 33.6




71 37.5 28.9 43.3



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

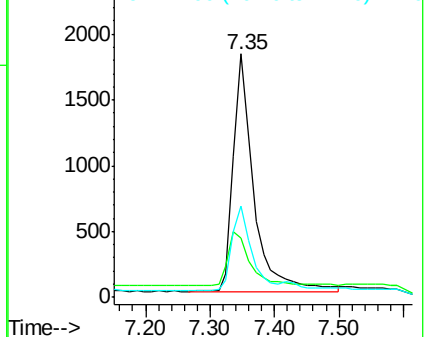

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.98 min Scan# 703

Delta R.T. -0.01 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Tgt Ion: 136 Resp: 59320


Ion Ratio Lower Upper

136 100

137 10.3 9.1 13.7

54 11.1 2.7 4.1#

68 7.7 2.2 3.4#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

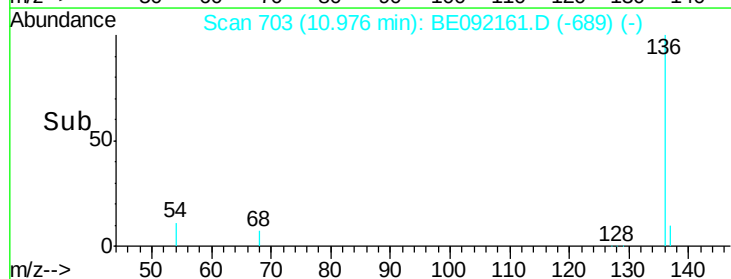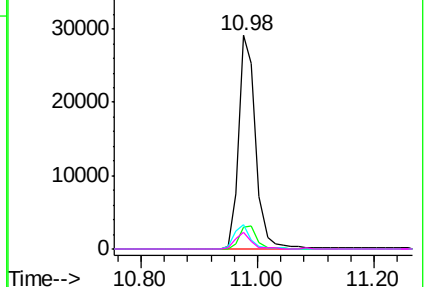

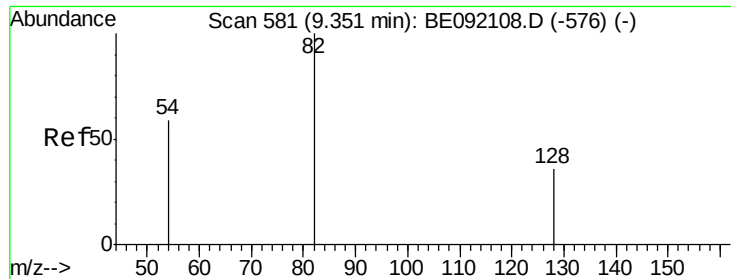

#7

Nitrobenzene-d5

Concen: 2.35 ng

RT: 9.35 min Scan# 581

Delta R.T. -0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion: 82 Resp: 11023

Ion Ratio Lower Upper

82 100

128 41.4 33.0 49.4


54 55.8 42.6 63.8

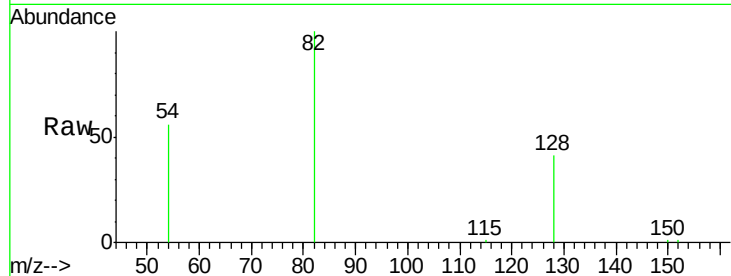



Abundance Ion 82.00 (81.70 to 82.70): BE092108.D (-576) (-)

Ion 128.00 (127.70 to 128.70): BE092108.D (-576) (-)

Ion 54.00 (53.70 to 54.70): BE092108.D (-576) (-)

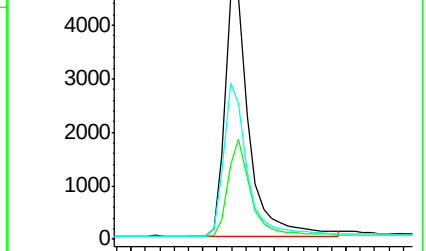

Time-->



#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.83 min Scan# 998

Delta R.T. -0.02 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09


Tgt Ion: 164 Resp: 34729

Ion Ratio Lower Upper

164 100

162 117.7 69.5 104.3#


160 59.0 27.6 41.4#




Abundance Ion 164.00 (163.70 to 164.70): BE092108.D (-992) (-)


Ion 162.00 (161.70 to 162.70): BE092108.D (-992) (-)

Ion 160.00 (159.70 to 160.70): BE092108.D (-992) (-)

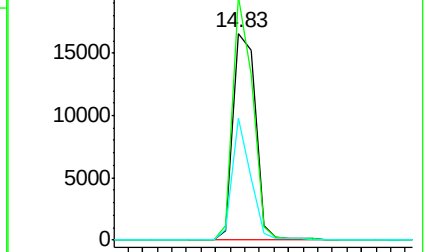

Time-->







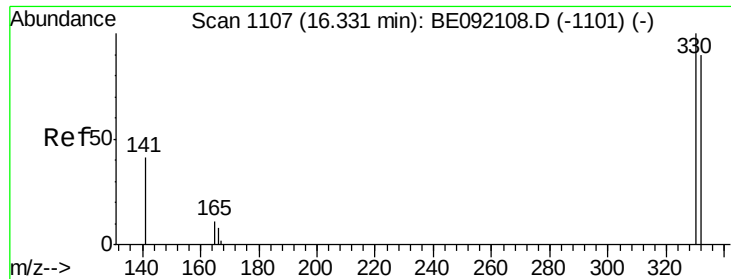

#11
 2,4,6-Tribromophenol
 Concen: 4.70 ng
 RT: 16.33 min Scan# 1107
 Delta R.T. -0.00 min
 Lab File: BE092161.D
 Acq: 4 Aug 2016 1:09




Instrument :
 BNA_E
 ClientSampleId :
 KY038PS027-160725


Tgt Ion:330 Resp: 5304
 Ion Ratio Lower Upper
 330 100
 332 96.3 74.2 111.4
 141 41.7 139.8 209.8#

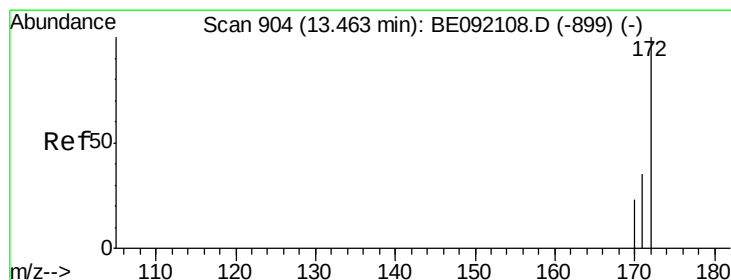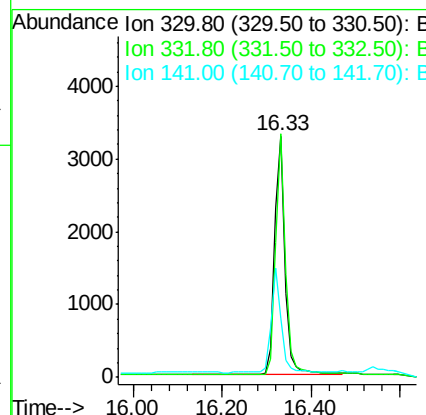

#12
 2-Fluorobiphenyl
 Concen: 2.58 ng
 RT: 13.46 min Scan# 904
 Delta R.T. -0.00 min
 Lab File: BE092161.D
 Acq: 4 Aug 2016 1:09

Tgt Ion:172 Resp: 28356
 Ion Ratio Lower Upper
 172 100
 171 31.3 30.3 45.5
 170 19.2 21.6 32.4#

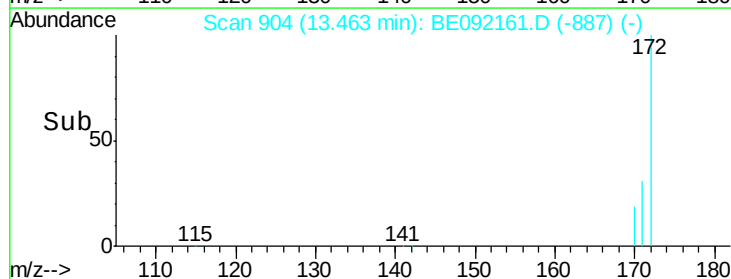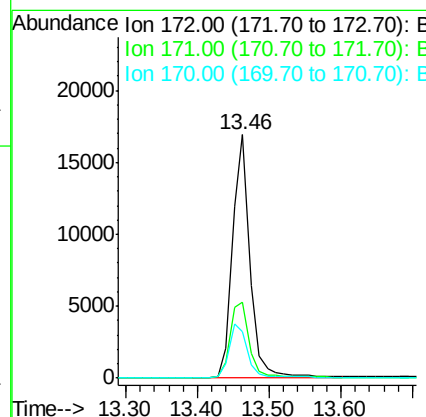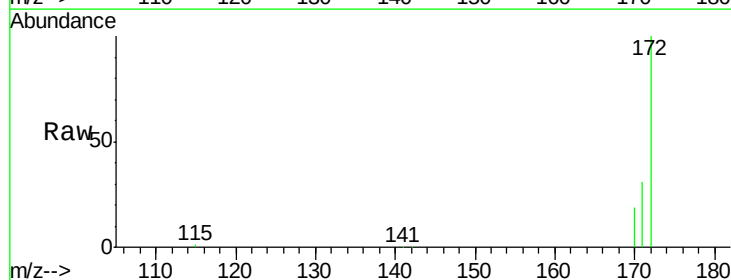

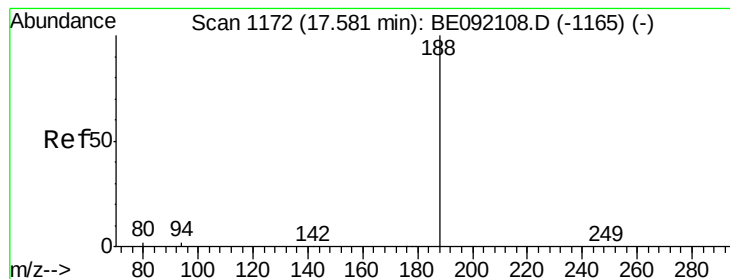

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1171

Delta R.T. -0.02 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion:188 Resp: 76322

Ion Ratio Lower Upper

188 100

94 16.6 3.9 5.9#




80 17.4 3.4 5.0#

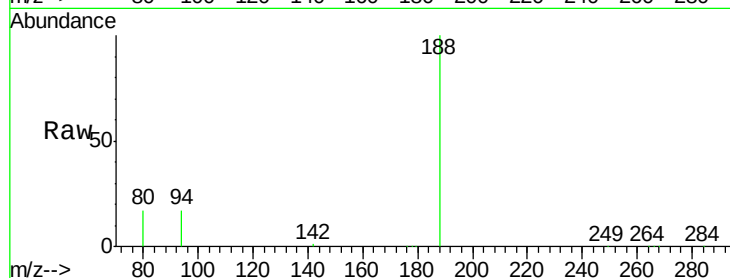

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

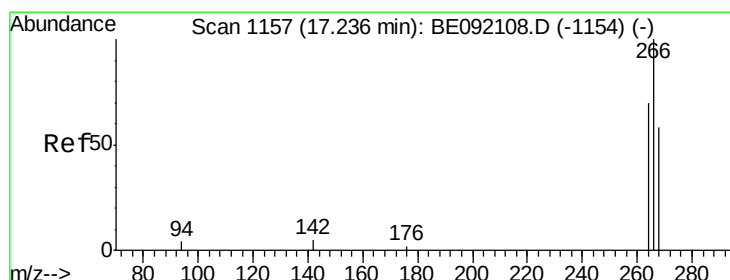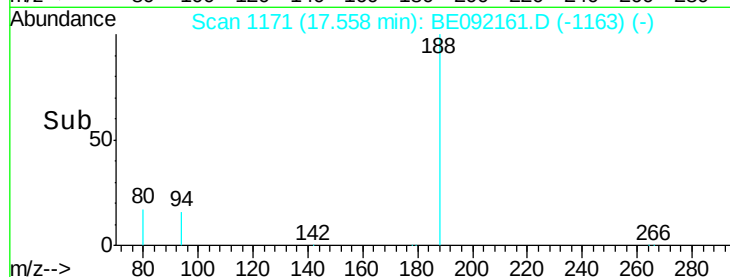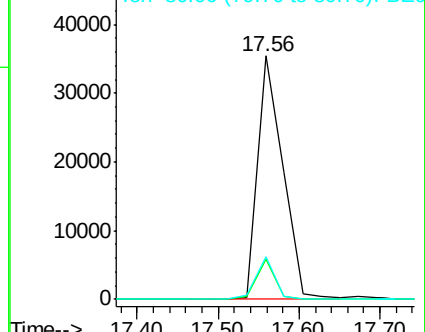

#18

Pentachlorophenol

Concen: 0.20 ng

RT: 17.24 min Scan# 1157

Delta R.T. 0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09


Tgt Ion:266 Resp: 10

Ion Ratio Lower Upper

266 100

268 102.0 62.7 94.1#



264 93.9 63.5 95.3

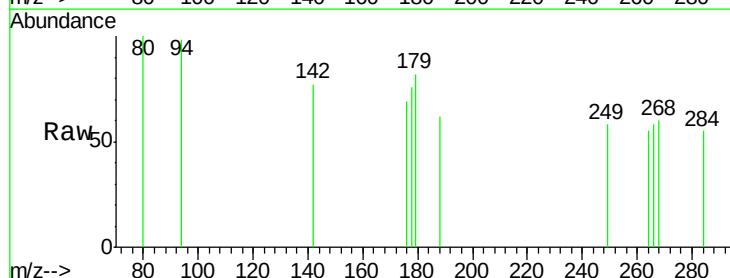


Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E

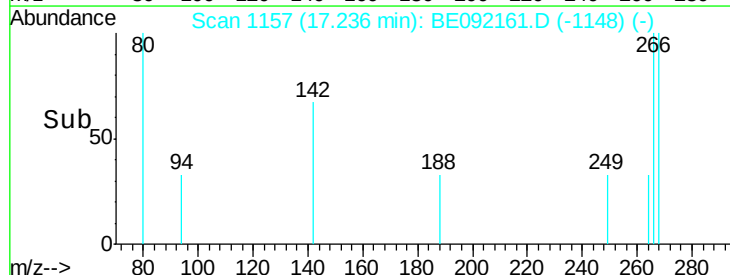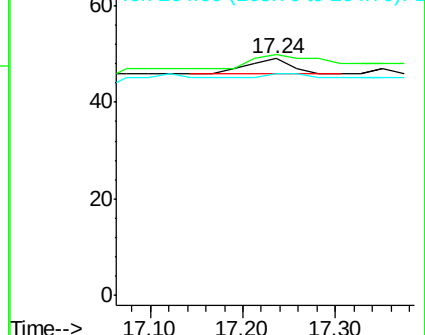

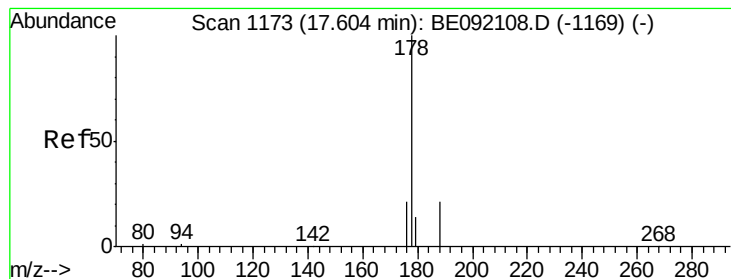

#19

Phenanthrene

Concen: Below Cal

RT: 17.60 min Scan# 1173

Delta R.T. 0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion:178 Resp: 217

Ion Ratio Lower Upper

178 100

176 30.0 15.4 23.0#




179 0.0 12.7 19.1#



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

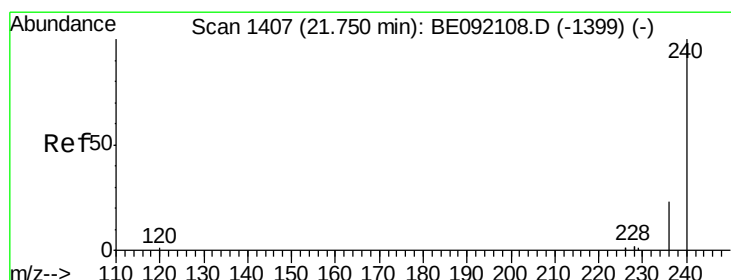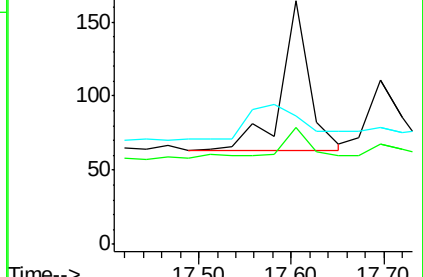

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1407

Delta R.T. -0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09


Tgt Ion:240 Resp: 92834

Ion Ratio Lower Upper

240 100

120 1.2 0.6 1.0#



236 22.5 18.2 27.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

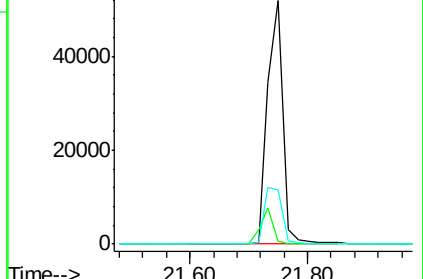



#24

Terphenyl-d14

Concen: 4.01 ng

RT: 20.19 min Scan# 1317

Delta R.T. -0.02 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09

Instrument :

BNA_E

ClientSampleId :

KY038PS027-160725


Tgt Ion:244 Resp: 53485

Ion Ratio Lower Upper

244 100

212 8.9 9.1 13.7#




122 7.4 11.0 16.4#

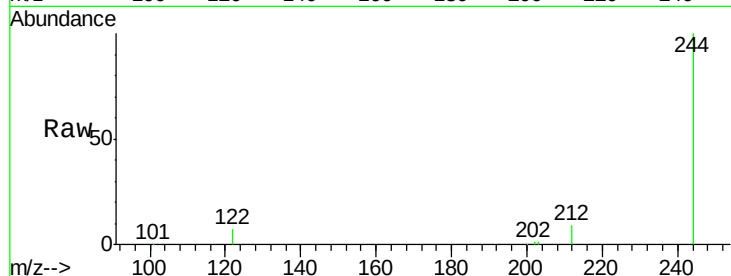

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

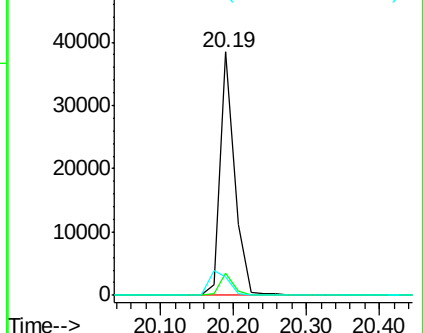

#28

Perylene-d12

Concen: 5.00 ng

RT: 24.14 min Scan# 1591

Delta R.T. 0.00 min

Lab File: BE092161.D

Acq: 4 Aug 2016 1:09


Tgt Ion:264 Resp: 91542

Ion Ratio Lower Upper

264 100

260 24.4 20.8 31.2

265 22.8 16.6 25.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

