


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080316\
 Data File : BE092148.D
 Acq On : 3 Aug 2016 16:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 16:59:37 2016

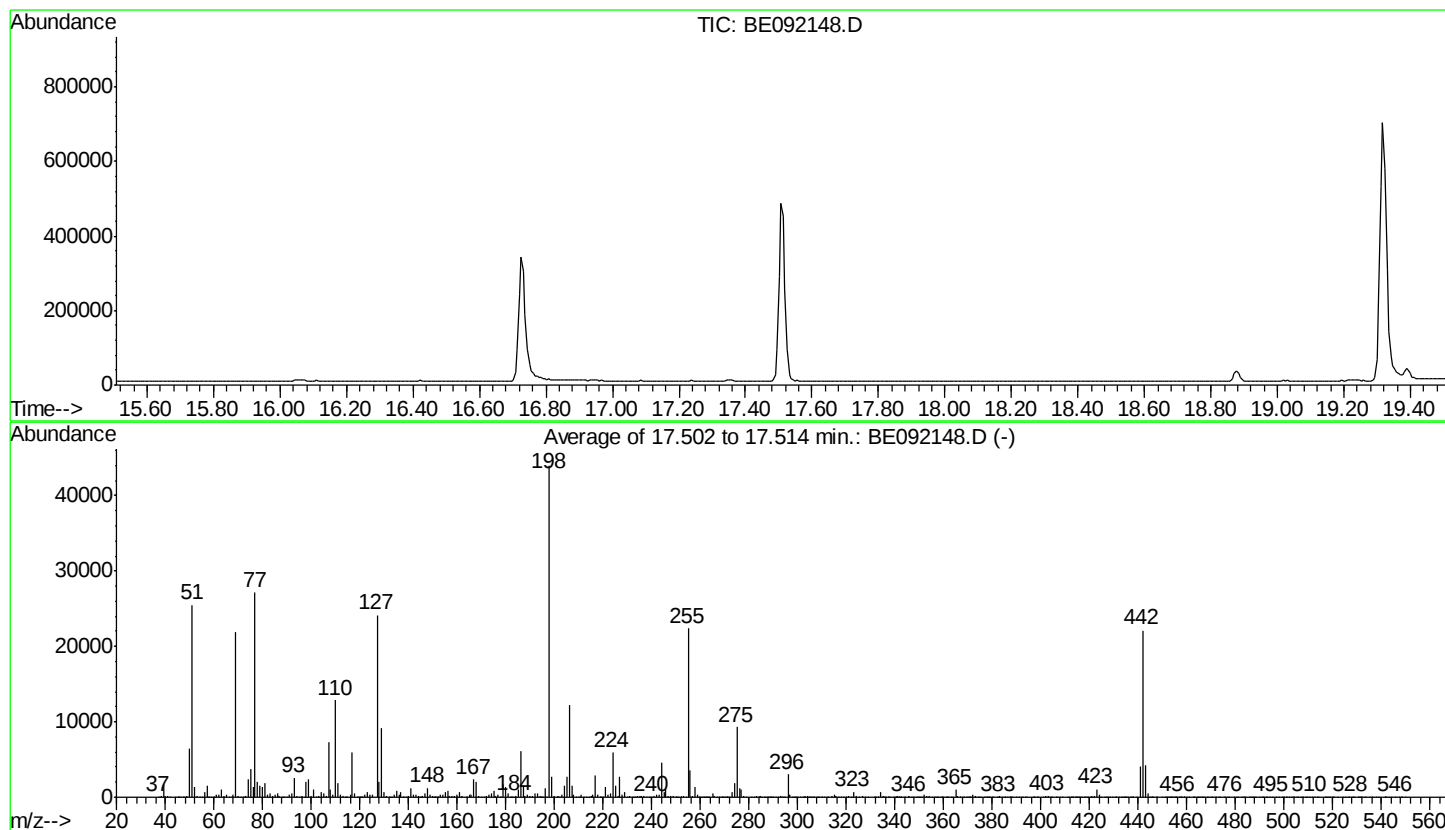

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.9	25486	PASS
68	69	0.00	2	1.7	380	PASS
69	198	0.00	100	49.6	21833	PASS
70	69	0.00	2	0.7	144	PASS
127	198	10	80	54.8	24113	PASS
197	198	0.00	2	0.1	53	PASS
198	198	100	100	100.0	43988	PASS
199	198	5	9	6.3	2762	PASS
275	198	10	60	21.1	9300	PASS
365	198	1	100	2.3	1002	PASS
441	442	0.01	24	18.1	4016	PASS
442	198	50	100	50.4	22155	PASS
443	442	15	24	19.5	4311	PASS