


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080316\
 Data File : BE092165.D
 Acq On : 4 Aug 2016 3:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 16:59:37 2016

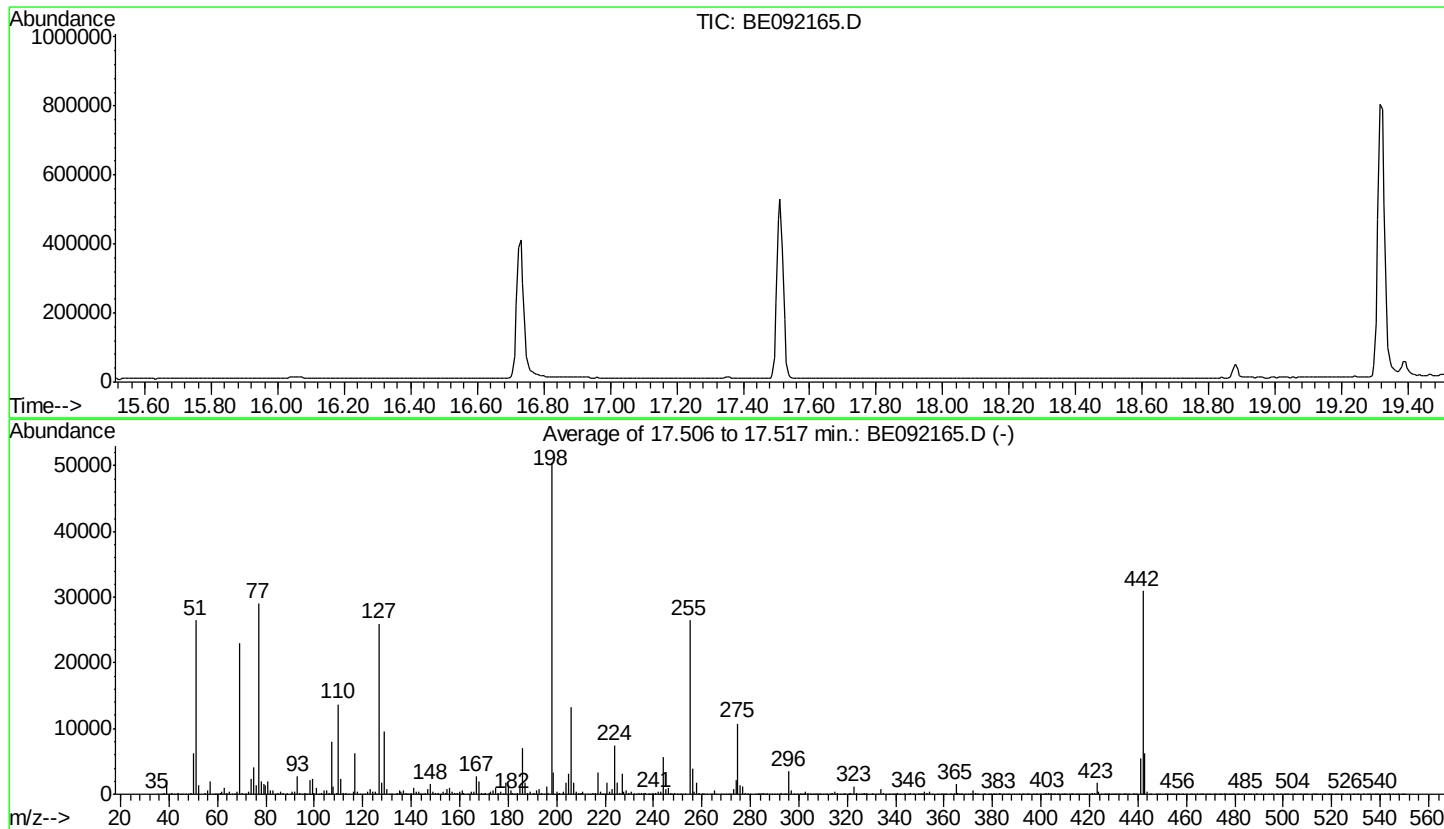

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	26456	PASS
68	69	0.00	2	1.8	427	PASS
69	198	0.00	100	45.7	23087	PASS
70	69	0.00	2	0.5	114	PASS
127	198	10	80	51.5	26001	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50488	PASS
199	198	5	9	6.7	3387	PASS
275	198	10	60	21.3	10735	PASS
365	198	1	100	2.9	1485	PASS
441	442	0.01	24	17.7	5464	PASS
442	198	50	100	61.3	30938	PASS
443	442	15	24	20.3	6283	PASS