
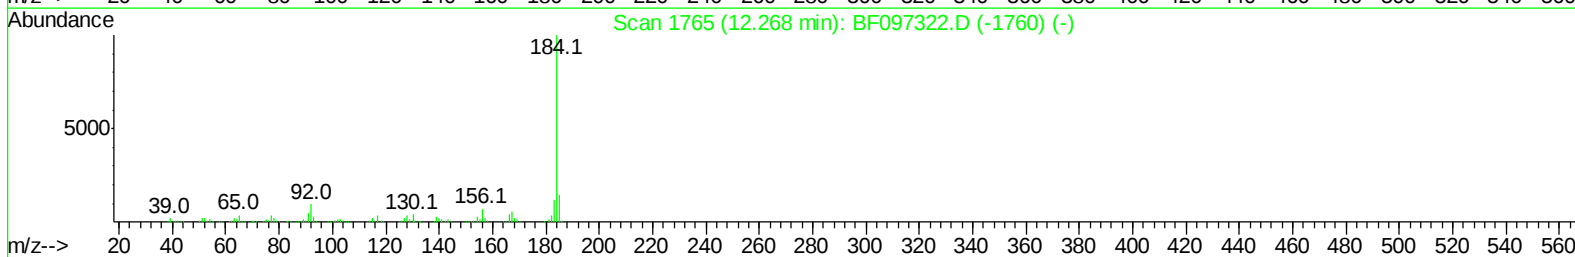
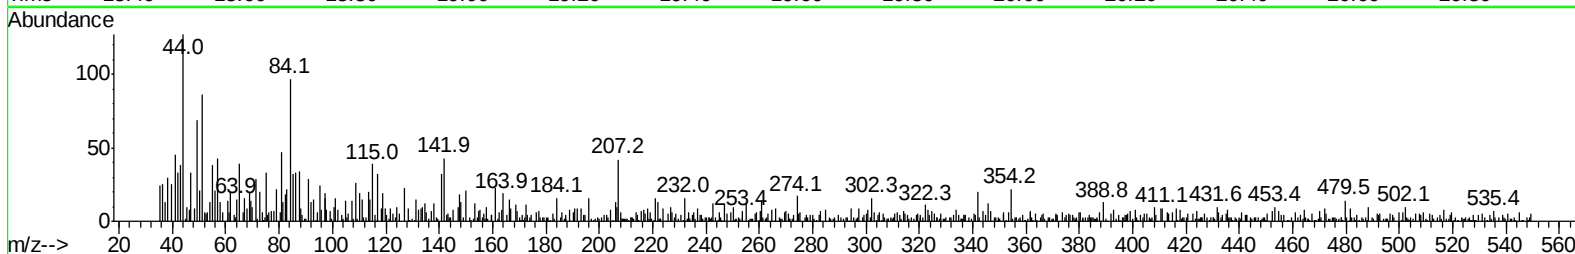


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080317\
Data File : BE093648.D
Acq On : 3 Aug 2017 8:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 05:27:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 01:17:22 2017
Response via : Initial Calibration

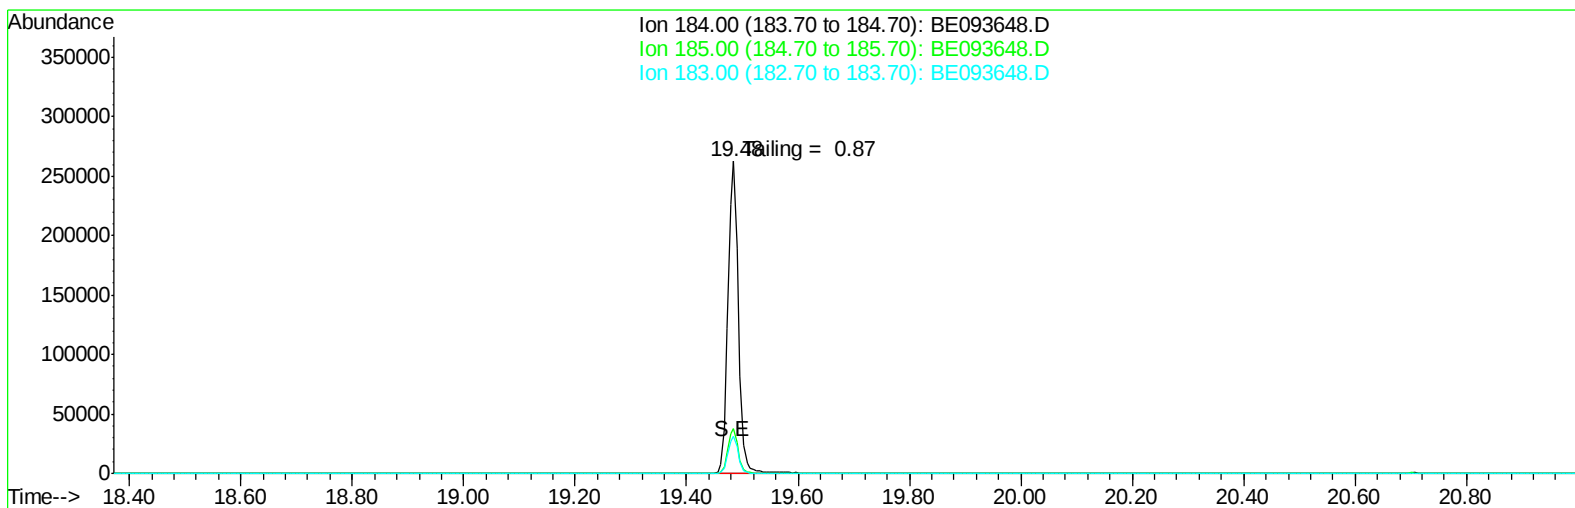

TIC: BE093648.D

(76) Benzidine




12.569min (+0.236) 12.68ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	18.75
183.00	12.20	12.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080317\
 Data File : BE093648.D
 Acq On : 3 Aug 2017 8:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 05:27:34 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 01:17:22 2017
 Response via : Initial Calibration

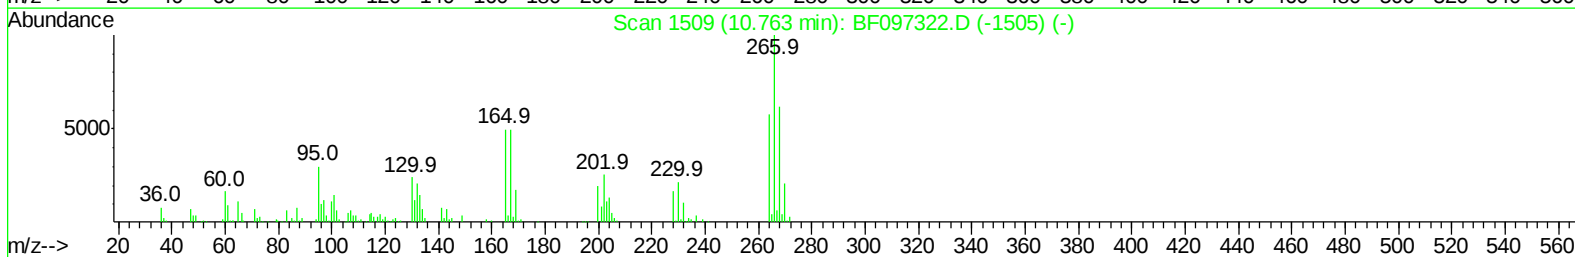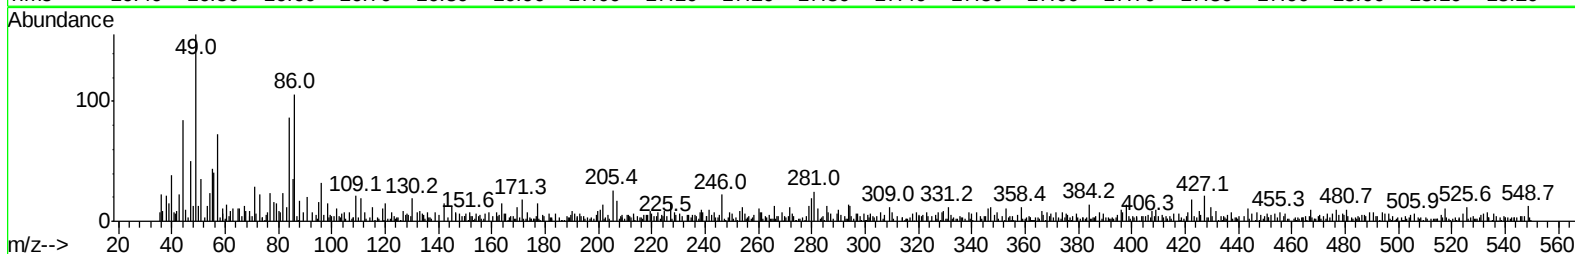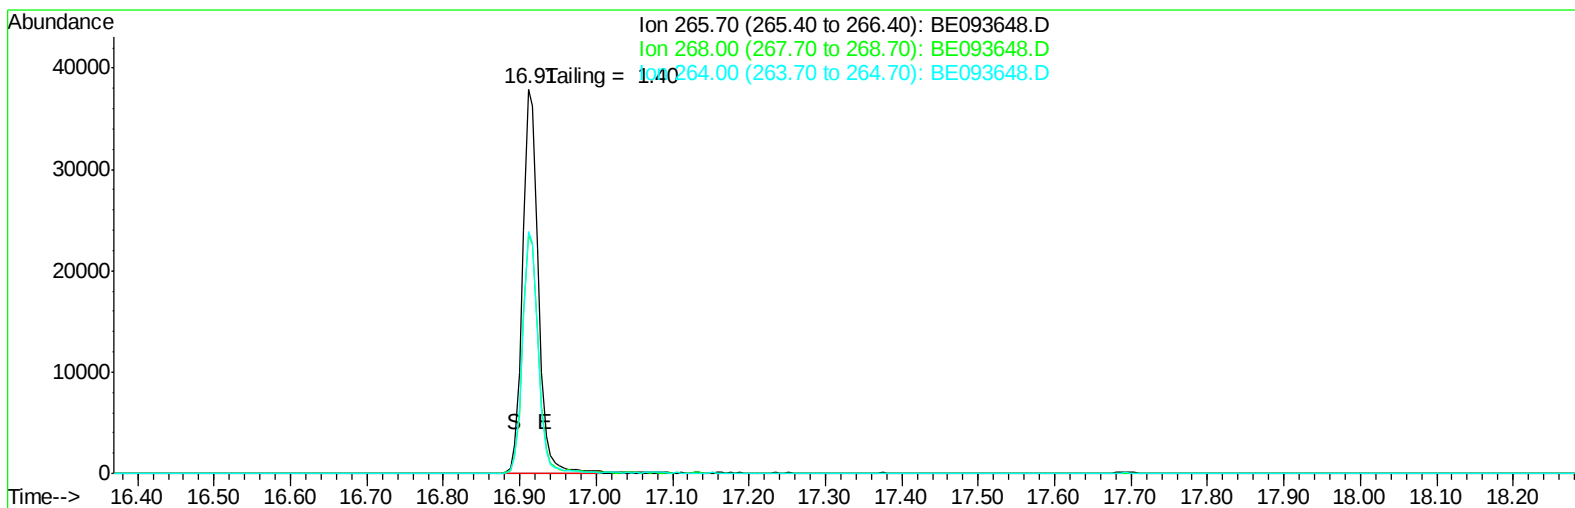

TIC: BE093648.D

(69) Pentachlorophenol (C)

10.818min (-0.003) 296.95ng

response 22

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	46.67#
264.00	64.60	46.67#
0.00	0.00	0.00