


Data Path : Z:\HPCHEM1\BNA E\Data\BE080317\
 Data File : BE093648.D
 Acq On : 3 Aug 2017 8:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 02 10:58:31 2017

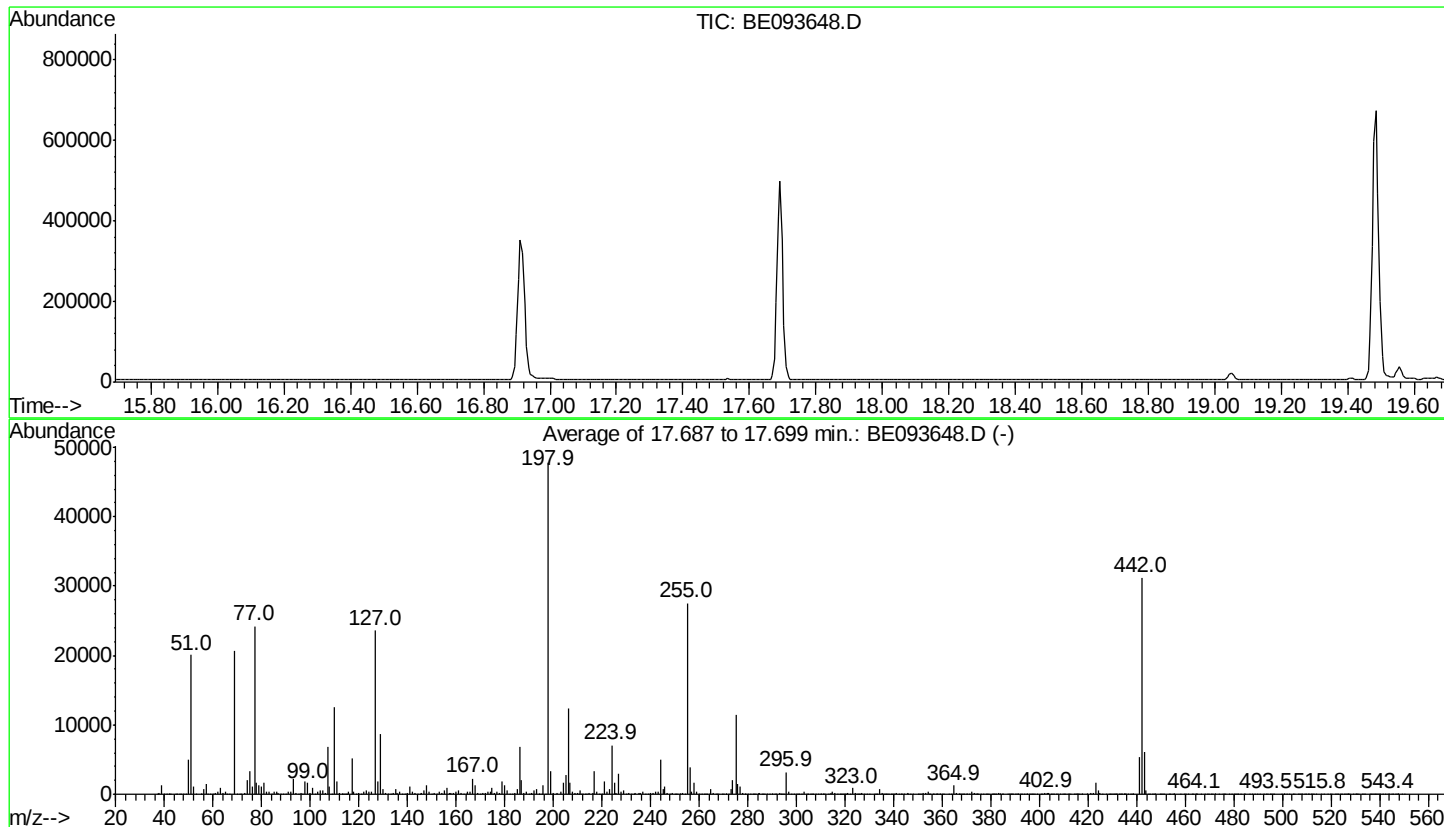

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	20095	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.3	20690	PASS
70	69	0.00	2	0.3	67	PASS
127	198	10	80	49.3	23578	PASS
197	198	0.00	2	0.2	82	PASS
198	198	100	100	100.0	47794	PASS
199	198	5	9	6.9	3297	PASS
275	198	10	60	23.9	11441	PASS
365	198	1	100	2.7	1268	PASS
441	442	0.01	24	17.1	5355	PASS
442	198	50	100	65.4	31253	PASS
443	442	15	24	19.8	6184	PASS