


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080415\
Data File : BE090343.D
Acq On : 4 Aug 2015 14:32
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 04 02:31:31 2015

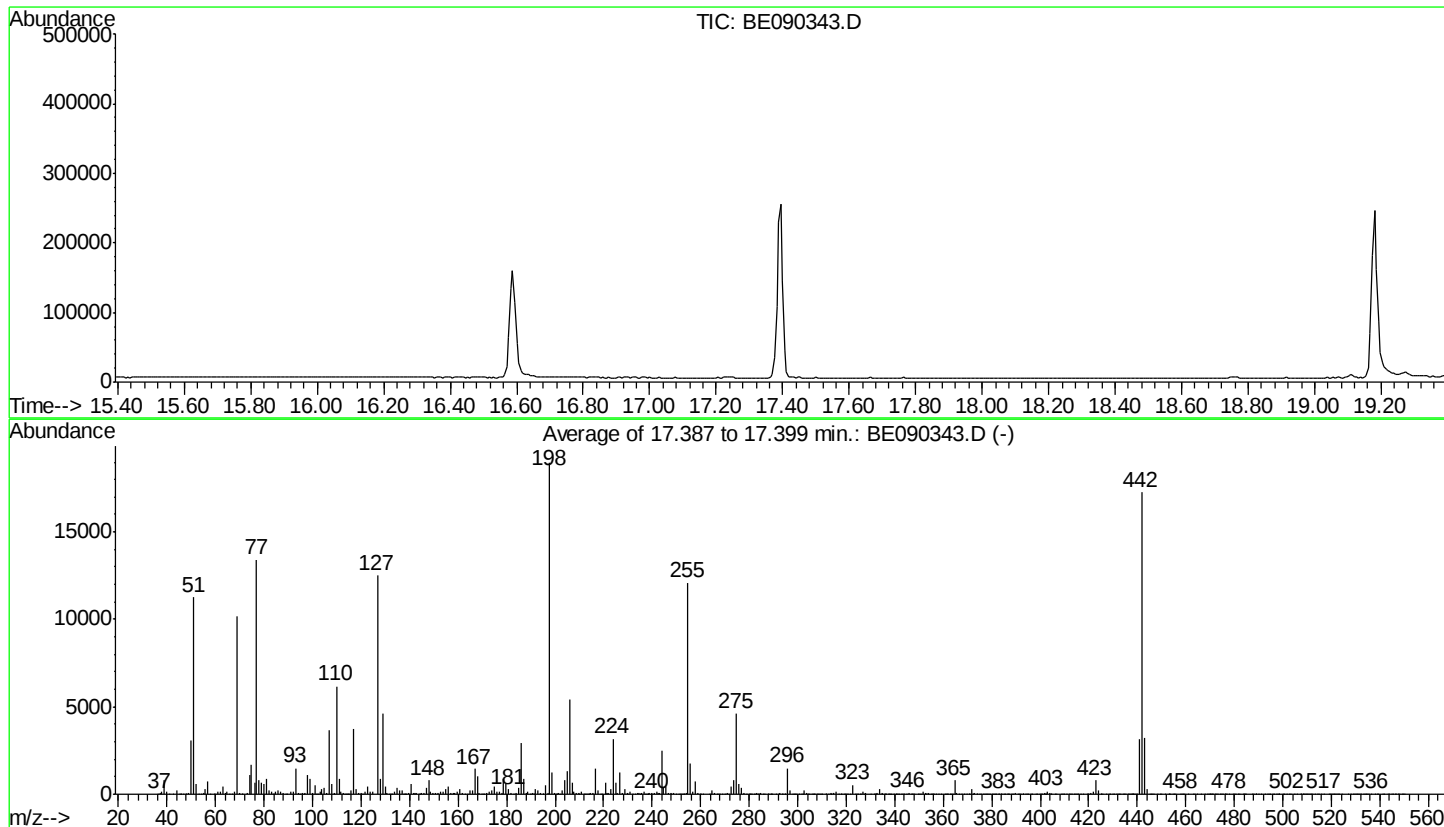

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.4	11273	PASS
68	69	0.00	2	1.3	132	PASS
69	198	0.00	100	53.5	10148	PASS
70	69	0.00	2	0.7	67	PASS
127	198	10	80	65.9	12504	PASS
197	198	0.00	2	0.3	54	PASS
198	198	100	100	100.0	18966	PASS
199	198	5	9	6.4	1222	PASS
275	198	10	60	24.2	4591	PASS
365	198	1	100	4.2	801	PASS
441	442	0.01	24	18.2	3144	PASS
442	198	50	100	91.1	17273	PASS
443	442	15	24	18.5	3191	PASS