

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080416\
 Data File : BE092188.D
 Acq On : 4 Aug 2016 18:39
 Operator : UM/SJ
 Sample : H4205-09RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 GW-42-6.1-15.0

Quant Time: Aug 05 03:13:48 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 16:59:37 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	13062	5.00	ng	0.00
6) Naphthalene-d8	10.98	136	57283	5.00	ng	-0.01
10) Acenaphthene-d10	14.83	164	30214	5.00	ng	-0.02
16) Phenanthrene-d10	17.56	188	64296	5.00	ng	-0.02
22) Chrysene-d12	21.75	240	79263	5.00	ng	0.00
28) Perylene-d12	24.14	264	85190	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.69	112	29479	8.79	ng	0.00
5) Phenol-d6	7.34	99	25910	5.80	ng	-0.01
7) Nitrobenzene-d5	9.34	82	29904	6.62	ng	-0.01
11) 2,4,6-Tribromophenol	16.33	330	15380	15.68	ng	0.00
12) 2-Fluorobiphenyl	13.46	172	62337	6.51	ng	0.00
24) Terphenyl-d14	20.19	244	83600	7.34	ng	-0.02
Target Compounds						
3) n-Nitrosodimethylamine	3.74	42	125	0.14	ng	# 13
8) Naphthalene	11.03	128	82	Below Cal		# 1
18) Pentachlorophenol	17.24	266	3	0.20	ng	# 76
19) Phenanthrene	17.60	178	189	Below Cal		# 80
25) Benzo(a)anthracene	21.73	228	1949	0.02	ng	# 71
26) Chrysene	21.73	228	1949	0.02	ng	# 74
30) Benzo(k)fluoranthene	23.46	252	117	Below Cal		# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080416\
Data File : BE092188.D
Acq On : 4 Aug 2016 18:39
Operator : UM/SJ
Sample : H4205-09RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
GW-42-6.1-15.0

Quant Time: Aug 05 03:13:48 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 16:59:37 2016
Response via : Initial Calibration

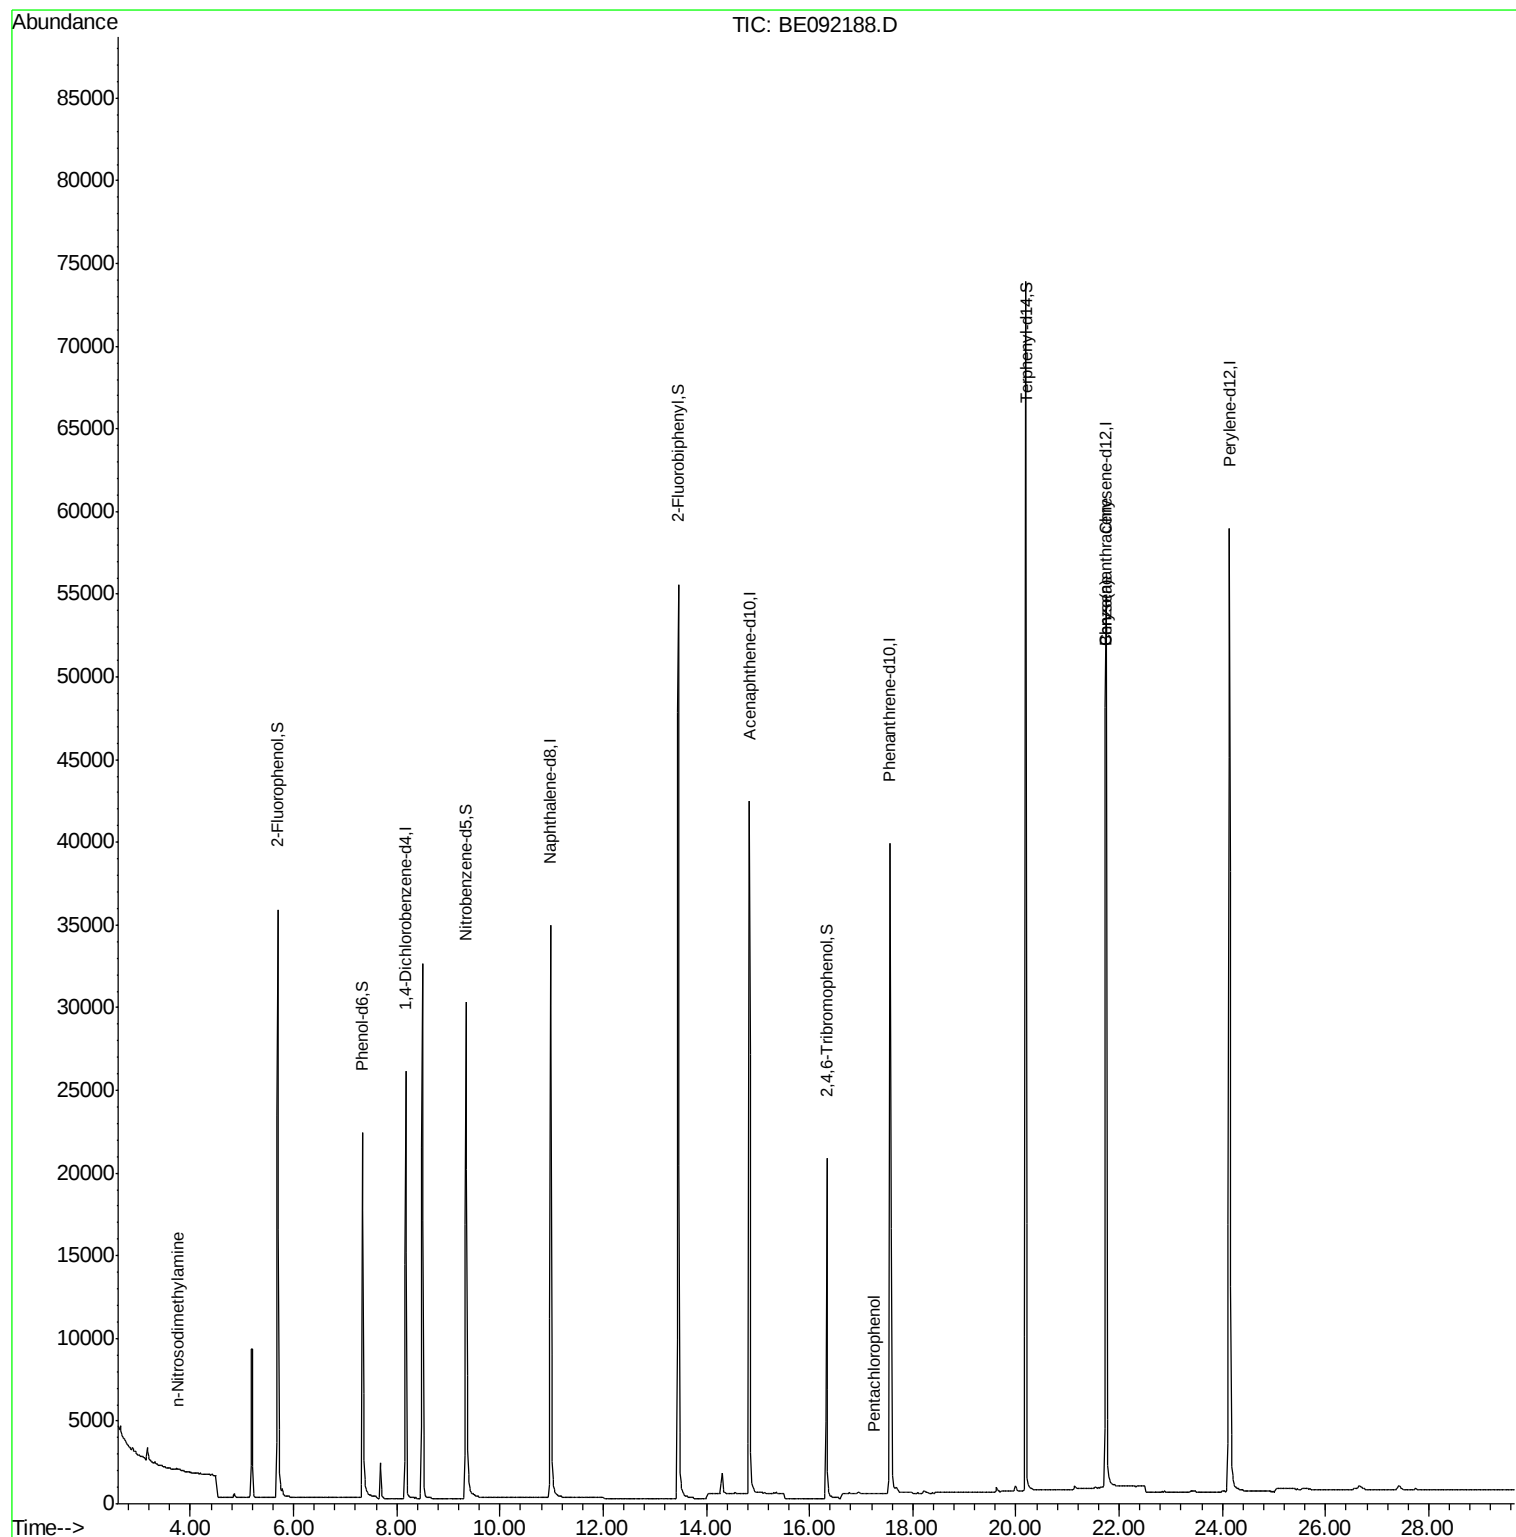

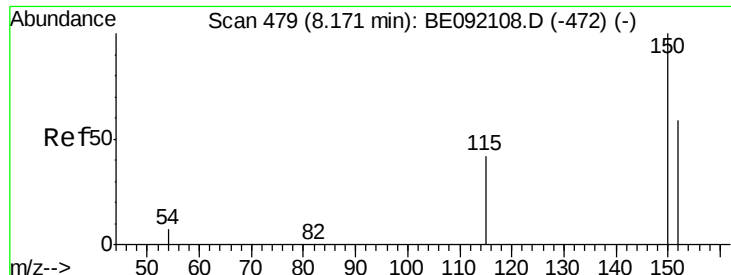

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.17 min Scan# 479

Delta R.T. -0.00 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39

Instrument :

BNA_E

ClientSampleId :

GW-42-6.1-15.0





Tgt Ion:152 Resp: 13062

Ion Ratio Lower Upper

152 100

150 161.8 106.0 159.0#

115 62.1 36.9 55.3#

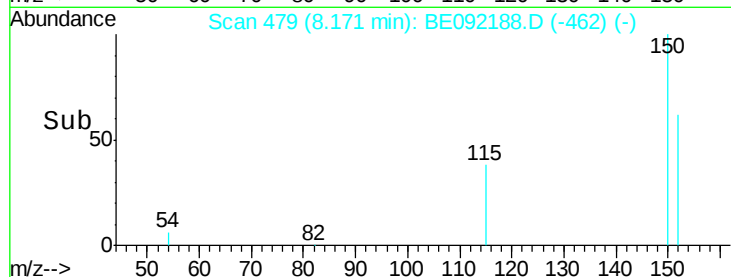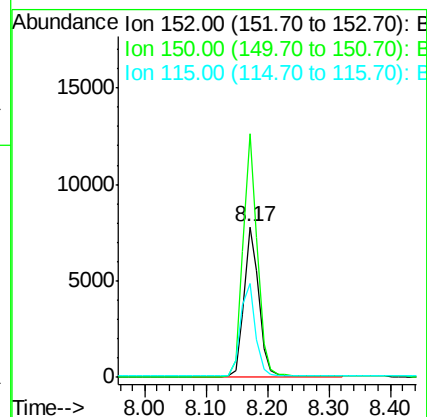

#3

n-Nitrosodimethylamine

Concen: 0.14 ng

RT: 3.74 min Scan# 100

Delta R.T. -0.06 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39




Tgt Ion: 42 Resp: 125


Ion Ratio Lower Upper

42 100

74 8.0 82.8 124.2#

44 0.0 9.0 13.4#

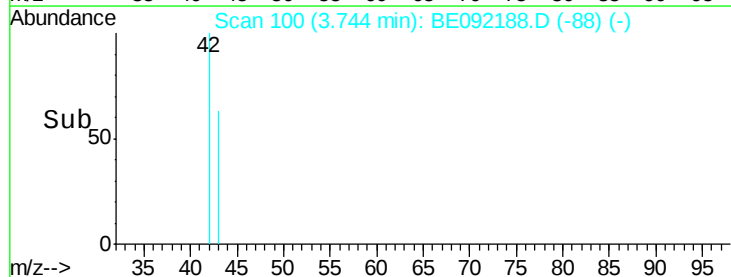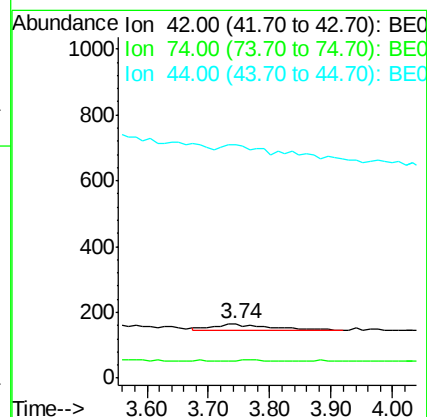

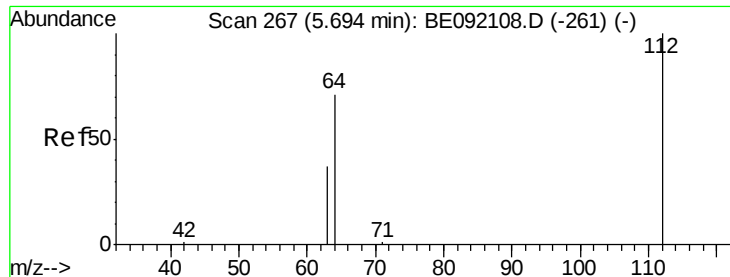

#4

2-Fluorophenol

Concen: 8.79 ng

RT: 5.69 min Scan# 267

Delta R.T. 0.00 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39

Instrument :

BNA_E

ClientSampleId :

GW-42-6.1-15.0


Tgt Ion: 112 Resp: 29479

Ion Ratio Lower Upper

112 100

64 67.0 55.9 83.9




63 36.4 31.1 46.7

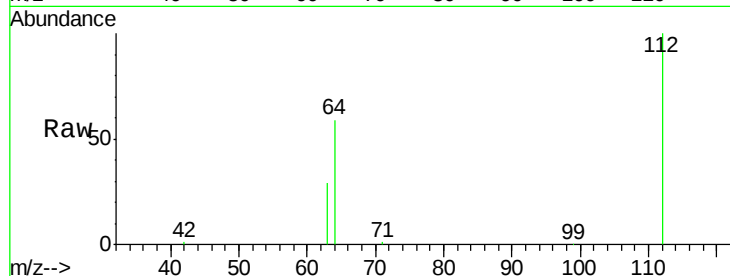

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

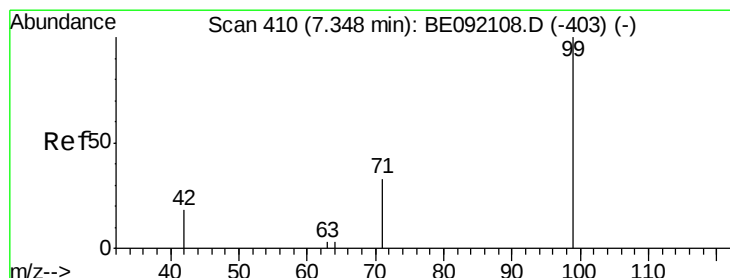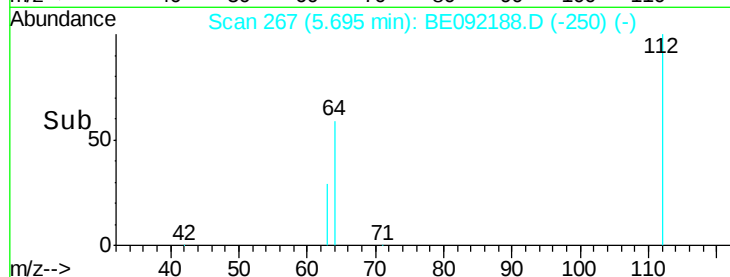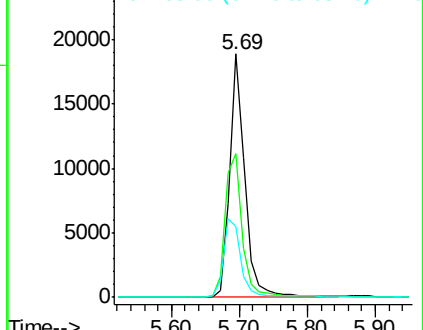

#5

Phenol-d6

Concen: 5.80 ng

RT: 7.34 min Scan# 409

Delta R.T. -0.01 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39


Tgt Ion: 99 Resp: 25910

Ion Ratio Lower Upper

99 100

42 25.0 22.4 33.6



71 35.4 28.9 43.3

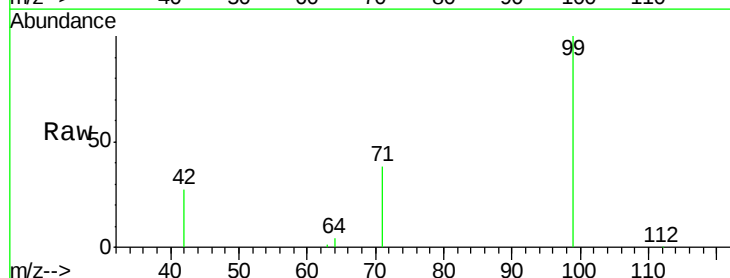


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

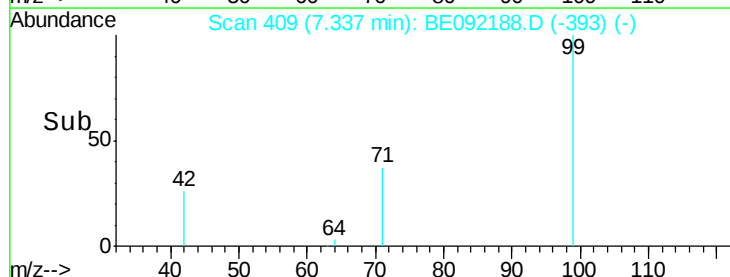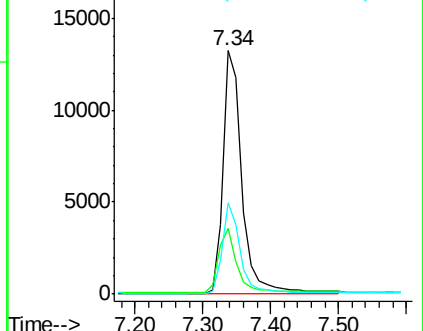


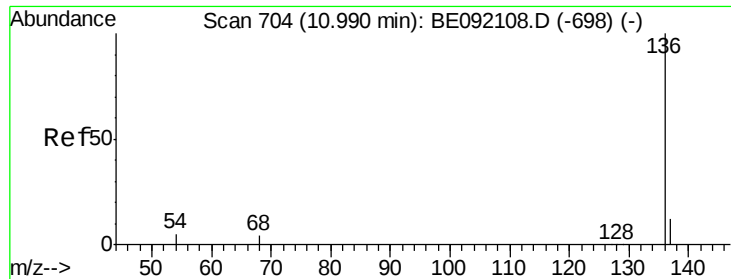




#6
Naphthalene-d8
Concen: 5.00 ng
RT: 10.98 min Scan# 703
Delta R.T. -0.01 min
Lab File: BE092188.D
Acq: 4 Aug 2016 18:39

Instrument :
BNA_E
ClientSampleId :
GW-42-6.1-15.0

Tgt Ion: 136 Resp: 57283
Ion Ratio Lower Upper
136 100
137 10.3 9.1 13.7
54 11.3 2.7 4.1#
68 7.7 2.2 3.4#




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

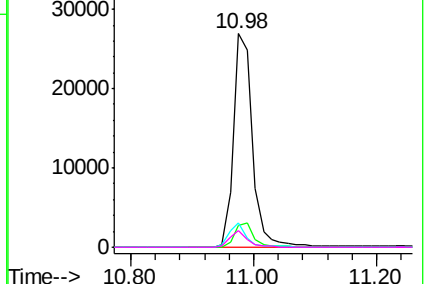
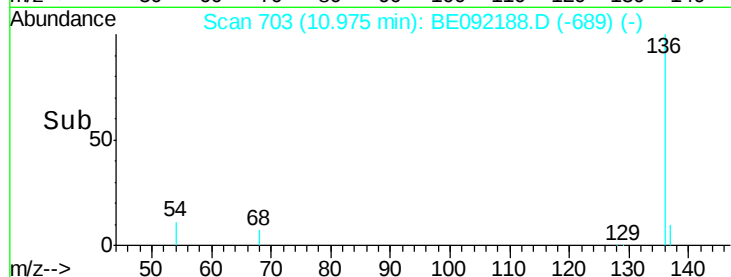



#7
Nitrobenzene-d5
Concen: 6.62 ng
RT: 9.34 min Scan# 580
Delta R.T. -0.01 min
Lab File: BE092188.D
Acq: 4 Aug 2016 18:39

Tgt Ion: 82 Resp: 29904
Ion Ratio Lower Upper
82 100
128 35.2 33.0 49.4
54 60.4 42.6 63.8



Abundance Ion 82.00 (81.70 to 82.70): BE0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE0

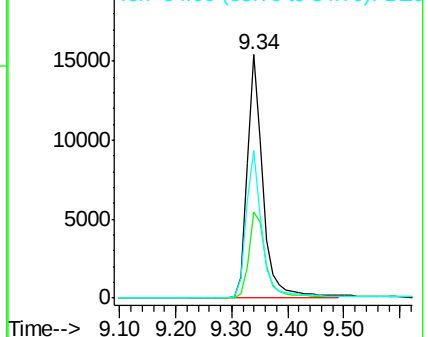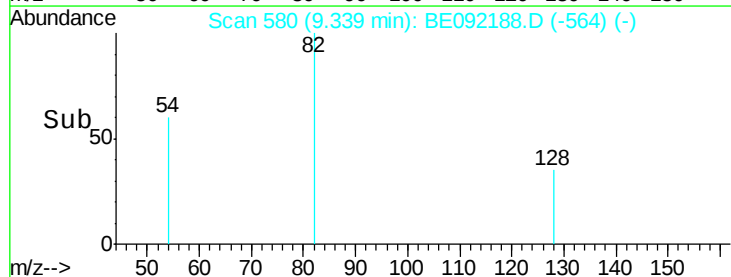

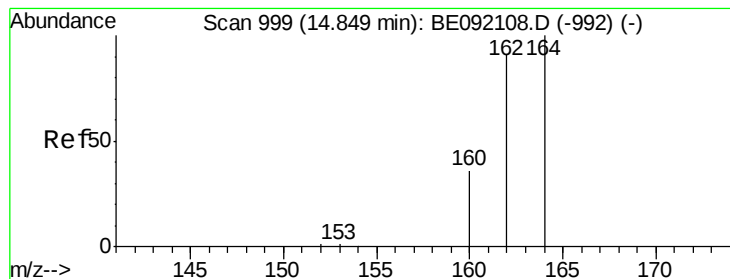

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.83 min Scan# 998

Delta R.T. -0.02 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39

Instrument :

BNA_E

ClientSampleId :

GW-42-6.1-15.0





Tgt Ion:164 Resp: 30214

Ion Ratio Lower Upper

164 100

162 115.7 69.5 104.3#

160 56.9 27.6 41.4#

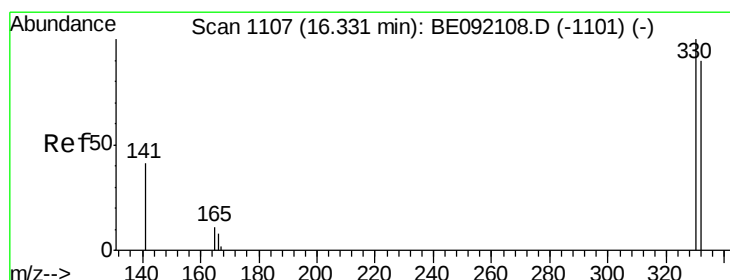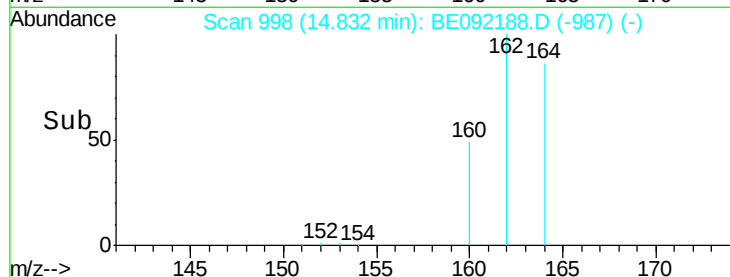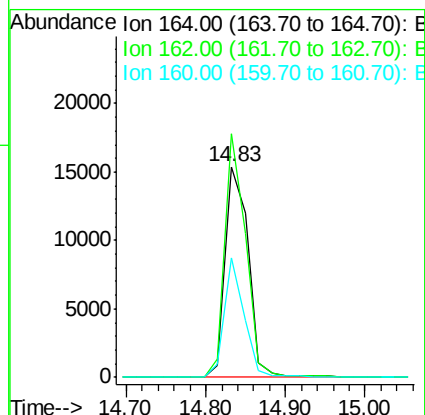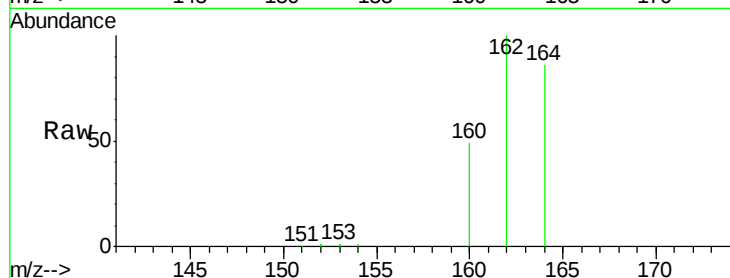

#11

2,4,6-Tribromophenol

Concen: 15.68 ng

RT: 16.33 min Scan# 1107

Delta R.T. 0.00 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39




Tgt Ion:330 Resp: 15380


Ion Ratio Lower Upper

330 100

332 96.2 74.2 111.4

141 43.8 139.8 209.8#

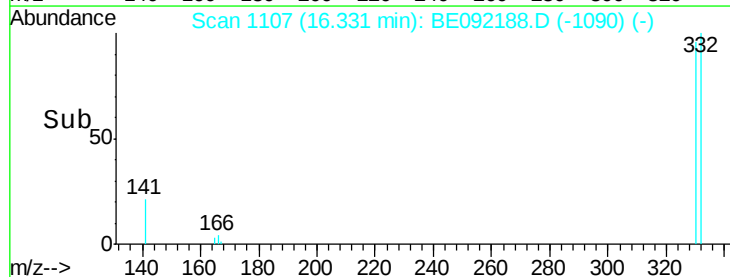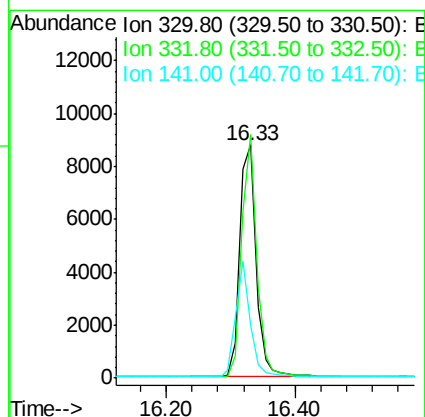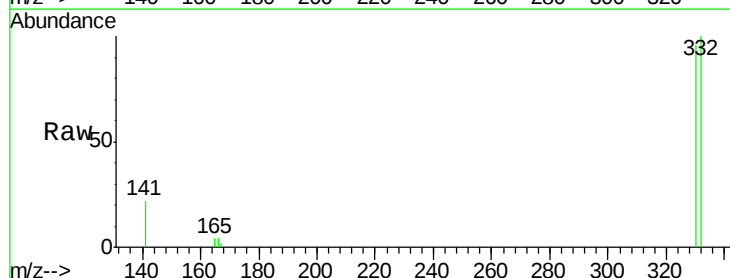

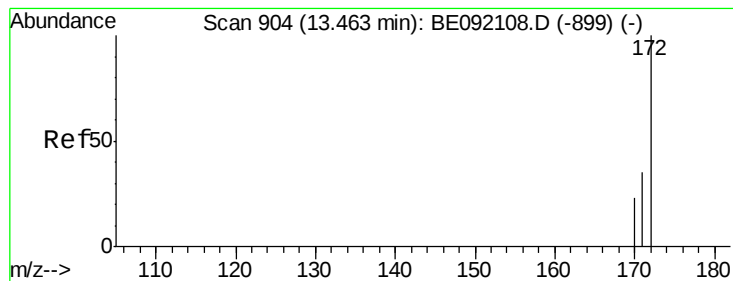

#12

2-Fluorobiphenyl

Concen: 6.51 ng

RT: 13.46 min Scan# 904

Delta R.T. -0.00 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39

Instrument :

BNA_E

ClientSampleId :

GW-42-6.1-15.0





Tgt Ion:172 Resp: 62337

Ion Ratio Lower Upper

172 100

171 31.4 30.3 45.5

170 19.5 21.6 32.4#

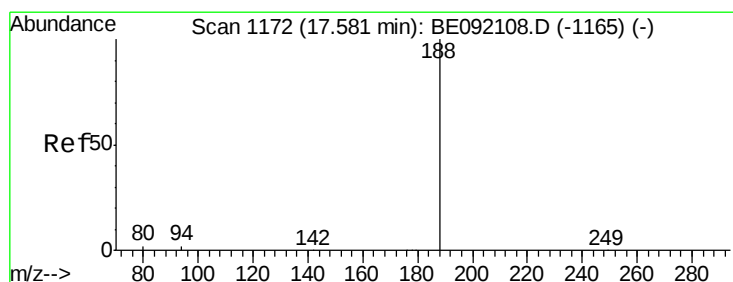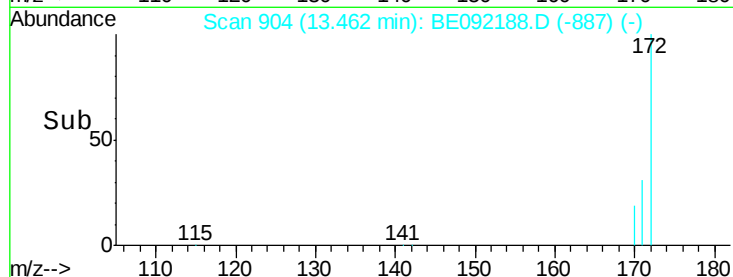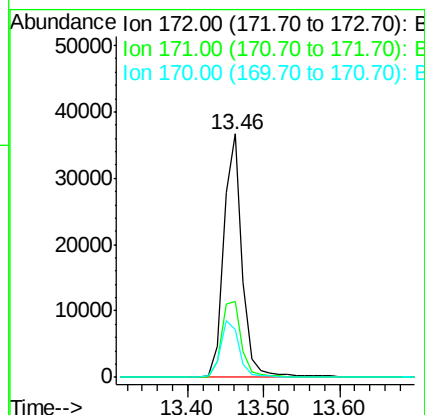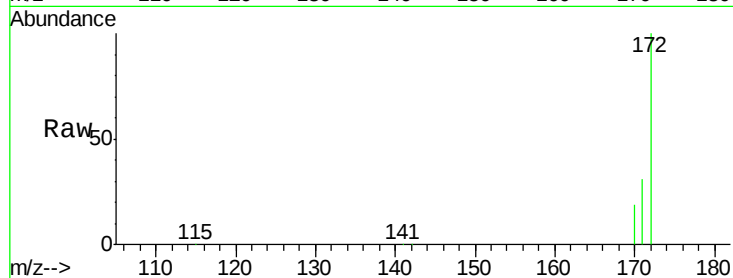

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1171

Delta R.T. -0.02 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39




Tgt Ion:188 Resp: 64296


Ion Ratio Lower Upper

188 100

94 15.5 3.9 5.9#

80 16.5 3.4 5.0#

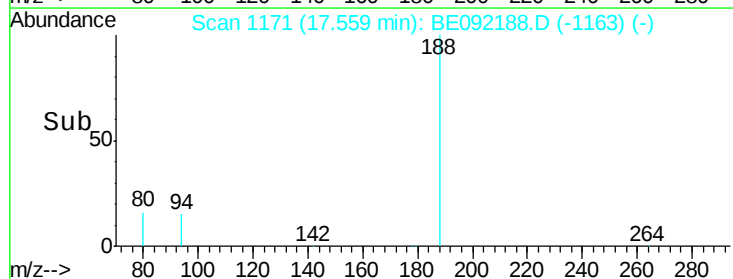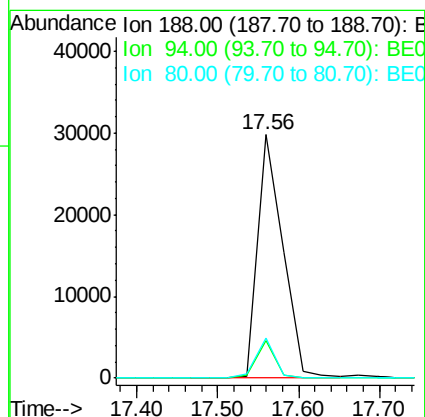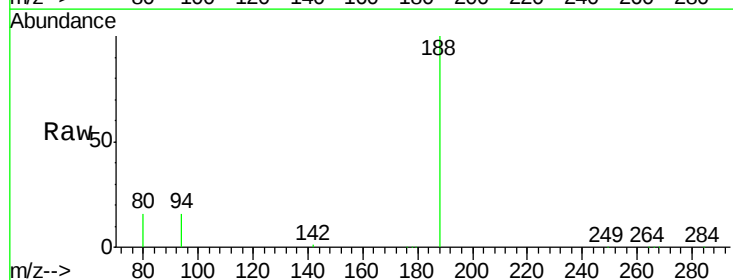

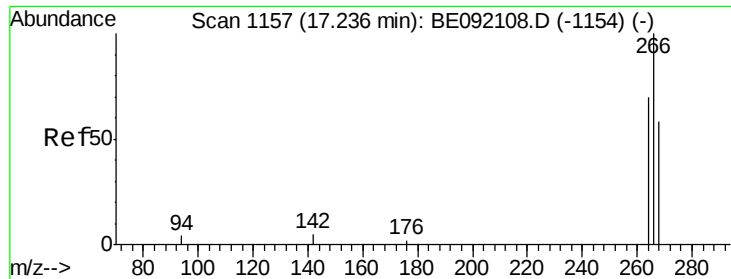

#18

Pentachlorophenol

Concen: 0.20 ng

RT: 17.24 min Scan# 1157

Delta R.T. 0.00 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39


Instrument :

BNA_E




ClientSampleId :

GW-42-6.1-15.0

Tgt Ion:	266	Resp:	3
Ion	Ratio	Lower	Upper
266	100		
268	102.2	62.7	94.1#
264	97.8	63.5	95.3#



Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

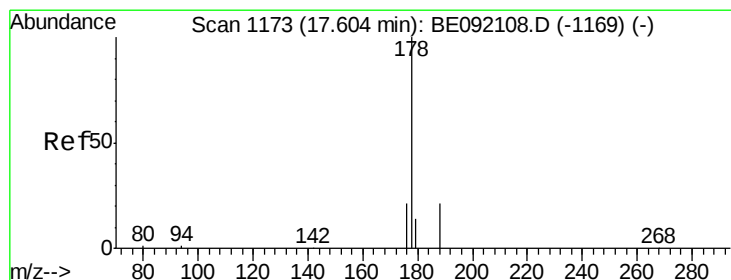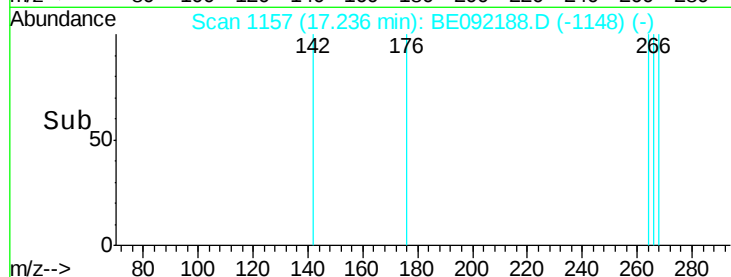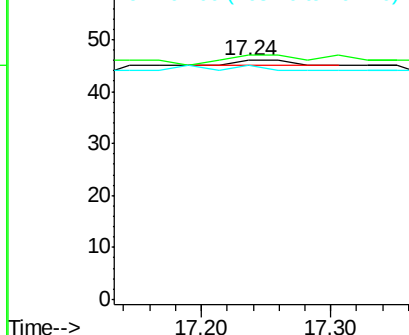

#19

Phenanthrene

Concen: Below Cal


RT: 17.60 min Scan# 1173

Delta R.T. 0.00 min



Lab File: BE092188.D


Acq: 4 Aug 2016 18:39

Tgt Ion:	178	Resp:	189
Ion	Ratio	Lower	Upper
178	100		
176	21.7	15.4	23.0
179	0.0	12.7	19.1#



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E



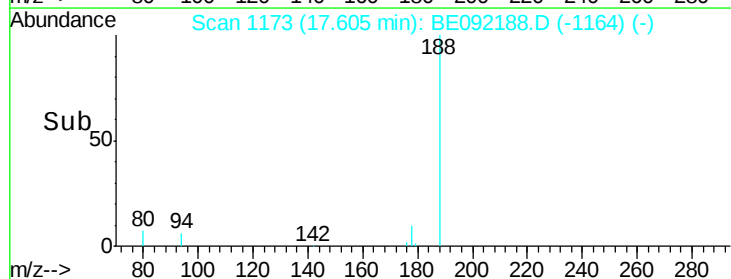
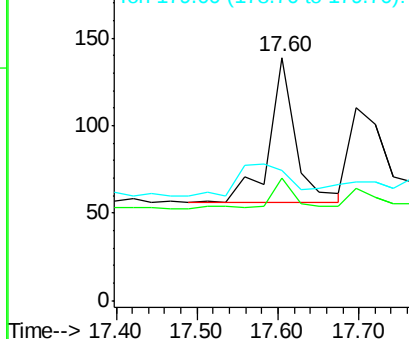


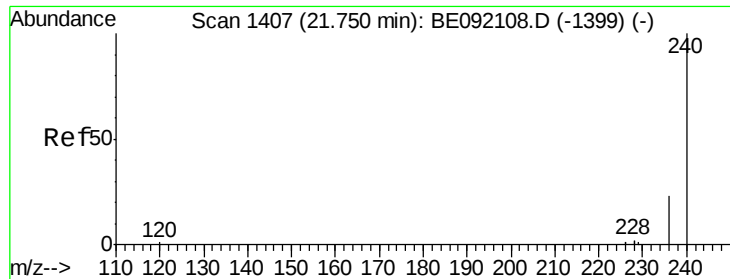

#22
Chrysene-d12
Concen: 5.00 ng
RT: 21.75 min Scan# 1407
Delta R.T. 0.00 min
Lab File: BE092188.D
Acq: 4 Aug 2016 18:39




Instrument :
BNA_E
ClientSampleId :
GW-42-6.1-15.0


Tgt Ion:240 Resp: 79263
Ion Ratio Lower Upper
240 100
120 1.3 0.6 1.0#
236 22.4 18.2 27.4

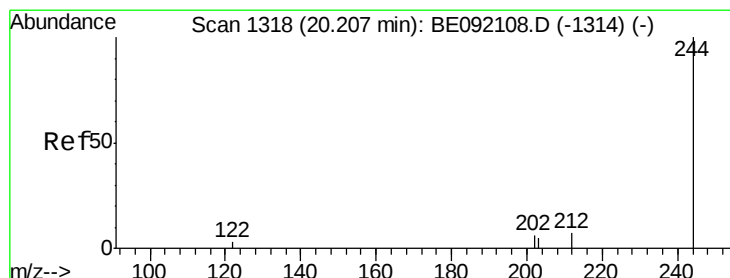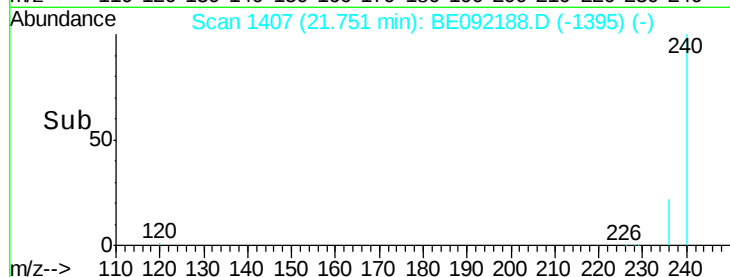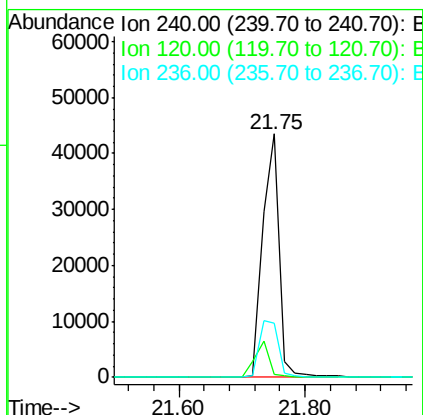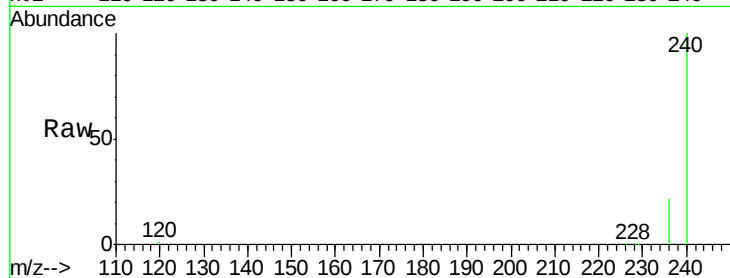

#24
Terphenyl-d14
Concen: 7.34 ng
RT: 20.19 min Scan# 1317
Delta R.T. -0.02 min
Lab File: BE092188.D
Acq: 4 Aug 2016 18:39

Tgt Ion:244 Resp: 83600
Ion Ratio Lower Upper
244 100
212 8.8 9.1 13.7#
122 6.6 11.0 16.4#


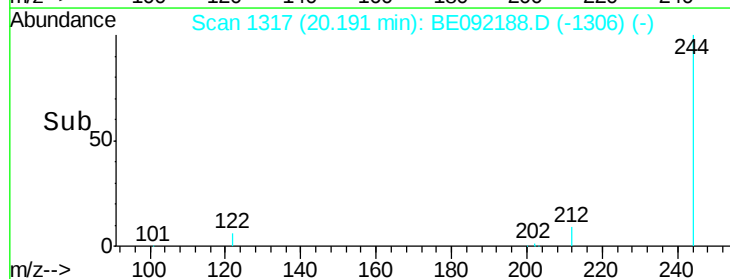
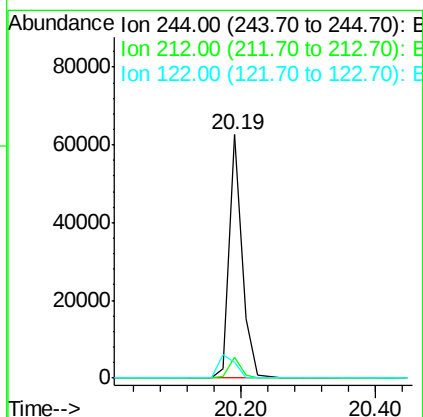
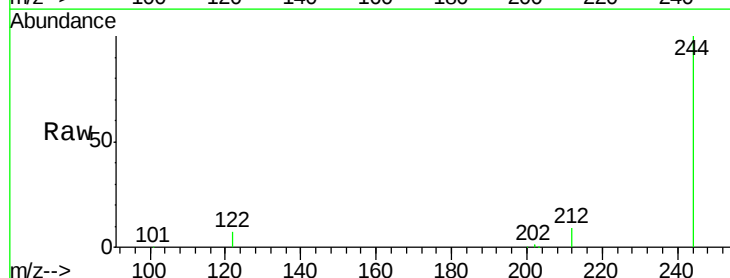


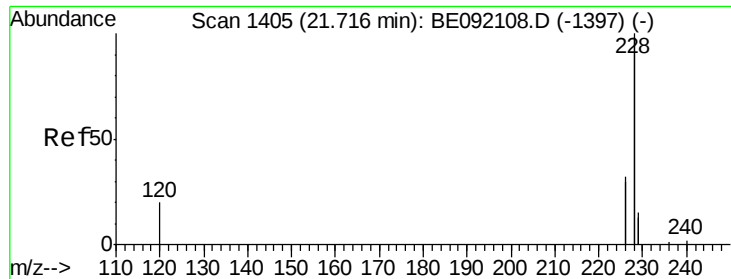

#25
Benzo(a)anthracene
Concen: 0.02 ng
RT: 21.73 min Scan# 1406
Delta R.T. 0.02 min
Lab File: BE092188.D
Acq: 4 Aug 2016 18:39




Instrument :
BNA_E
ClientSampleId :
GW-42-6.1-15.0




Tgt Ion:228 Resp: 1949
Ion Ratio Lower Upper
228 100
226 31.0 22.1 33.1
229 46.2 15.1 22.7#

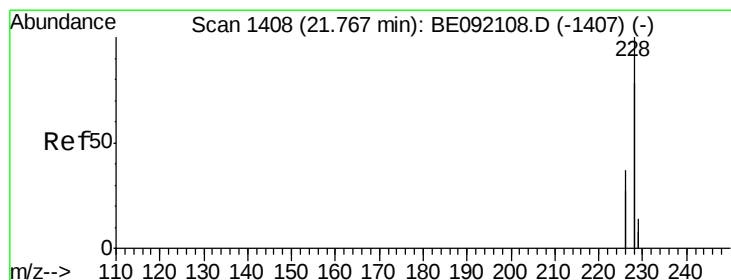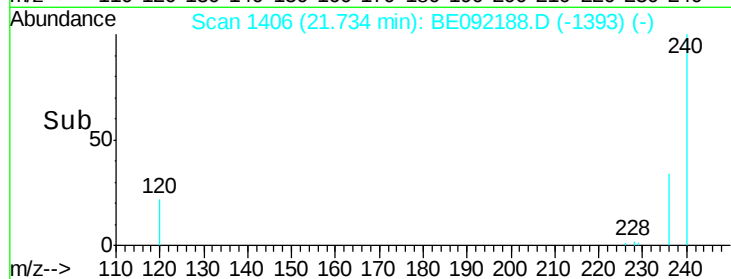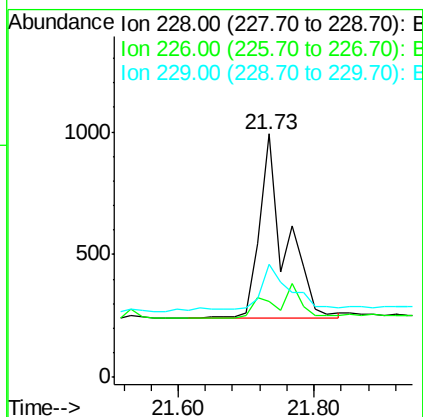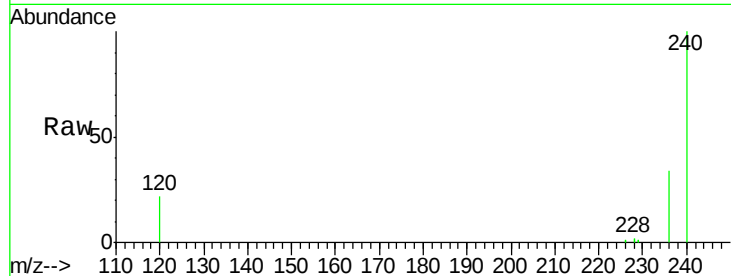

#26
Chrysene
Concen: 0.02 ng
RT: 21.73 min Scan# 1406
Delta R.T. -0.03 min
Lab File: BE092188.D
Acq: 4 Aug 2016 18:39

Tgt Ion:228 Resp: 1949
Ion Ratio Lower Upper
228 100
226 31.0 22.3 33.5
229 46.2 16.9 25.3#

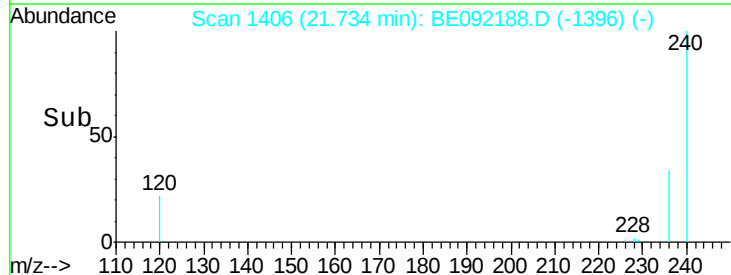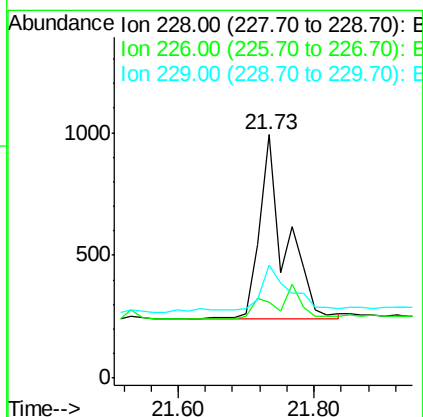

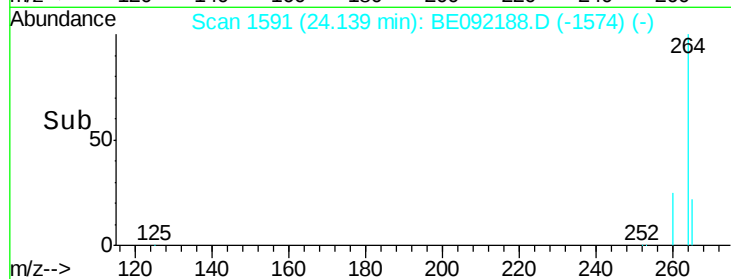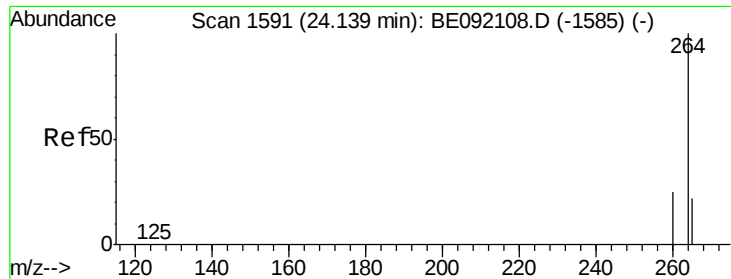

#28

Perylene-d12

Concen: 5.00 ng

RT: 24.14 min Scan# 1591

Delta R.T. 0.00 min

Lab File: BE092188.D

Acq: 4 Aug 2016 18:39

Instrument :

BNA_E

ClientSampleId :

GW-42-6.1-15.0

Tgt Ion: 264 Resp: 85190

Ion Ratio Lower Upper

264 100

260 24.7 20.8 31.2

265 22.5 16.6 25.0

