

Data Path : Z:\HPCHEM1\BNA E\Data\BE080416\
 Data File : BE092190.D
 Acq On : 4 Aug 2016 19:57
 Operator : UM/SJ
 Sample : H4227-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS037-160725

Quant Time: Aug 05 03:36:31 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 16:59:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	12477	5.00	ng	0.00
6) Naphthalene-d8	10.98	136	58050	5.00	ng	-0.01
10) Acenaphthene-d10	14.83	164	32995	5.00	ng	-0.02
16) Phenanthrene-d10	17.56	188	78687	5.00	ng	-0.02
22) Chrysene-d12	21.75	240	92403	5.00	ng	0.00
28) Perylene-d12	24.14	264	91764	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.69	112	5589	1.74	ng	0.00
5) Phenol-d6	7.35	99	6286	1.47	ng	0.00
7) Nitrobenzene-d5	9.35	82	10663	2.33	ng	0.00
11) 2,4,6-Tribromophenol	16.33	330	5027	4.69	ng	0.00
12) 2-Fluorobiphenyl	13.46	172	27819	2.66	ng	0.00
24) Terphenyl-d14	20.19	244	53565	4.04	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\BE080416\
Data File : BE092190.D
Acq On : 4 Aug 2016 19:57
Operator : UM/SJ
Sample : H4227-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
KY038PS037-160725

Quant Time: Aug 05 03:36:31 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 16:59:37 2016
Response via : Initial Calibration

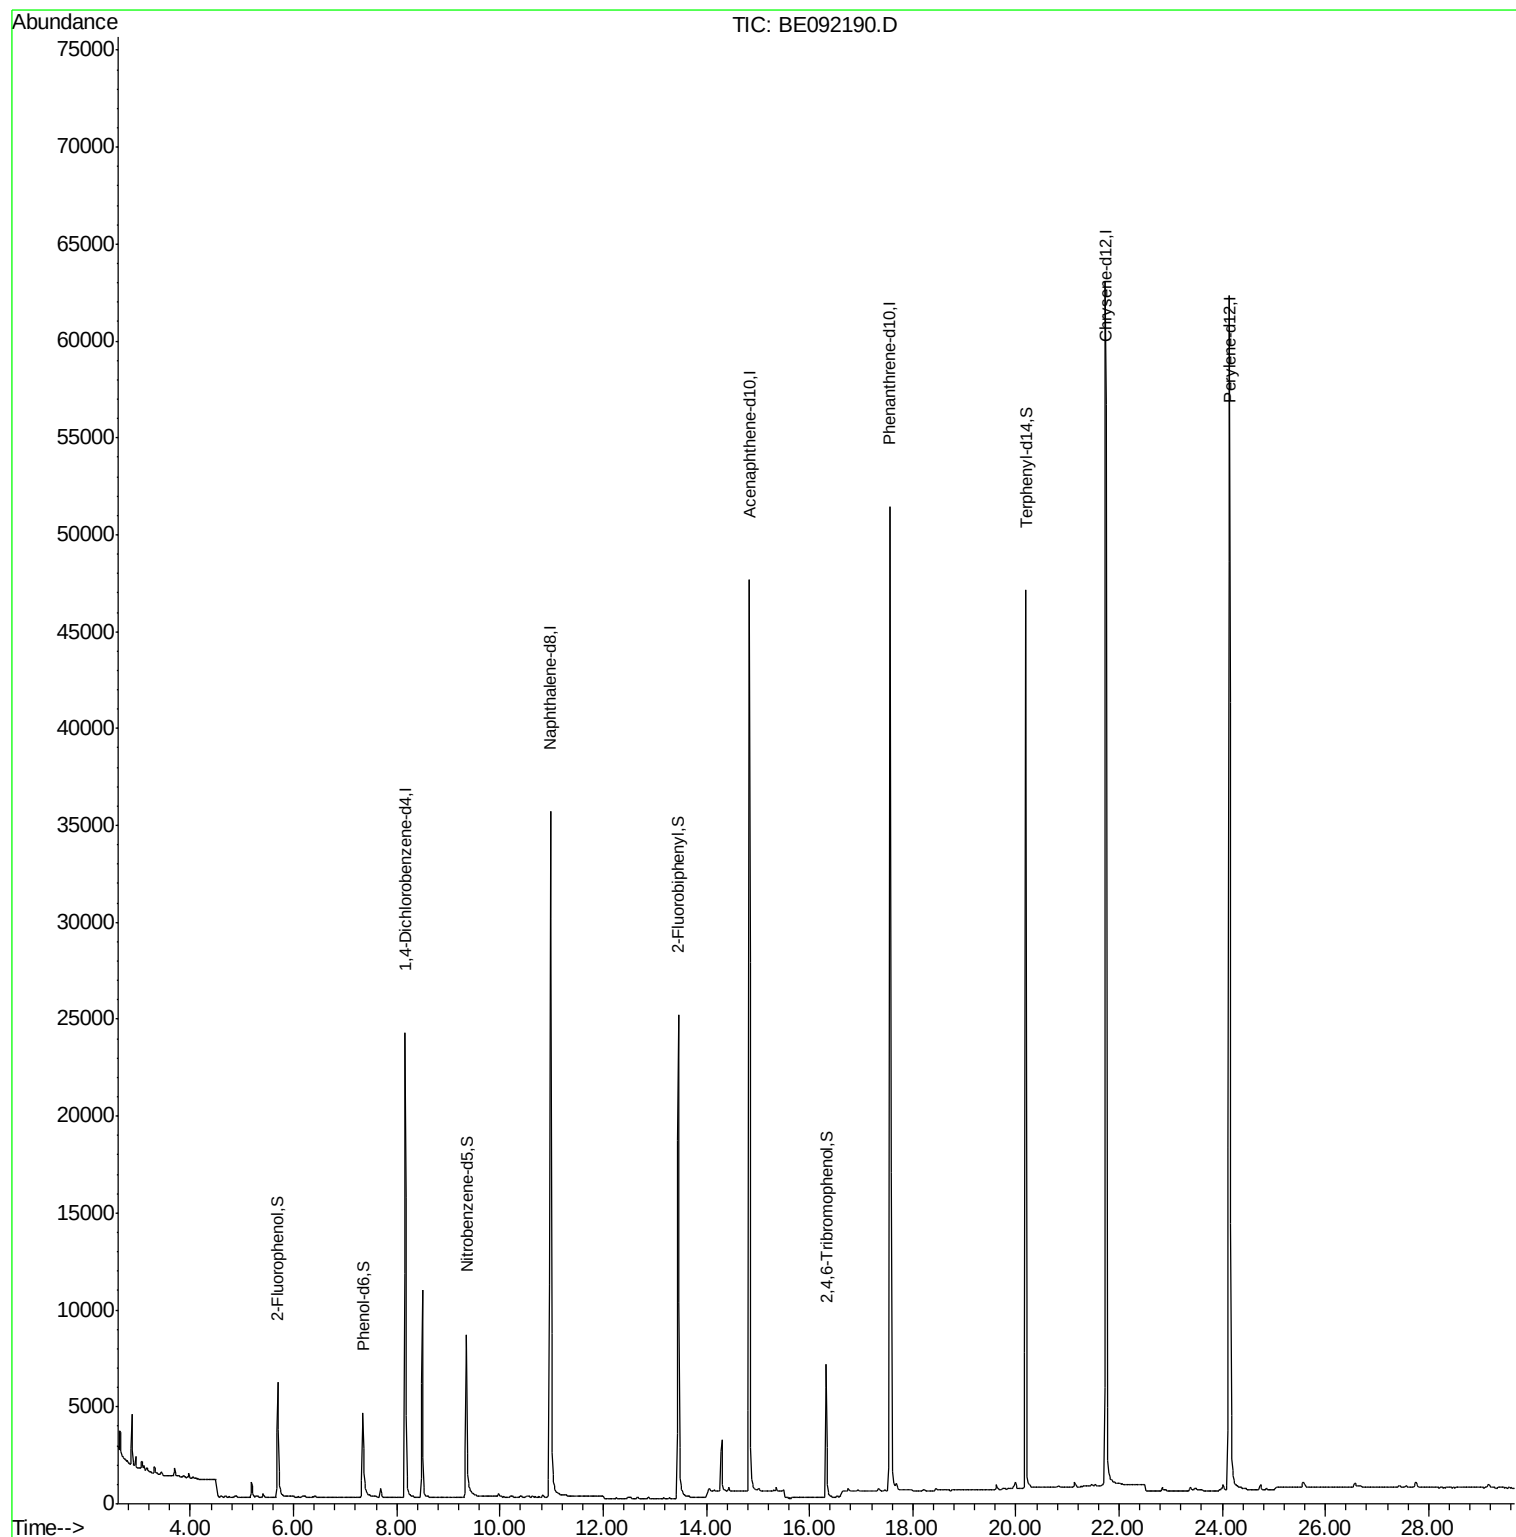



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.17 min Scan# 479

Delta R.T. -0.00 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57

Instrument :

BNA_E

ClientSampleId :

KY038PS037-160725


Tot Ion:152 Resp: 12477

Ion Ratio Lower Upper




152 100

150 163.7 106.0 159.0#

115 65.8 36.9 55.3#

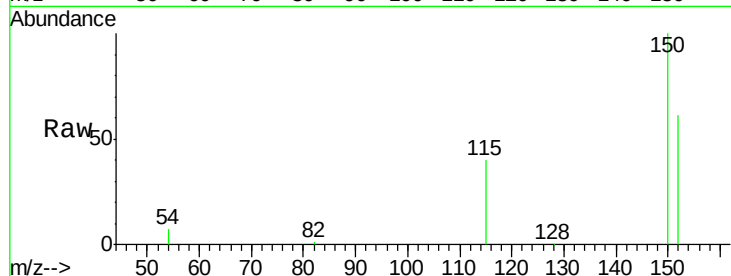

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

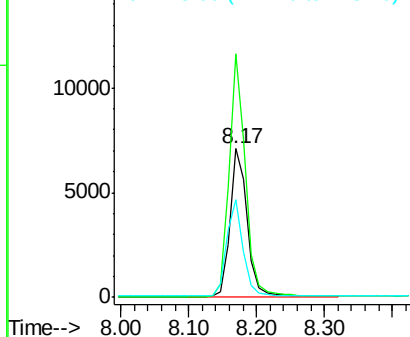

#4

2-Fluorophenol

Concen: 1.74 ng

RT: 5.69 min Scan# 267

Delta R.T. 0.00 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57


Tgt Ion:112 Resp: 5589

Ion Ratio Lower Upper



112 100


64 66.4 55.9 83.9

63 36.3 31.1 46.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

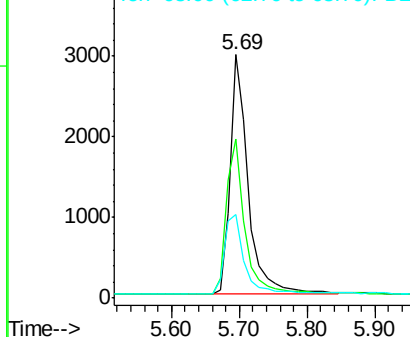

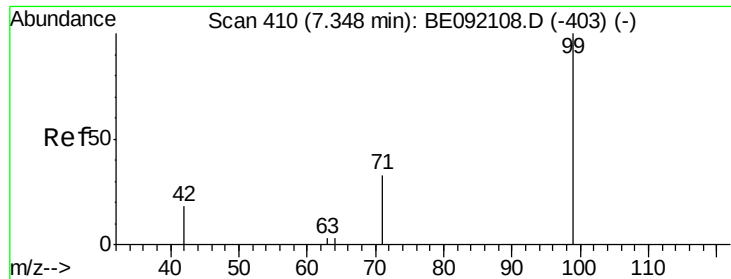

#5

Phenol-d6

Concen: 1.47 ng

RT: 7.35 min Scan# 410

Delta R.T. 0.00 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57

Instrument :

BNA_E

ClientSampleId :

KY038PS037-160725


Tot Ion: 99 Resp: 6286

Ion Ratio Lower Upper

99 100

42 25.3 22.4 33.6




71 36.6 28.9 43.3



Abundance Ion 99.00 (98.70 to 99.70): BE092108.D (-403) (-)

Ion 42.00 (41.70 to 42.70): BE092108.D (-403) (-)

Ion 71.00 (70.70 to 71.70): BE092108.D (-403) (-)

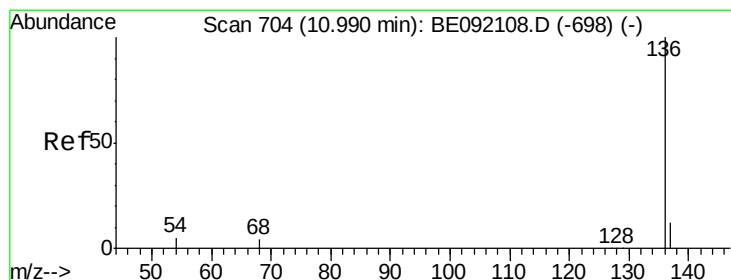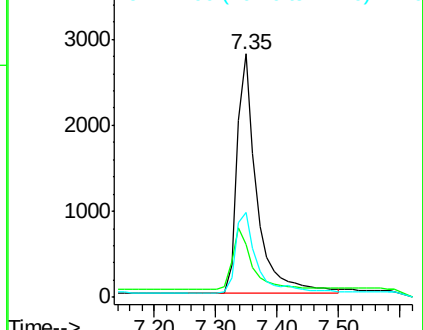

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.98 min Scan# 703

Delta R.T. -0.01 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57

Tgt Ion: 136 Resp: 58050


Ion Ratio Lower Upper

136 100

137 10.3 9.1 13.7

54 11.1 2.7 4.1#

68 7.6 2.2 3.4#






Abundance Ion 136.00 (135.70 to 136.70): BE092108.D (-698) (-)

Ion 137.00 (136.70 to 137.70): BE092108.D (-698) (-)

Ion 54.00 (53.70 to 54.70): BE092108.D (-698) (-)

Ion 68.00 (67.70 to 68.70): BE092108.D (-698) (-)

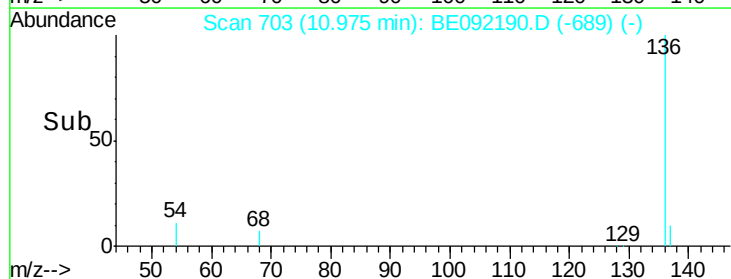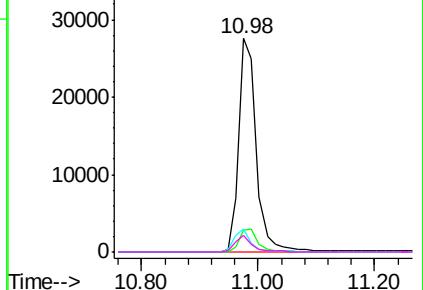

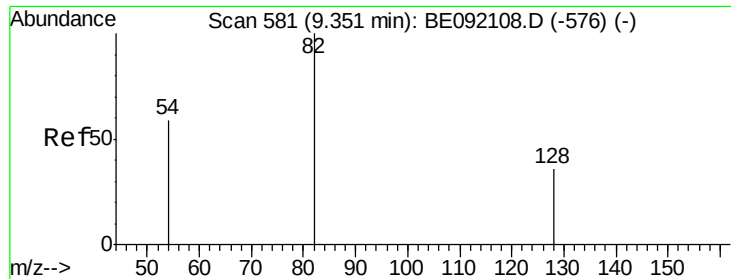

#7

Nitrobenzene-d5

Concen: 2.33 ng

RT: 9.35 min Scan# 581

Delta R.T. -0.00 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57

Instrument :

BNA_E

ClientSampleId :

KY038PS037-160725





Tot Ion: 82 Resp: 10663

Ion Ratio Lower Upper

82 100

128 40.7 33.0 49.4

54 57.6 42.6 63.8

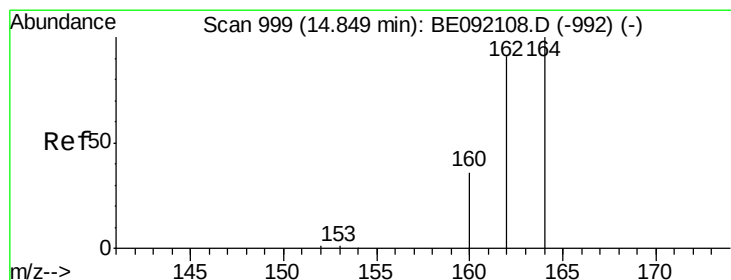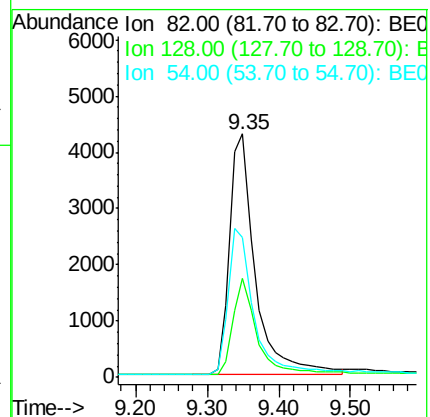

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.83 min Scan# 998

Delta R.T. -0.02 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57




Tgt Ion: 164 Resp: 32995


Ion Ratio Lower Upper

164 100

162 115.2 69.5 104.3#

160 57.2 27.6 41.4#



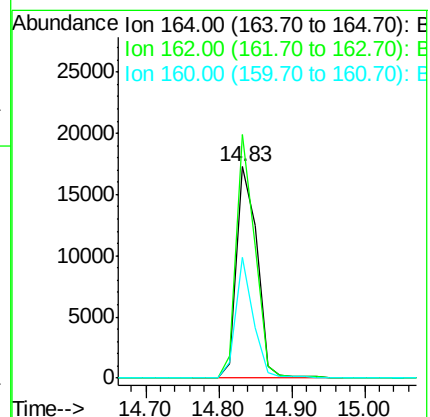



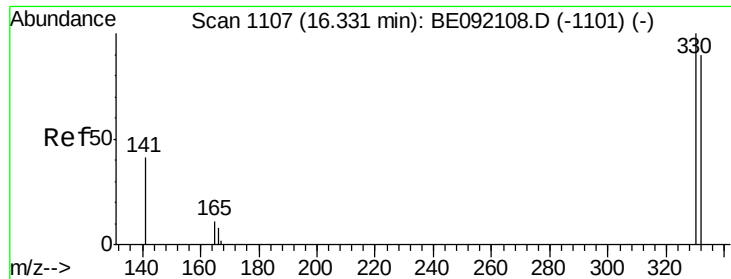

#11
 2,4,6-Tribromophenol
 Concen: 4.69 ng
 RT: 16.33 min Scan# 1107
 Delta R.T. 0.00 min
 Lab File: BE092190.D
 Acq: 4 Aug 2016 19:57




Instrument :
 BNA_E
 ClientSampleId :
 KY038PS037-160725


Tot Ion:330 Resp: 5027
 Ion Ratio Lower Upper
 330 100
 332 96.3 74.2 111.4
 141 43.8 139.8 209.8#

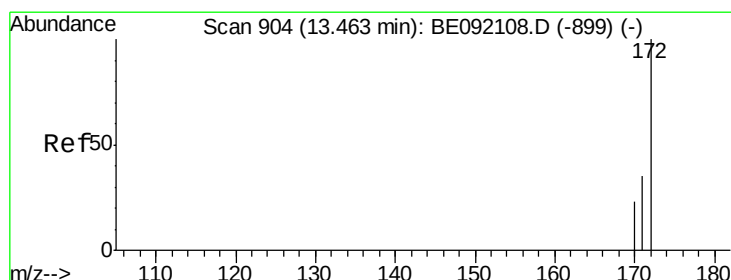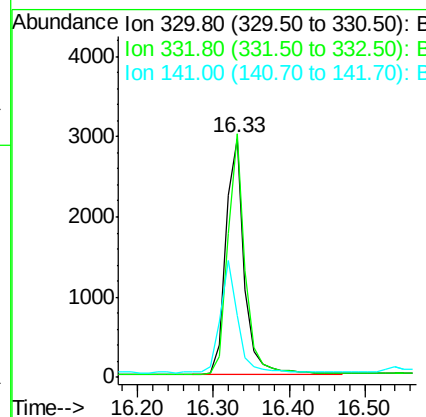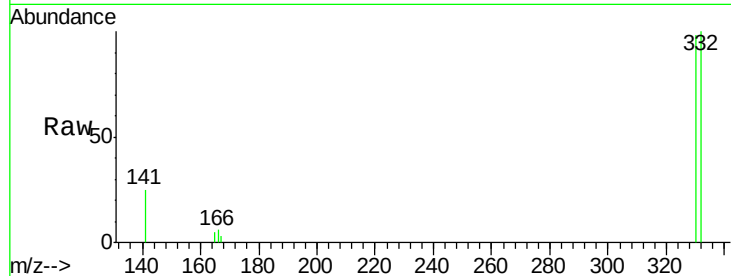

#12
 2-Fluorobiphenyl
 Concen: 2.66 ng
 RT: 13.46 min Scan# 904
 Delta R.T. -0.00 min
 Lab File: BE092190.D
 Acq: 4 Aug 2016 19:57

Tgt Ion:172 Resp: 27819
 Ion Ratio Lower Upper
 172 100
 171 31.9 30.3 45.5
 170 19.9 21.6 32.4#

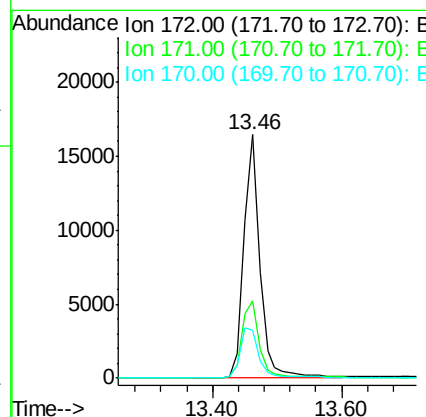

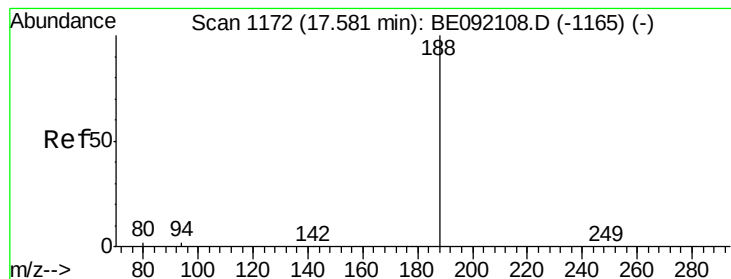

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1171

Delta R.T. -0.02 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57

Instrument :

BNA_E

ClientSampleId :

KY038PS037-160725


Tot Ion:188 Resp: 78687

Ion Ratio Lower Upper

188 100

94 13.7 3.9 5.9#




80 14.1 3.4 5.0#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

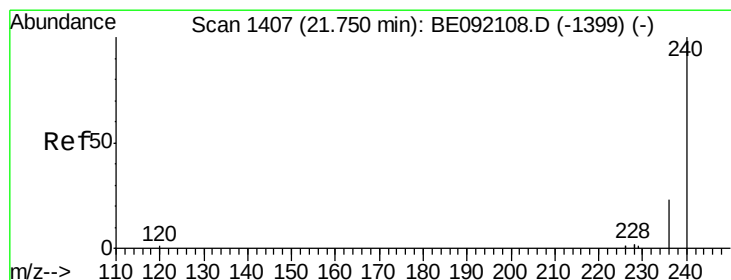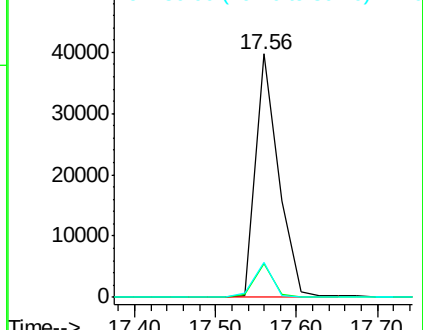

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1407

Delta R.T. 0.00 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57


Tgt Ion:240 Resp: 92403

Ion Ratio Lower Upper

240 100

120 1.3 0.6 1.0#



236 22.2 18.2 27.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

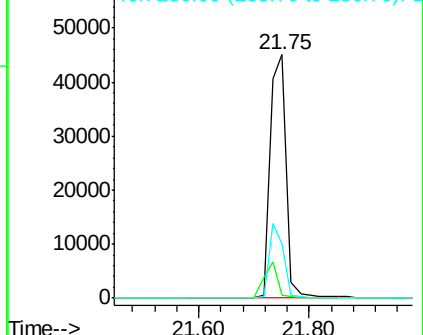

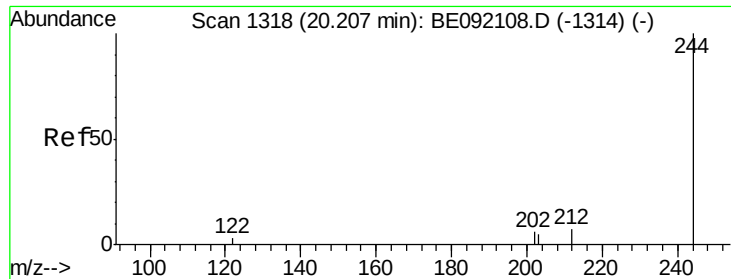

#24

Terphenyl-d14

Concen: 4.04 ng

RT: 20.19 min Scan# 1317

Delta R.T. -0.02 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57

Instrument :

BNA_E

ClientSampleId :

KY038PS037-160725


Tot Ion:244 Resp: 53565

Ion Ratio Lower Upper

244 100

212 8.7 9.1 13.7#




122 6.3 11.0 16.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

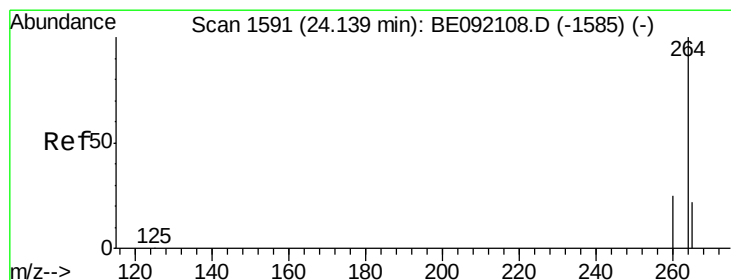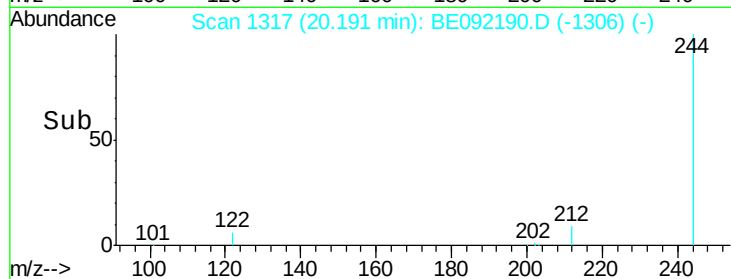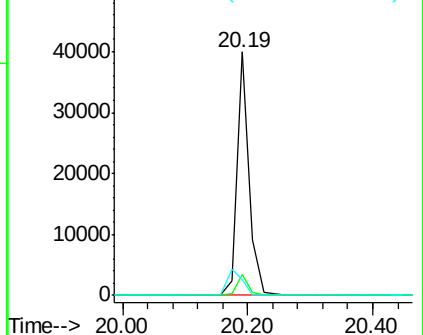

#28

Perylene-d12

Concen: 5.00 ng

RT: 24.14 min Scan# 1591

Delta R.T. 0.00 min

Lab File: BE092190.D

Acq: 4 Aug 2016 19:57


Tgt Ion:264 Resp: 91764

Ion Ratio Lower Upper

264 100

260 24.9 20.8 31.2

265 22.0 16.6 25.0

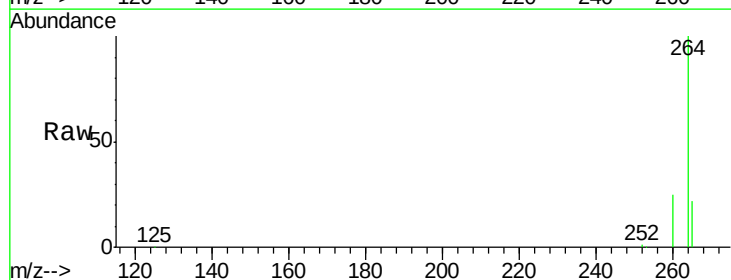

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

