

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080416\
 Data File : BE092197.D
 Acq On : 5 Aug 2016 00:19
 Operator : UM/SJ
 Sample : H4269-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 GW-56-15.0-19.5

Quant Time: Aug 05 04:02:02 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 16:59:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	11880	5.00	ng	0.00
6) Naphthalene-d8	10.98	136	54814	5.00	ng	-0.01
10) Acenaphthene-d10	14.83	164	30112	5.00	ng	-0.02
16) Phenanthrene-d10	17.56	188	68902	5.00	ng	-0.02
22) Chrysene-d12	21.75	240	90922	5.00	ng	0.00
28) Perylene-d12	24.14	264	90149	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.69	112	12642	4.14	ng	0.00
5) Phenol-d6	7.35	99	10929	2.69	ng	0.00
7) Nitrobenzene-d5	9.34	82	14005	3.24	ng	-0.01
11) 2,4,6-Tribromophenol	16.33	330	8226	8.41	ng	0.00
12) 2-Fluorobiphenyl	13.46	172	32055	3.36	ng	0.00
24) Terphenyl-d14	20.19	244	50793	3.89	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080416\
Data File : BE092197.D
Acq On : 5 Aug 2016 00:19
Operator : UM/SJ
Sample : H4269-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
GW-56-15.0-19.5

Quant Time: Aug 05 04:02:02 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 16:59:37 2016
Response via : Initial Calibration

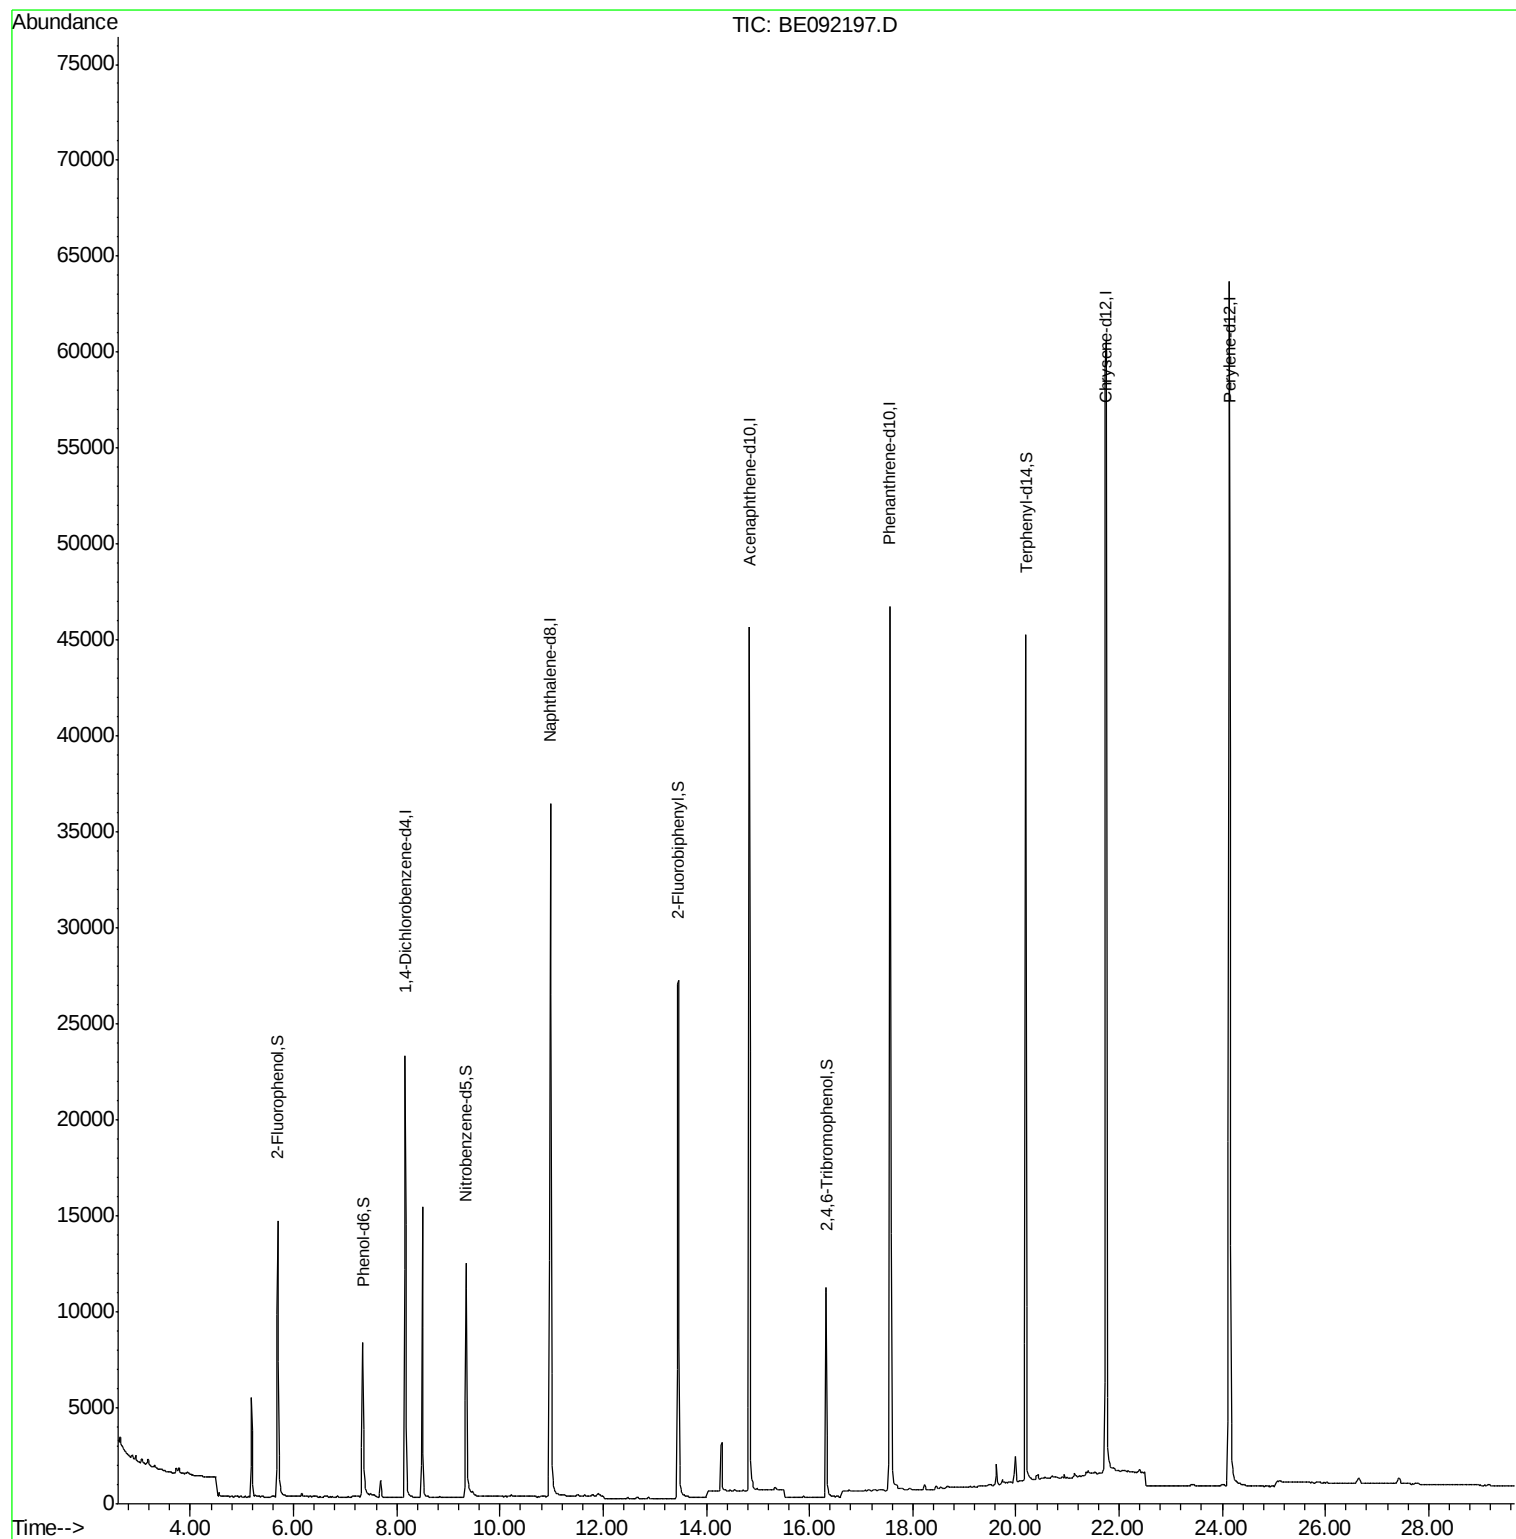


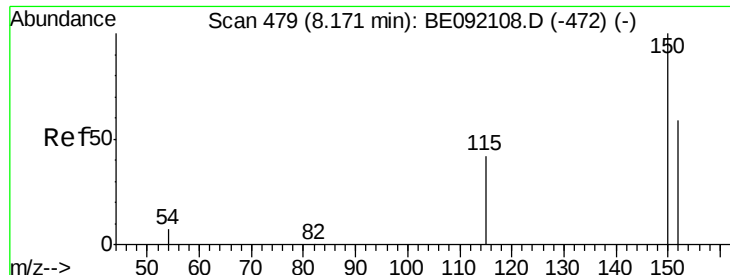




#1
 1,4-Dichlorobenzene-d4
 Concen: 5.00 ng
 RT: 8.17 min Scan# 479
 Delta R.T. -0.00 min
 Lab File: BE092197.D
 Acq: 5 Aug 2016 00:19

Instrument :
 BNA_E
 ClientSampleId :
 GW-56-15.0-19.5

Tot Ion:152 Resp: 11880
 Ion Ratio Lower Upper
 152 100
 150 161.2 106.0 159.0#
 115 63.3 36.9 55.3#

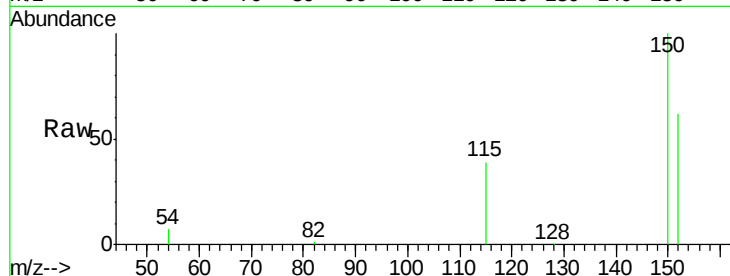


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

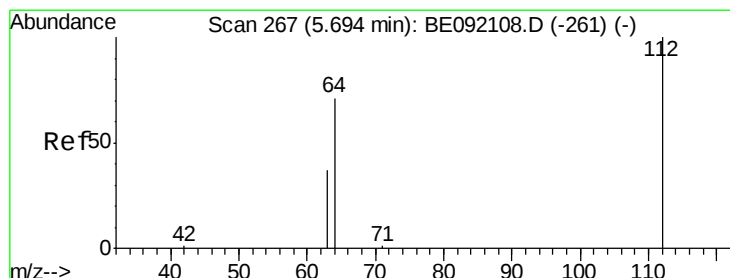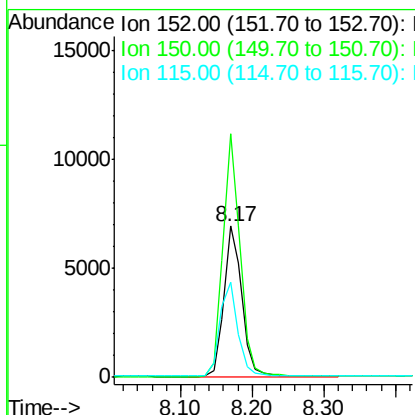
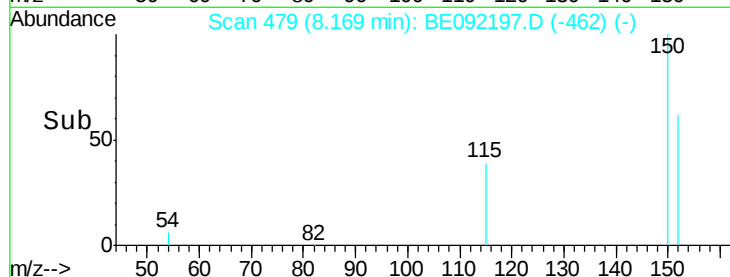



#4
 2-Fluorophenol
 Concen: 4.14 ng
 RT: 5.69 min Scan# 267
 Delta R.T. 0.00 min
 Lab File: BE092197.D
 Acq: 5 Aug 2016 00:19

Tgt Ion:112 Resp: 12642
 Ion Ratio Lower Upper
 112 100
 64 67.0 55.9 83.9
 63 36.7 31.1 46.7

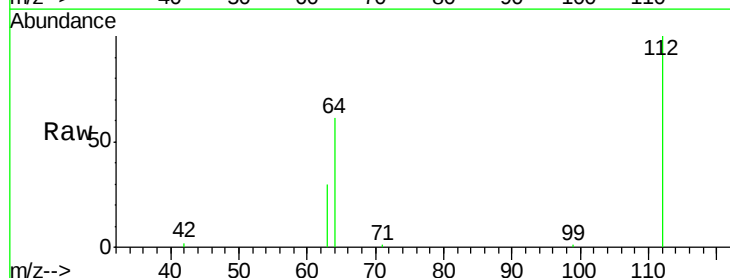

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

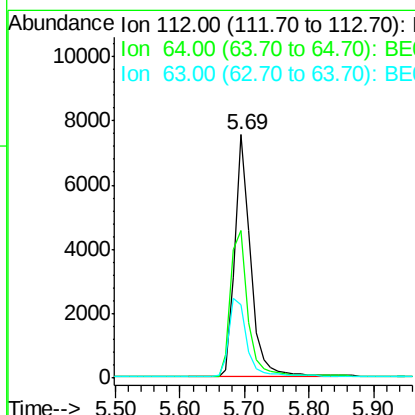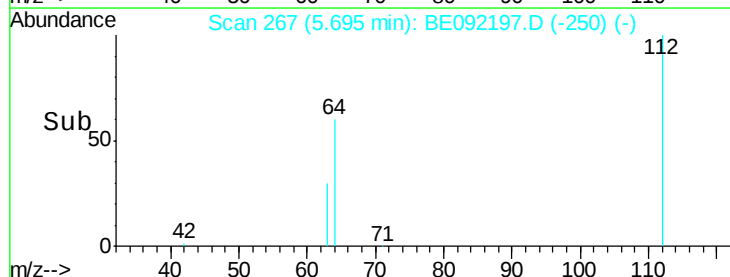

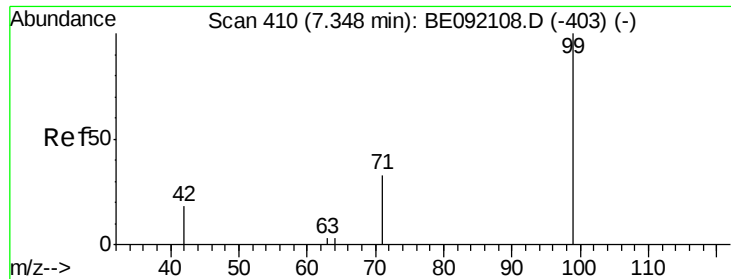

#5

Phenol-d6

Concen: 2.69 ng

RT: 7.35 min Scan# 410

Delta R.T. 0.00 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19

Instrument :

BNA_E

ClientSampleId :

GW-56-15.0-19.5


Tot Ion: 99 Resp: 10929

Ion Ratio Lower Upper




99 100

42 24.6 22.4 33.6

71 35.0 28.9 43.3

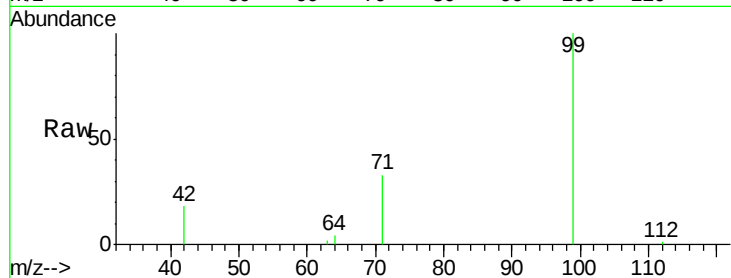

Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

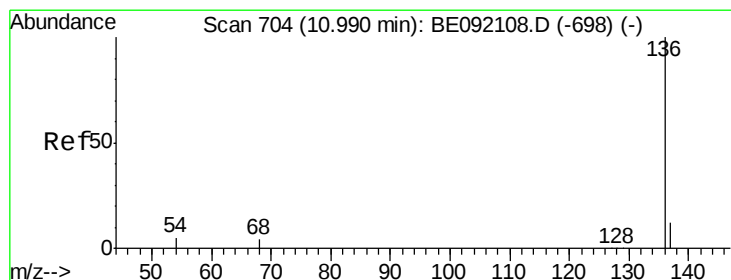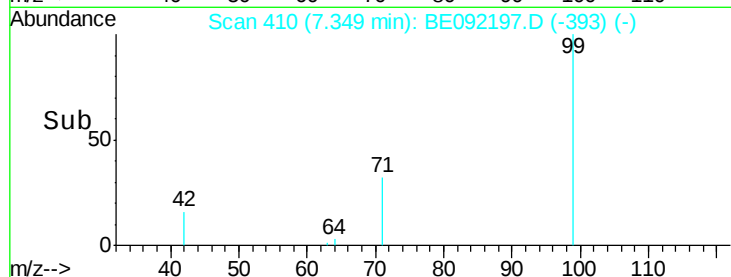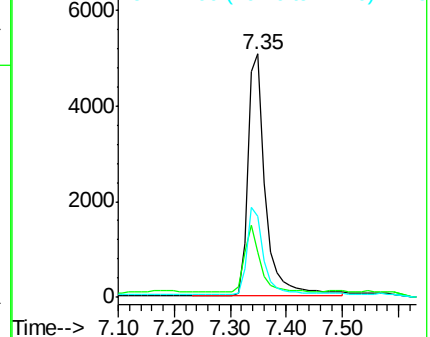

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.98 min Scan# 703

Delta R.T. -0.01 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19

Tgt Ion: 136 Resp: 54814


Ion Ratio Lower Upper

136 100



137 10.5 9.1 13.7


54 9.7 2.7 4.1#

68 6.9 2.2 3.4#

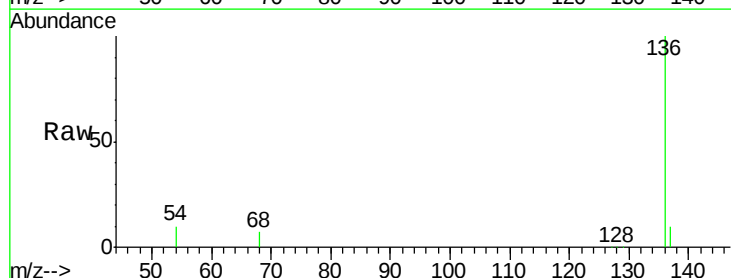

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

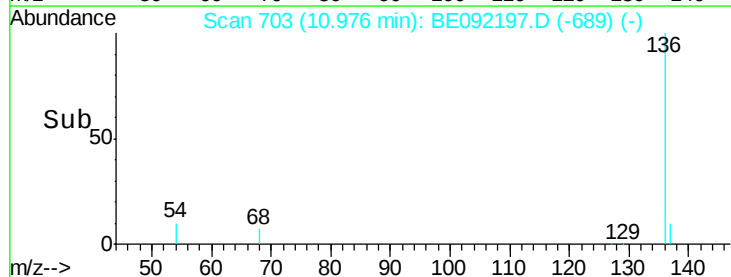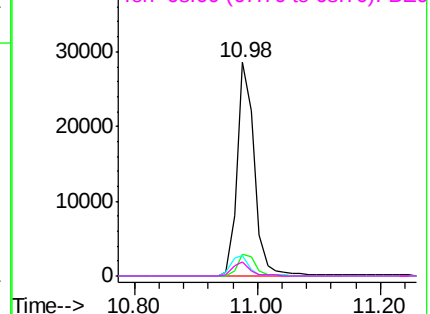

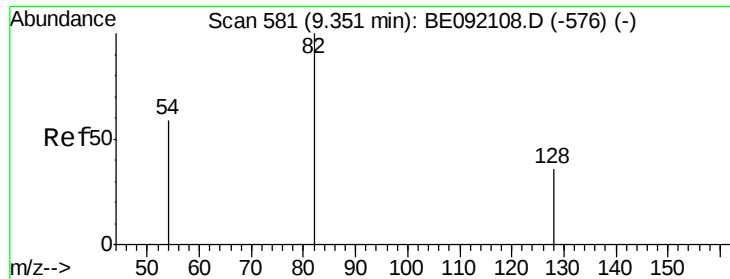

#7

Nitrobenzene-d5

Concen: 3.24 ng

RT: 9.34 min Scan# 580

Delta R.T. -0.01 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19

Instrument :

BNA_E

ClientSampleId :

GW-56-15.0-19.5


Tot Ion: 82 Resp: 14005

Ion Ratio Lower Upper

82 100

128 32.0 33.0 49.4#




54 62.9 42.6 63.8

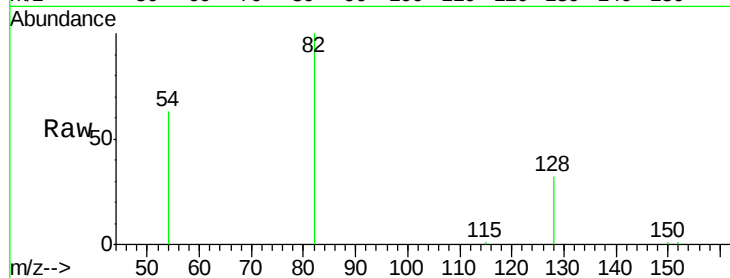

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

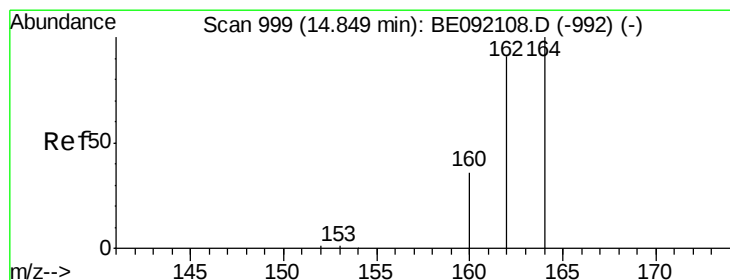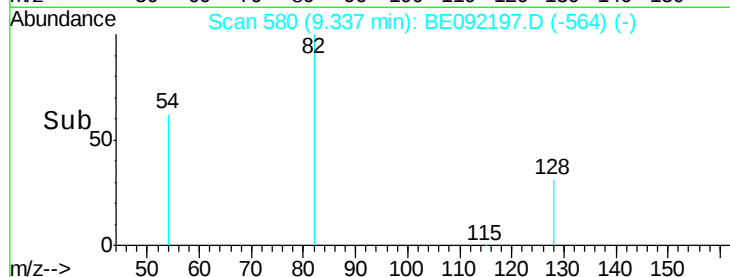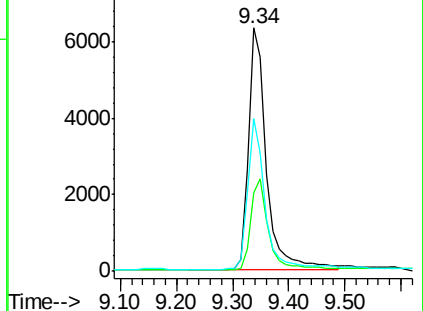

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.83 min Scan# 998

Delta R.T. -0.02 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19


Tgt Ion: 164 Resp: 30112

Ion Ratio Lower Upper

164 100

162 111.6 69.5 104.3#



160 53.9 27.6 41.4#

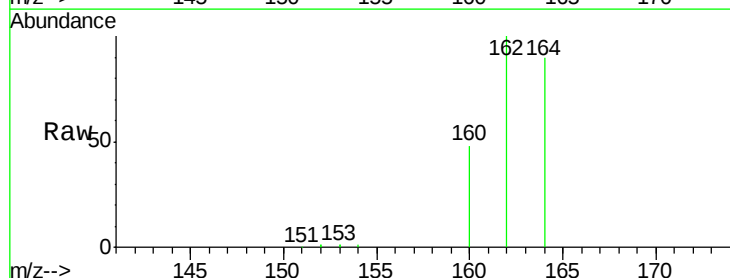


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



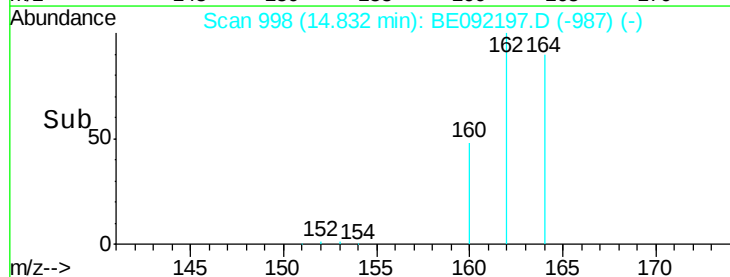
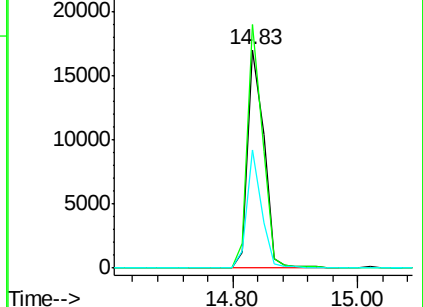


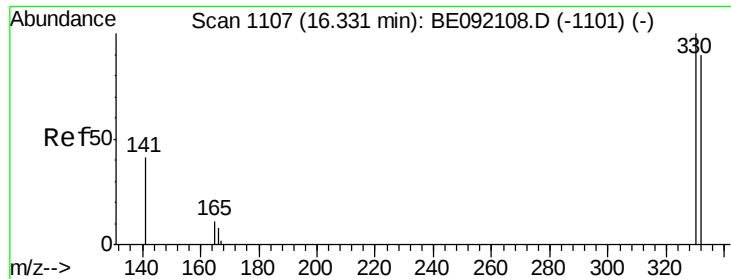

#11
 2,4,6-Tribromophenol
 Concen: 8.41 ng
 RT: 16.33 min Scan# 1107
 Delta R.T. 0.00 min
 Lab File: BE092197.D
 Acq: 5 Aug 2016 00:19




Instrument :
 BNA_E
 ClientSampleId :
 GW-56-15.0-19.5


Tot Ion:330 Resp: 8226
 Ion Ratio Lower Upper
 330 100
 332 96.8 74.2 111.4
 141 43.9 139.8 209.8#

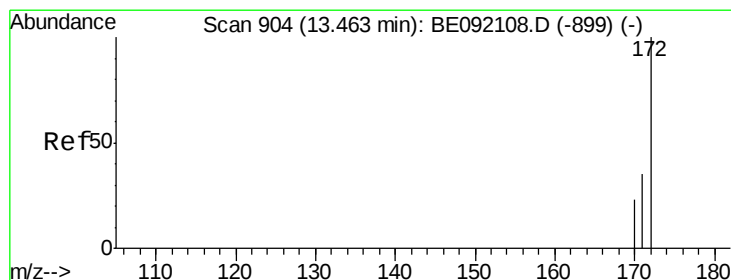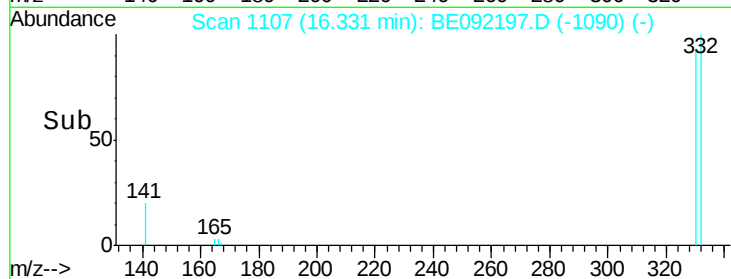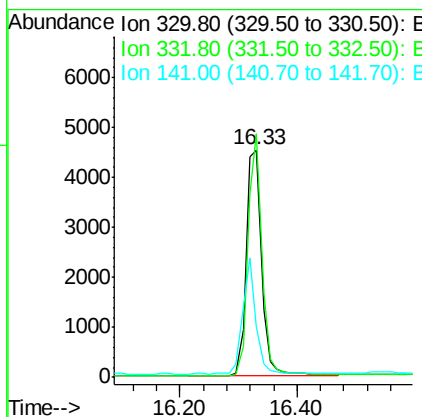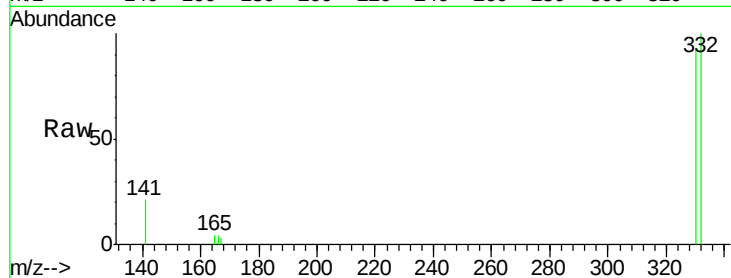

#12
 2-Fluorobiphenyl
 Concen: 3.36 ng
 RT: 13.46 min Scan# 904
 Delta R.T. -0.00 min
 Lab File: BE092197.D
 Acq: 5 Aug 2016 00:19

Tgt Ion:172 Resp: 32055
 Ion Ratio Lower Upper
 172 100
 171 30.8 30.3 45.5
 170 18.5 21.6 32.4#

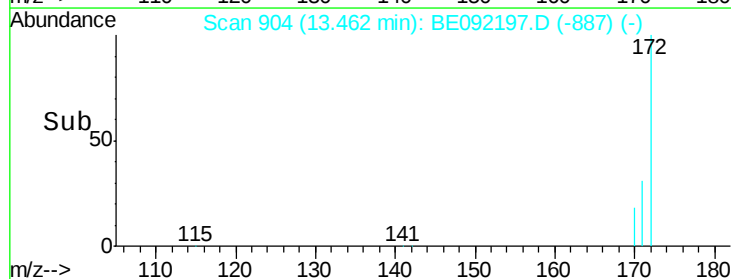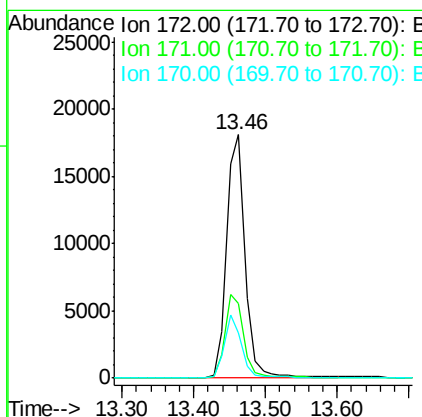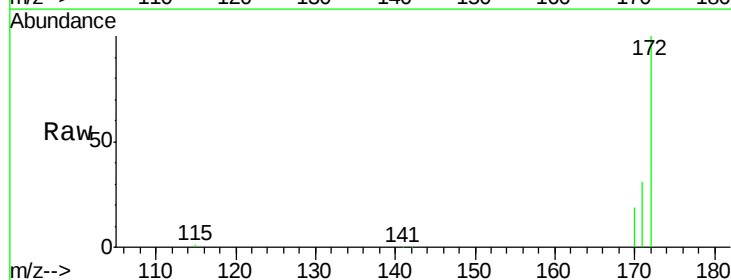

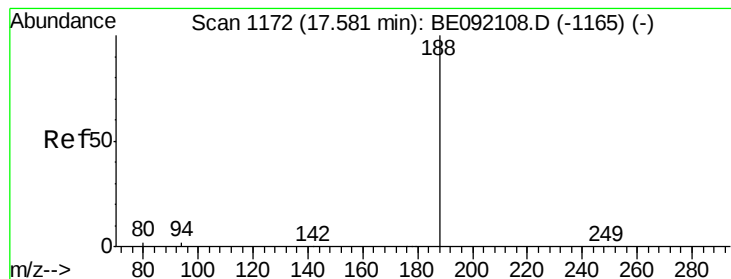

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1171

Delta R.T. -0.02 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19

Instrument :

BNA_E

ClientSampleId :

GW-56-15.0-19.5


Tot Ion:188 Resp: 68902

Ion Ratio Lower Upper

188 100

94 14.1 3.9 5.9#




80 14.3 3.4 5.0#

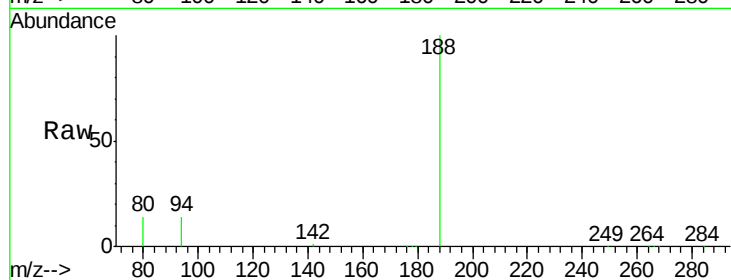

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

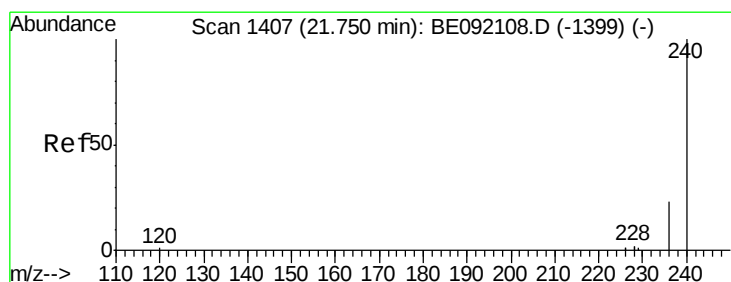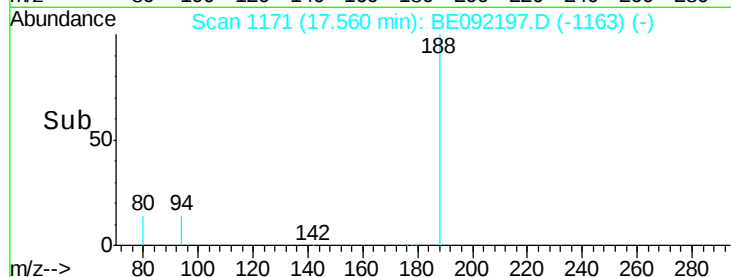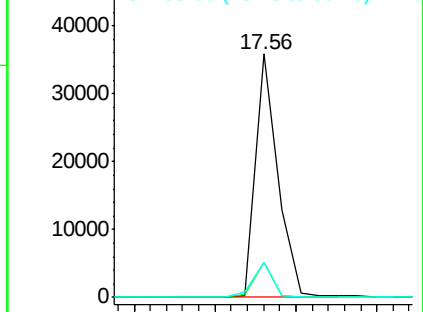

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1407

Delta R.T. 0.00 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19


Tgt Ion:240 Resp: 90922

Ion Ratio Lower Upper

240 100

120 1.2 0.6 1.0#



236 21.9 18.2 27.4

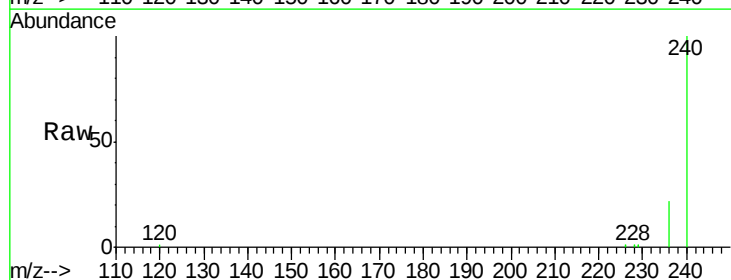


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

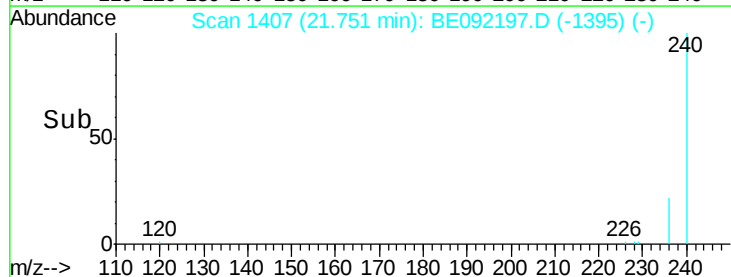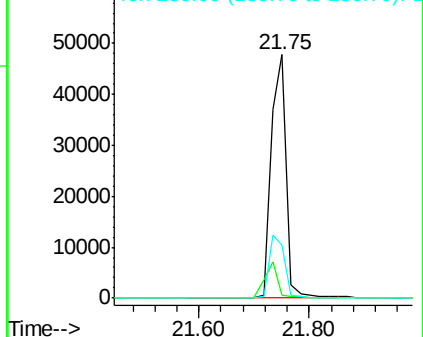

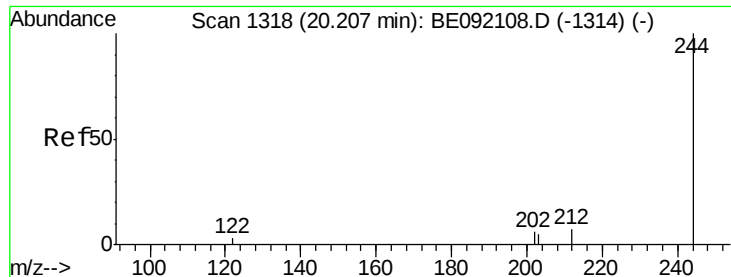

#24

Terphenyl-d14

Concen: 3.89 ng

RT: 20.19 min Scan# 1317

Delta R.T. -0.02 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19

Instrument :

BNA_E

ClientSampleId :

GW-56-15.0-19.5


Tot Ion:244 Resp: 50793

Ion Ratio Lower Upper

244 100

212 8.8 9.1 13.7#




122 6.7 11.0 16.4#

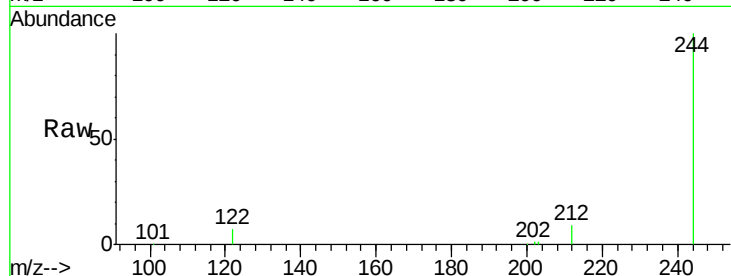

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

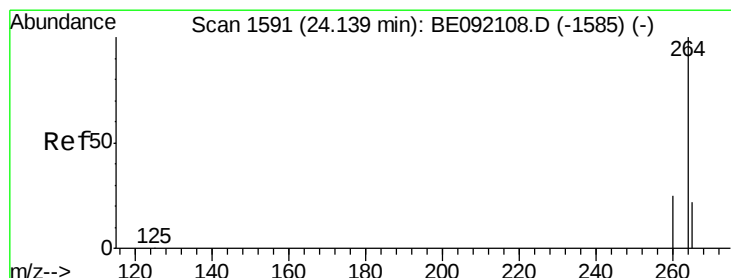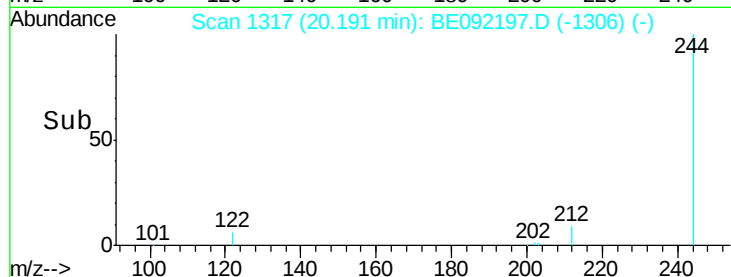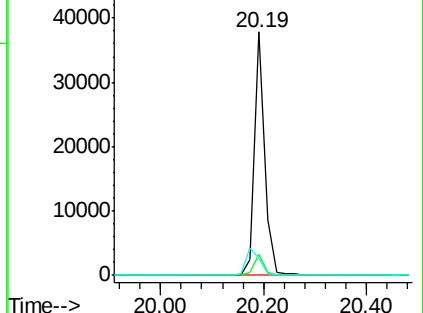

#28

Perylene-d12

Concen: 5.00 ng

RT: 24.14 min Scan# 1591

Delta R.T. 0.00 min

Lab File: BE092197.D

Acq: 5 Aug 2016 00:19


Tgt Ion:264 Resp: 90149

Ion Ratio Lower Upper

264 100

260 25.0 20.8 31.2

265 22.3 16.6 25.0

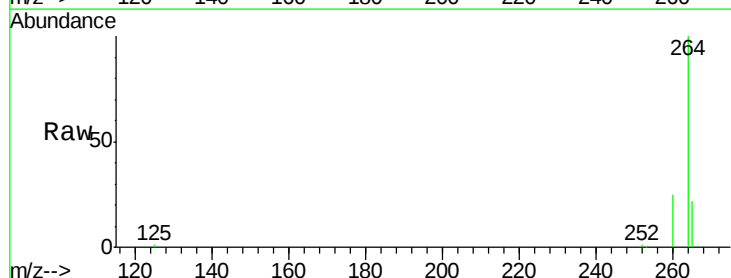

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

