

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080416\
 Data File : BE092203.D
 Acq On : 5 Aug 2016 4:33
 Operator : UM/SJ
 Sample : H4287-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 GW-59-9.6-19.0

Quant Time: Aug 05 06:37:37 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 16:59:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	11711	5.00	ng	0.00
6) Naphthalene-d8	10.98	136	53161	5.00	ng	-0.01
10) Acenaphthene-d10	14.83	164	28451	5.00	ng	-0.02
16) Phenanthrene-d10	17.56	188	66192	5.00	ng	-0.02
22) Chrysene-d12	21.75	240	76505	5.00	ng	0.00
28) Perylene-d12	24.14	264	80465	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.69	112	12997	4.32	ng	0.00
5) Phenol-d6	7.35	99	11123	2.78	ng	0.00
7) Nitrobenzene-d5	9.34	82	14382	3.43	ng	-0.01
11) 2,4,6-Tribromophenol	16.33	330	7466	8.08	ng	0.00
12) 2-Fluorobiphenyl	13.46	172	32740	3.63	ng	0.00
24) Terphenyl-d14	20.19	244	45575	4.15	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080416\
Data File : BE092203.D
Acq On : 5 Aug 2016 4:33
Operator : UM/SJ
Sample : H4287-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
GW-59-9.6-19.0

Quant Time: Aug 05 06:37:37 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-PAH-BE080216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 16:59:37 2016
Response via : Initial Calibration

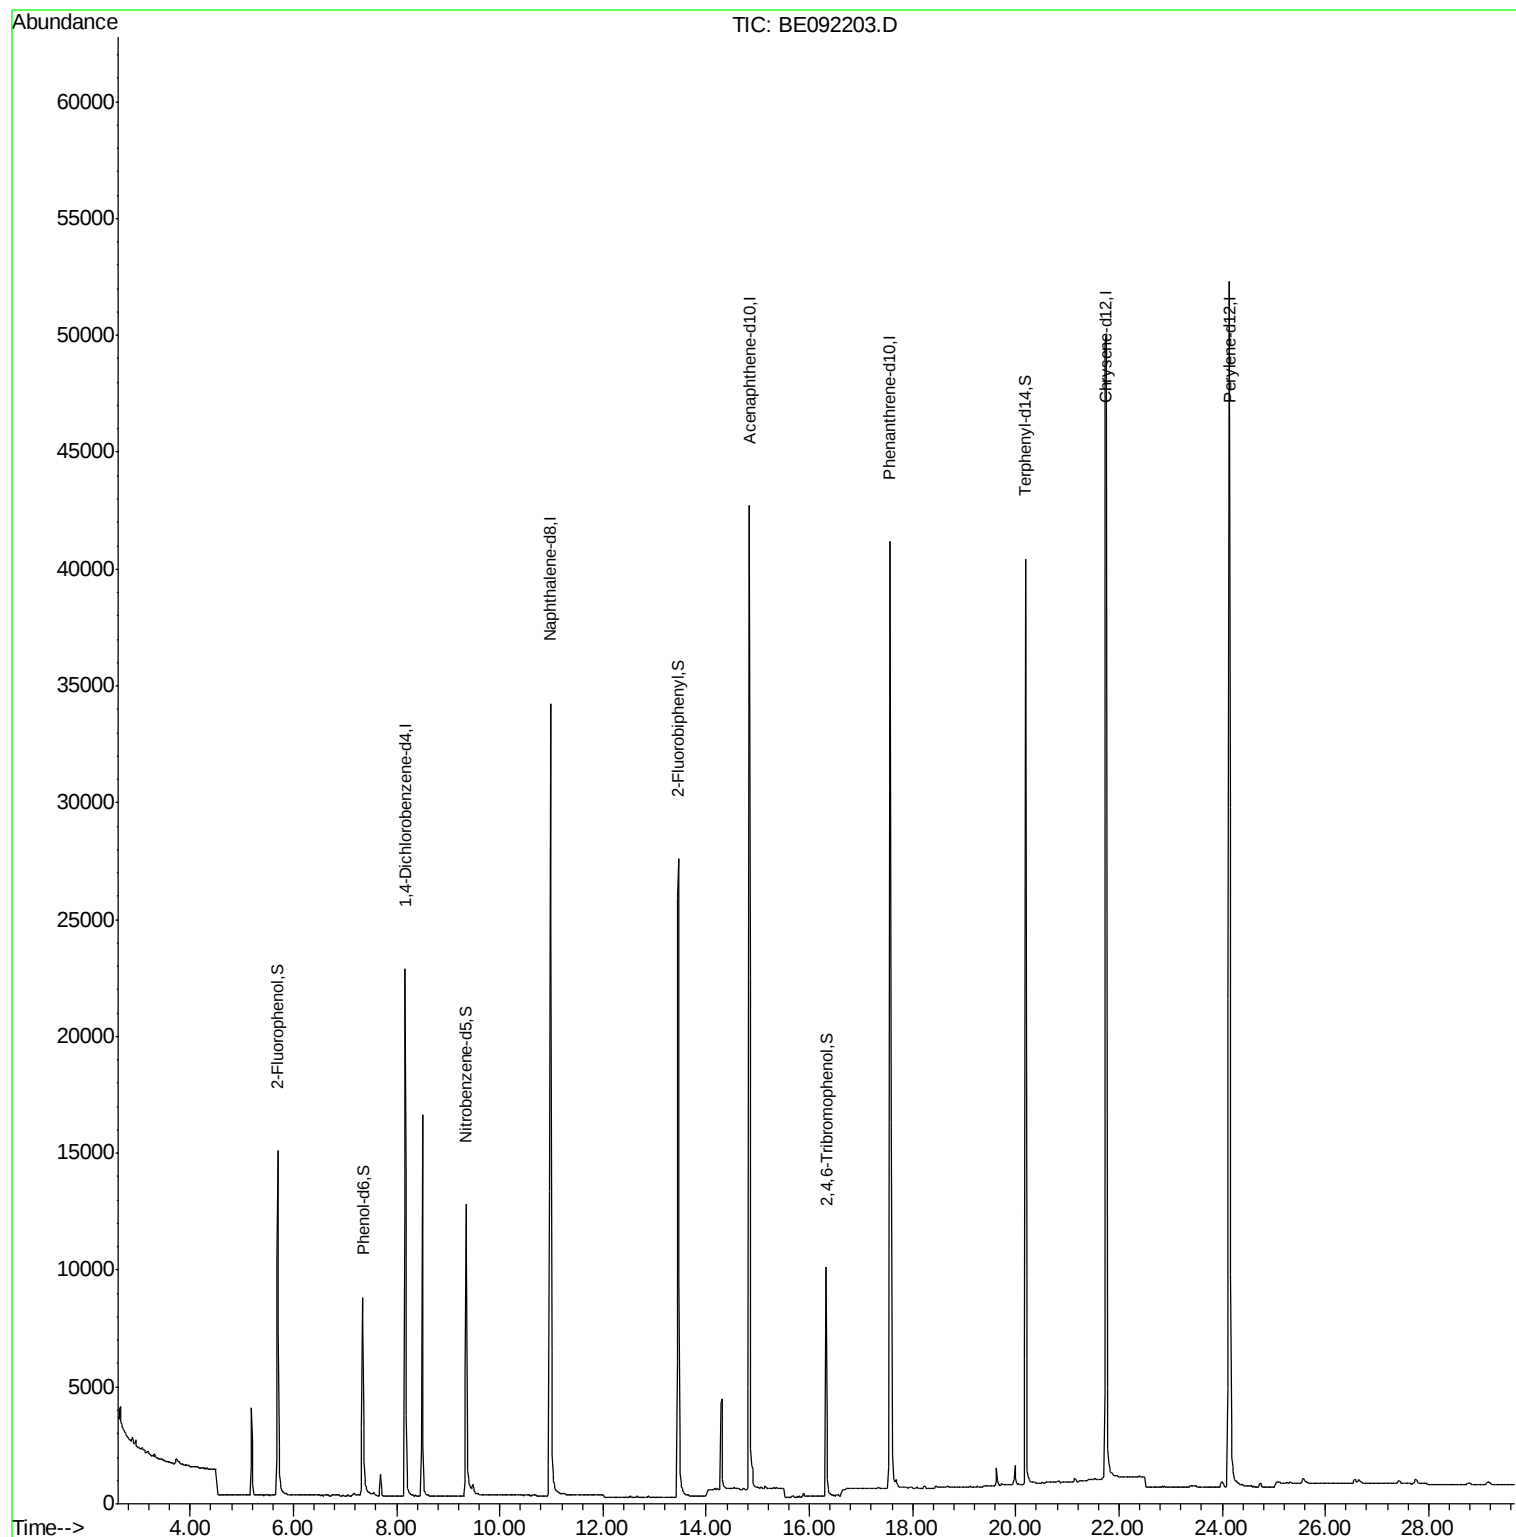

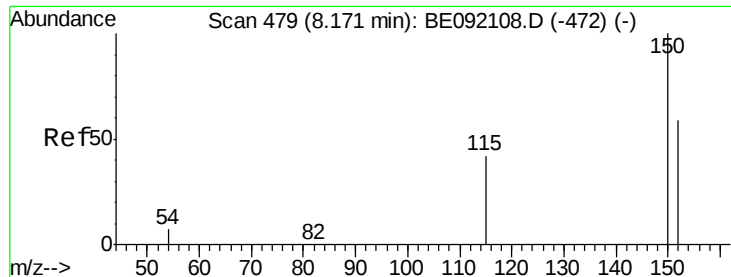

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.17 min Scan# 479

Delta R.T. -0.00 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33

Instrument :

BNA_E

ClientSampleId :

GW-59-9.6-19.0


Tot Ion:152 Resp: 11711

Ion Ratio Lower Upper

152 100

150 161.7 106.0 159.0#




115 63.1 36.9 55.3#

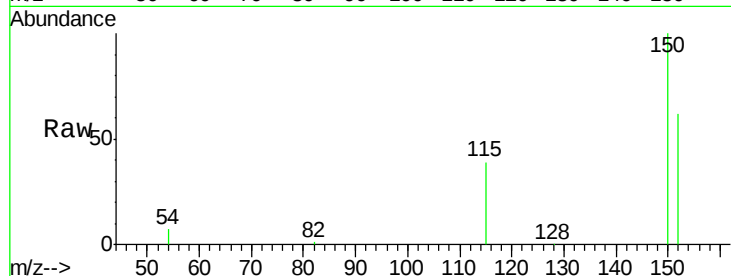

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

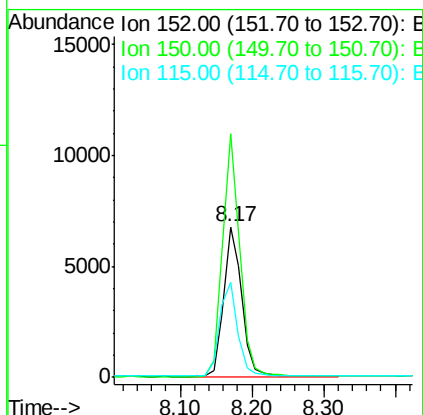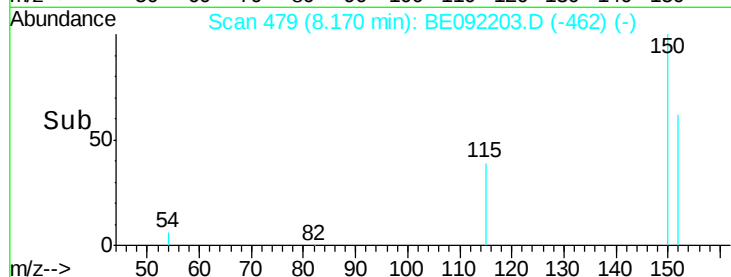

#4

2-Fluorophenol

Concen: 4.32 ng

RT: 5.69 min Scan# 267

Delta R.T. 0.00 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33


Tgt Ion:112 Resp: 12997

Ion Ratio Lower Upper

112 100

64 67.5 55.9 83.9



63 36.5 31.1 46.7




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

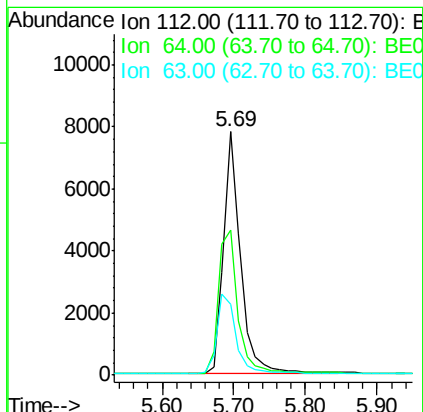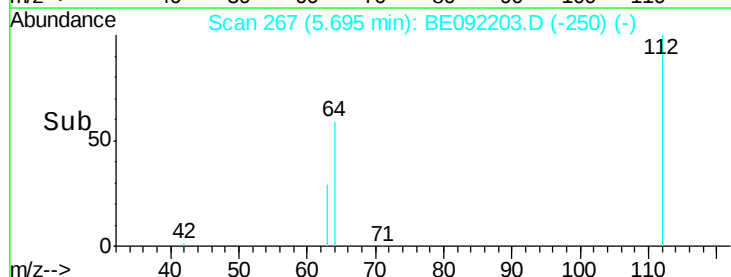

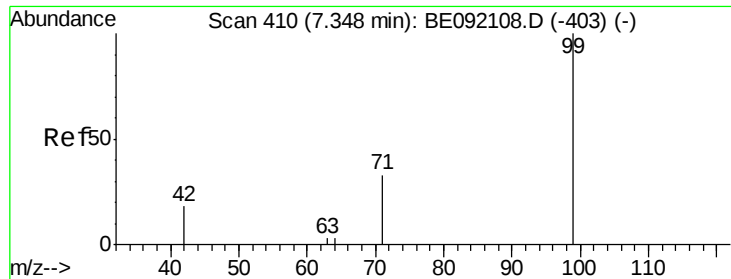

#5

Phenol-d6

Concen: 2.78 ng

RT: 7.35 min Scan# 410

Delta R.T. 0.00 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33

Instrument :

BNA_E

ClientSampleId :

GW-59-9.6-19.0


Tot Ion: 99 Resp: 11123

Ion Ratio Lower Upper

99 100

42 24.9 22.4 33.6




71 34.9 28.9 43.3



Abundance Ion 99.00 (98.70 to 99.70): BE092108.D (-403) (-)

Ion 42.00 (41.70 to 42.70): BE092108.D (-403) (-)

Ion 71.00 (70.70 to 71.70): BE092108.D (-403) (-)

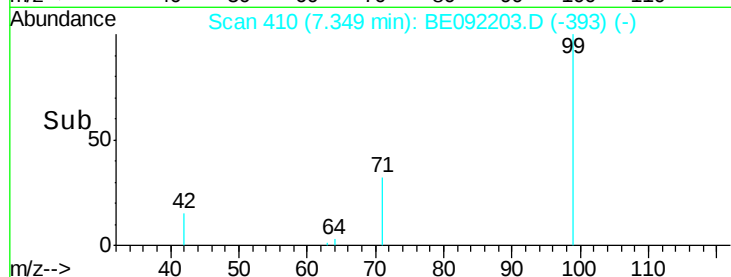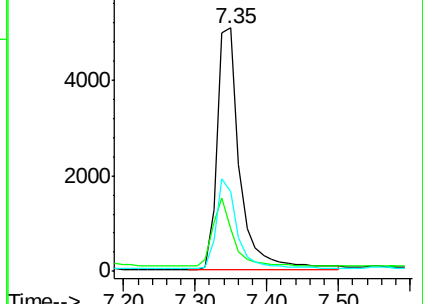

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.98 min Scan# 703

Delta R.T. -0.01 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33

Tgt Ion: 136 Resp: 53161


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 9.7 2.7 4.1#

68 6.7 2.2 3.4#






Abundance Ion 136.00 (135.70 to 136.70): BE092108.D (-698) (-)

Ion 137.00 (136.70 to 137.70): BE092108.D (-698) (-)

Ion 54.00 (53.70 to 54.70): BE092108.D (-698) (-)

Ion 68.00 (67.70 to 68.70): BE092108.D (-698) (-)

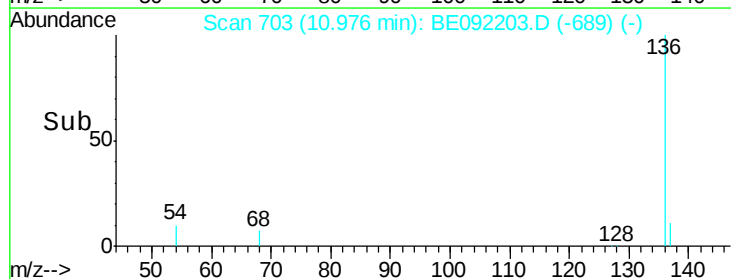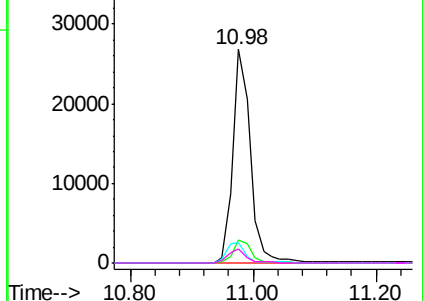

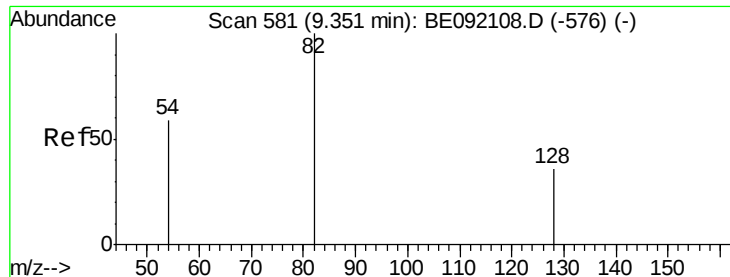

#7

Nitrobenzene-d5

Concen: 3.43 ng

RT: 9.34 min Scan# 580

Delta R.T. -0.01 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33

Instrument :

BNA_E

ClientSampleId :

GW-59-9.6-19.0


Tot Ion: 82 Resp: 14382

Ion Ratio Lower Upper

82 100

128 32.2 33.0 49.4#




54 63.1 42.6 63.8

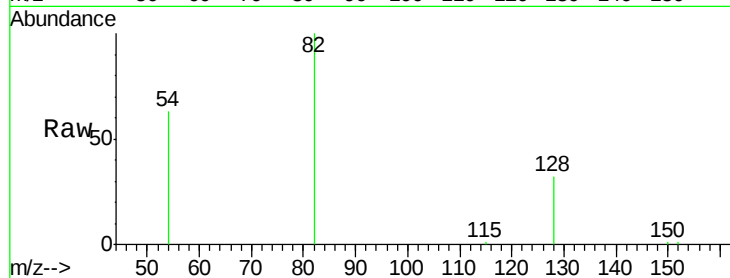

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

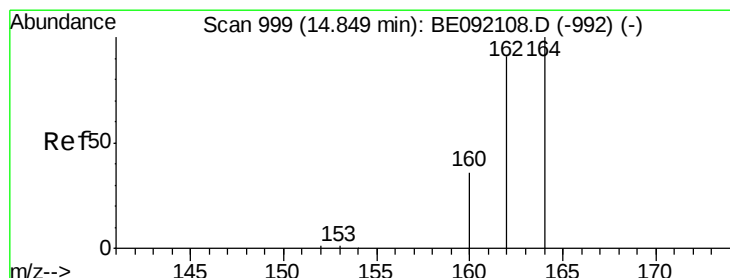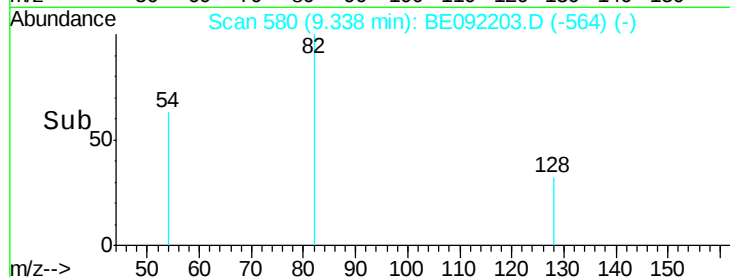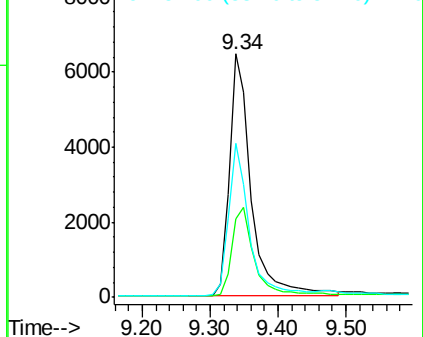

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.83 min Scan# 998

Delta R.T. -0.02 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33


Tgt Ion: 164 Resp: 28451

Ion Ratio Lower Upper

164 100

162 112.3 69.5 104.3#



160 54.3 27.6 41.4#

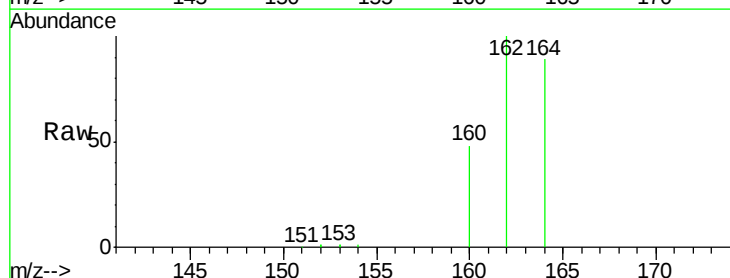


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



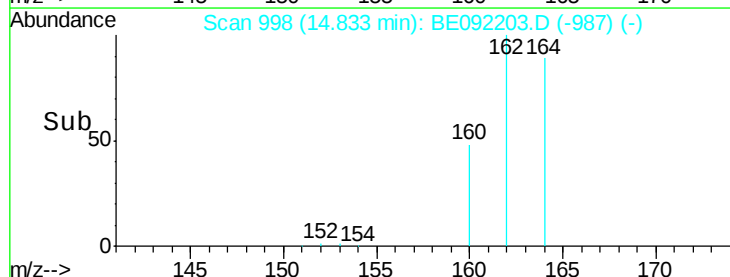
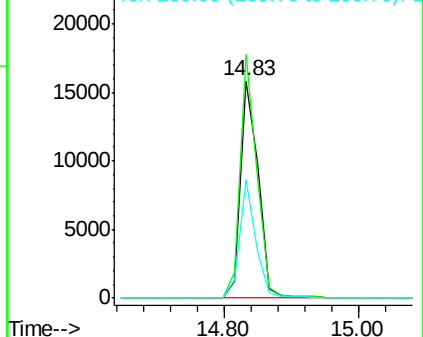


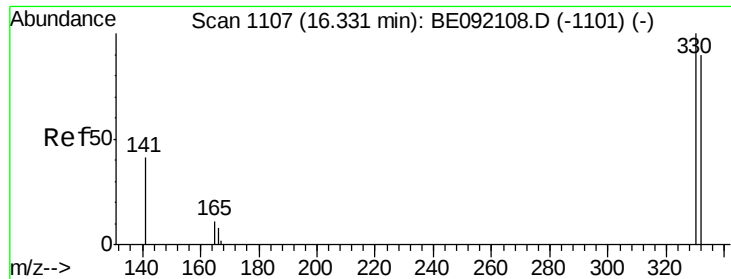

#11
 2,4,6-Tribromophenol
 Concen: 8.08 ng
 RT: 16.33 min Scan# 1107
 Delta R.T. 0.00 min
 Lab File: BE092203.D
 Acq: 5 Aug 2016 4:33




Instrument :
 BNA_E
 ClientSampleId :
 GW-59-9.6-19.0


Tot Ion:330 Resp: 7466
 Ion Ratio Lower Upper
 330 100
 332 96.5 74.2 111.4
 141 44.4 139.8 209.8#

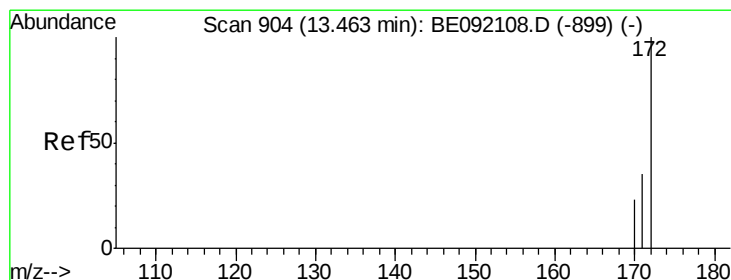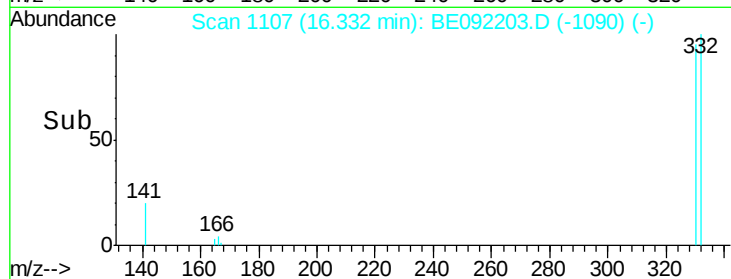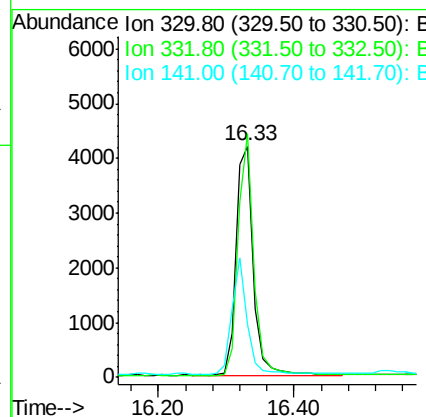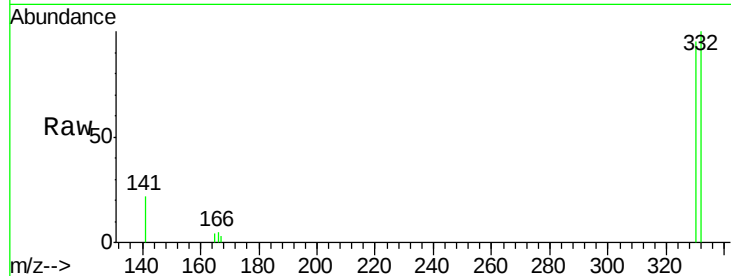

#12
 2-Fluorobiphenyl
 Concen: 3.63 ng
 RT: 13.46 min Scan# 904
 Delta R.T. -0.00 min
 Lab File: BE092203.D
 Acq: 5 Aug 2016 4:33

Tgt Ion:172 Resp: 32740
 Ion Ratio Lower Upper
 172 100
 171 31.2 30.3 45.5
 170 18.9 21.6 32.4#

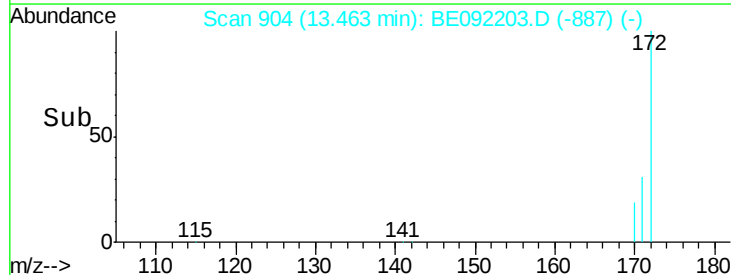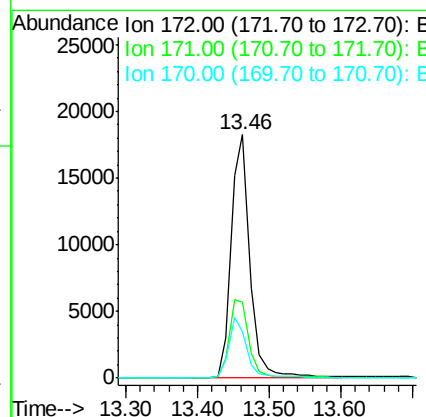


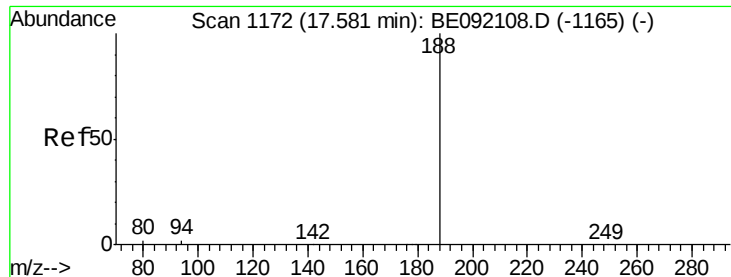




#16
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.56 min Scan# 1171
Delta R.T. -0.02 min
Lab File: BE092203.D
Acq: 5 Aug 2016 4:33

Instrument :
BNA_E
ClientSampleId :
GW-59-9.6-19.0

Tot Ion:188 Resp: 66192
Ion Ratio Lower Upper
188 100
94 14.0 3.9 5.9#
80 14.5 3.4 5.0#

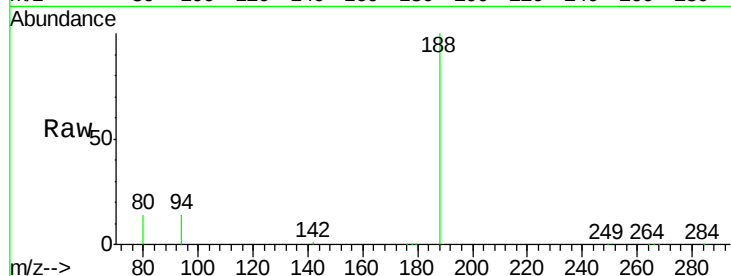


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

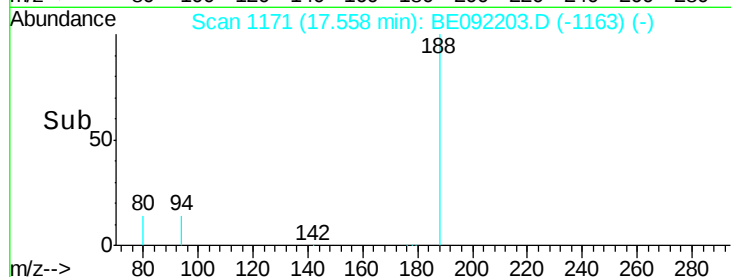
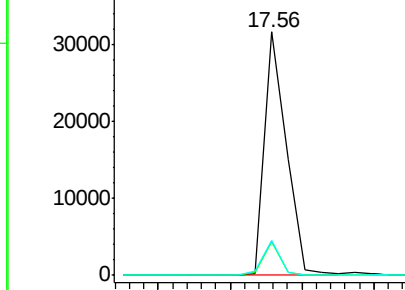



#22
Chrysene-d12
Concen: 5.00 ng
RT: 21.75 min Scan# 1407
Delta R.T. -0.00 min
Lab File: BE092203.D
Acq: 5 Aug 2016 4:33

Tgt Ion:240 Resp: 76505
Ion Ratio Lower Upper
240 100
120 1.4 0.6 1.0#
236 22.2 18.2 27.4



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

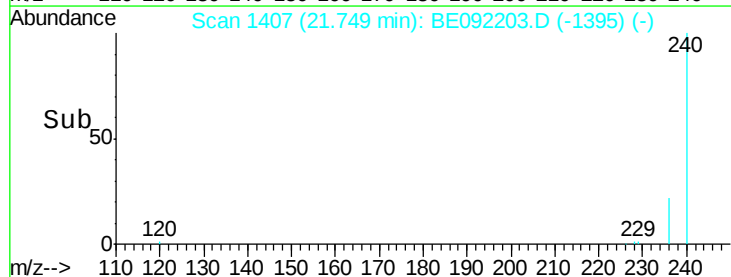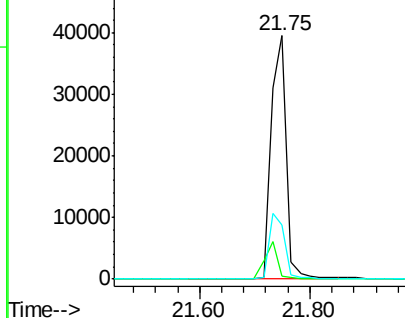

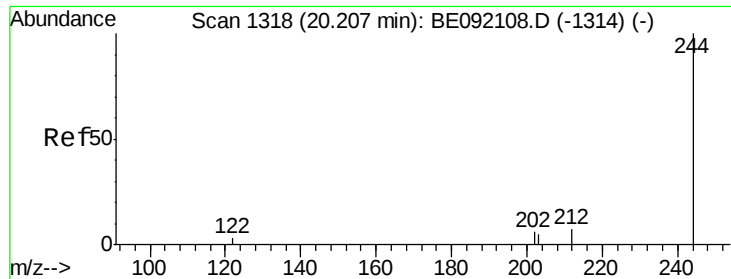

#24

Terphenyl-d14

Concen: 4.15 ng

RT: 20.19 min Scan# 1317

Delta R.T. -0.02 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33

Instrument :

BNA_E

ClientSampleId :

GW-59-9.6-19.0


Tot Ion:244 Resp: 45575

Ion Ratio Lower Upper




244 100

212 9.0 9.1 13.7#

122 6.7 11.0 16.4#

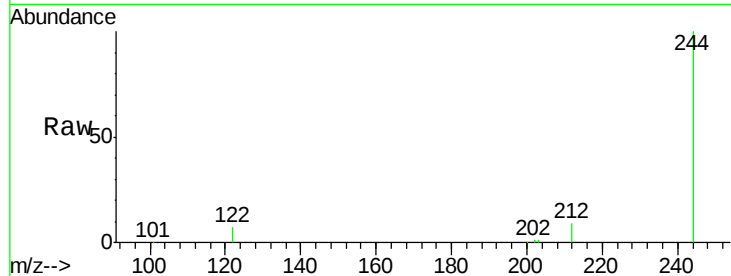

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

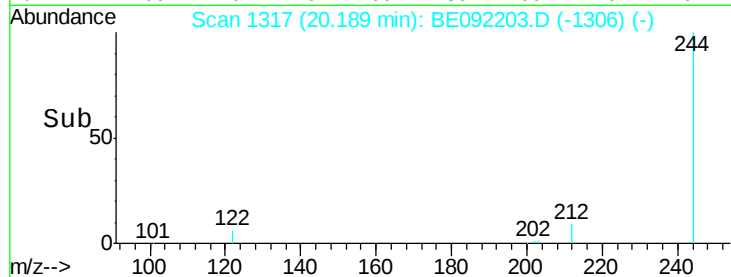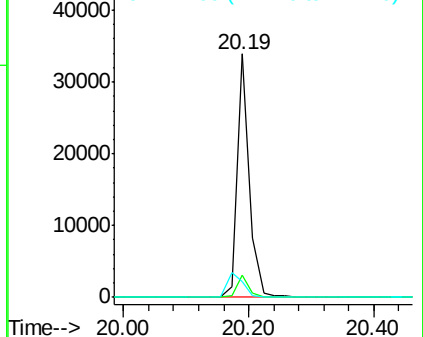

#28

Perylene-d12

Concen: 5.00 ng

RT: 24.14 min Scan# 1591

Delta R.T. 0.00 min

Lab File: BE092203.D

Acq: 5 Aug 2016 4:33


Tgt Ion:264 Resp: 80465

Ion Ratio Lower Upper

264 100

260 24.7 20.8 31.2

265 22.7 16.6 25.0



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

